

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060425AL\
Data File : FE054182.D
Signal(s) : FID1B.ch
Acq On : 04 Jun 2025 21:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 05 06:29:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051425.M
Quant Title : GC Extractables
QLast Update : Wed May 14 12:15:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.005	23930	0.192 ug/ml
18) T	n-Dotriacontane (C32)	18.838	37564	0.300 ug/ml
20) T	n-Hexatriacontane (C36)	20.368	14684	0.127 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060425AL\
Data File : FE054182.D
Signal(s) : FID1B.ch
Acq On : 04 Jun 2025 21:55
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 05 06:29:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051425.M
Quant Title : GC Extractables
QLast Update : Wed May 14 12:15:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

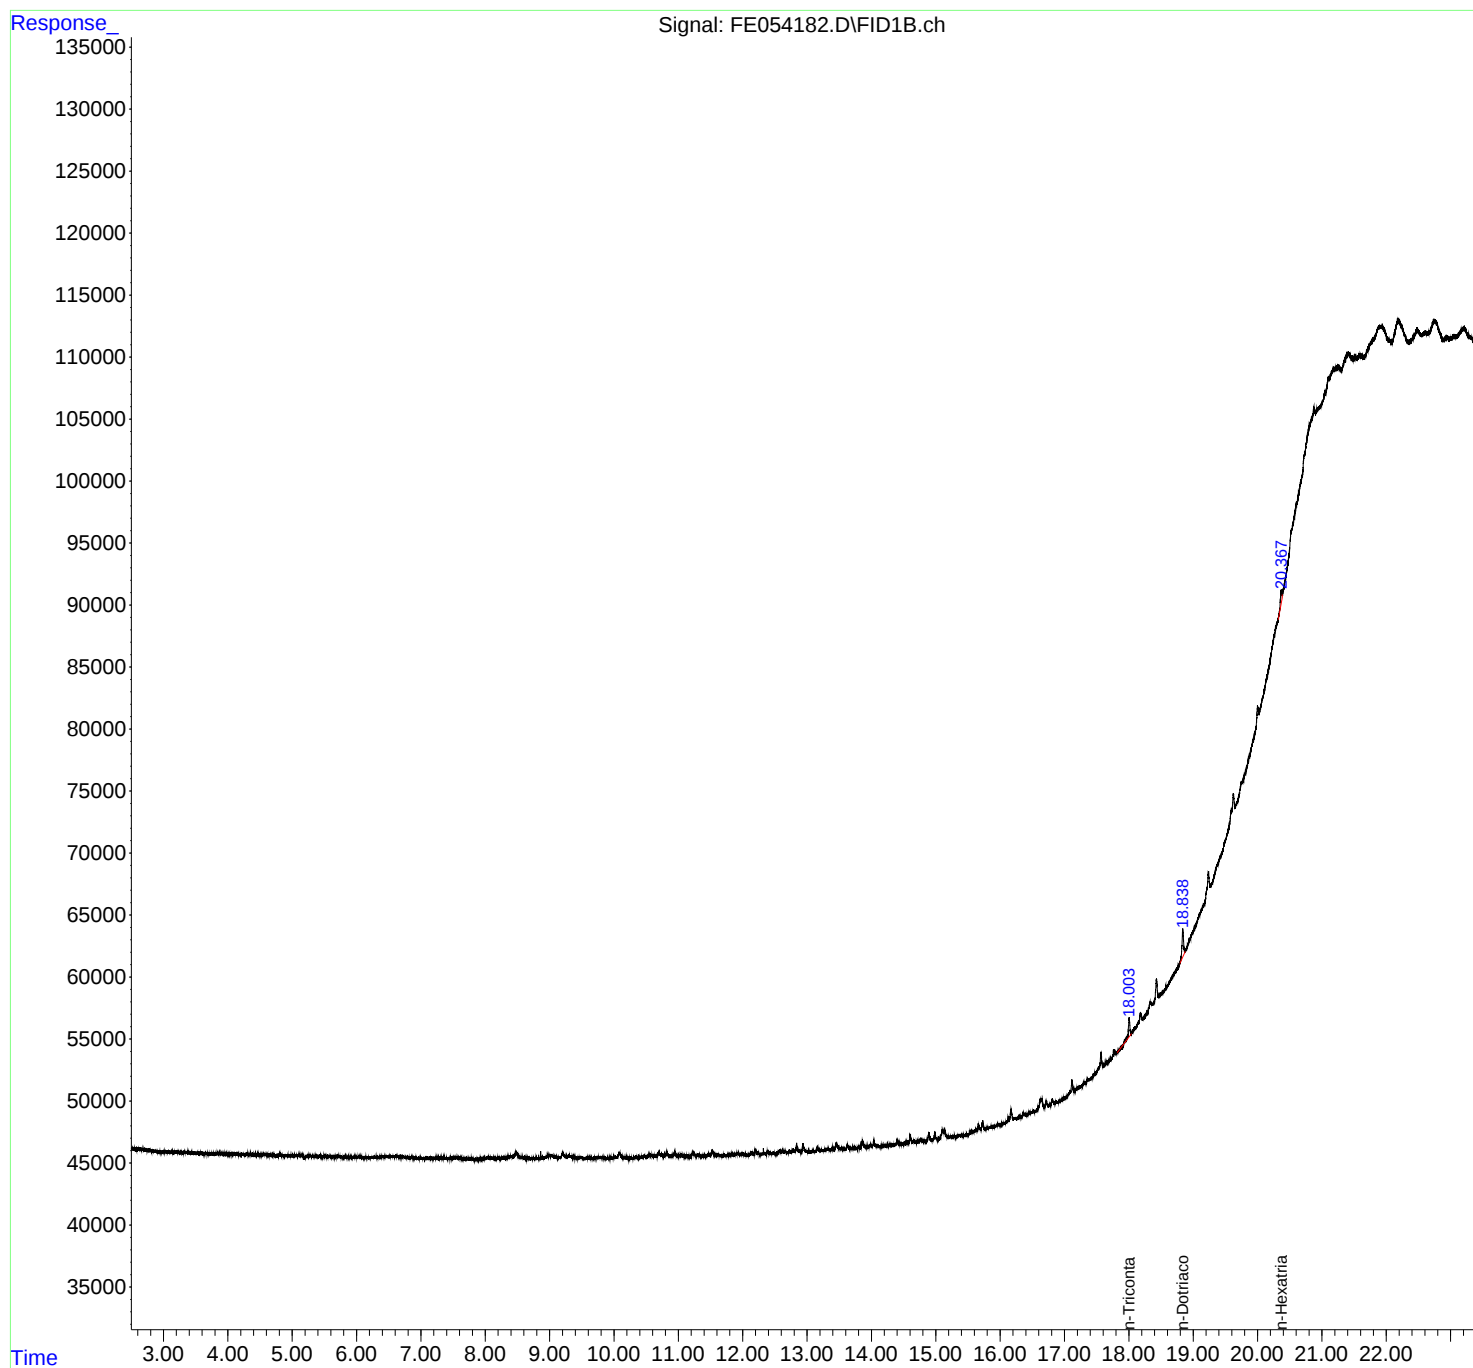


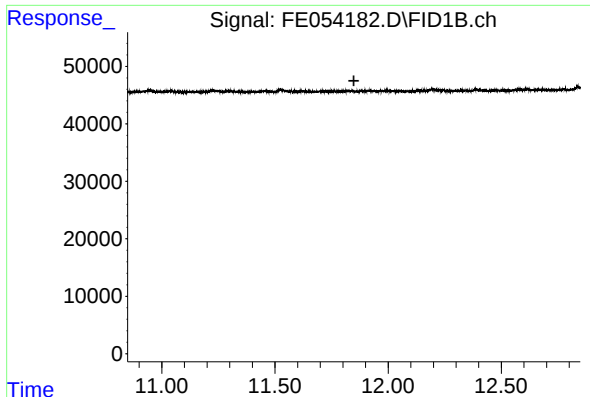

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.849 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

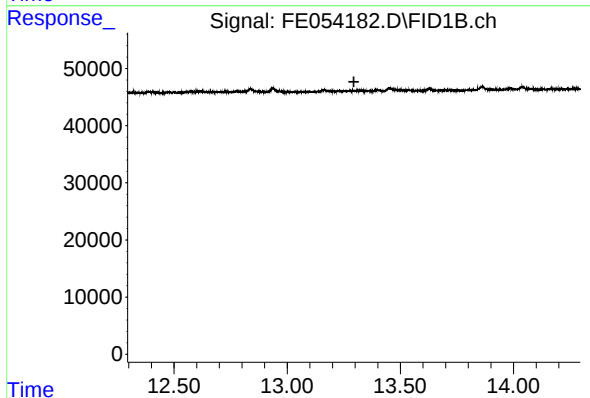


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.295 min
Response: 0
Conc: N.D.

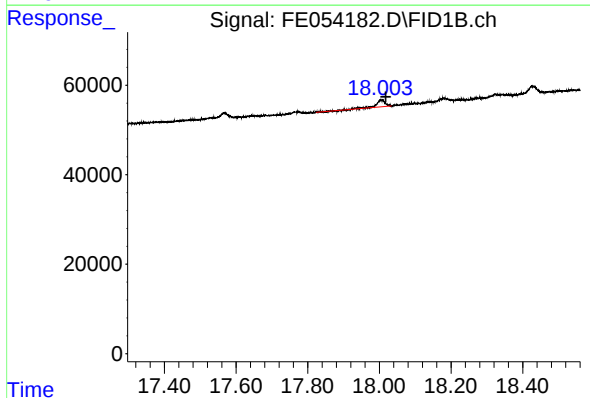


#17 n-Tricontane (C30)

R.T.: 18.005 min
Delta R.T.: -0.013 min
Response: 23930
Conc: 0.19 ug/ml

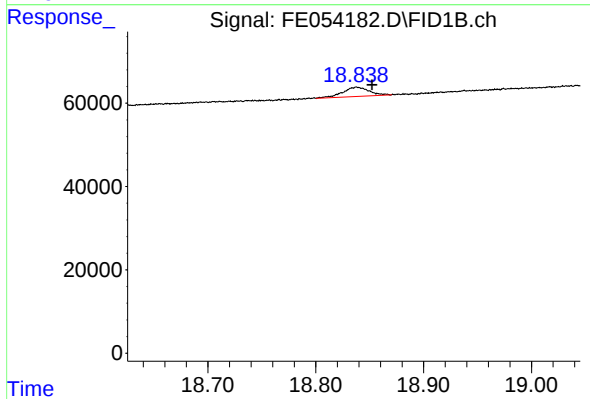

#18 n-Dotriacontane (C32)

R.T.: 18.838 min
Delta R.T.: -0.014 min
Response: 37564
Conc: 0.30 ug/ml

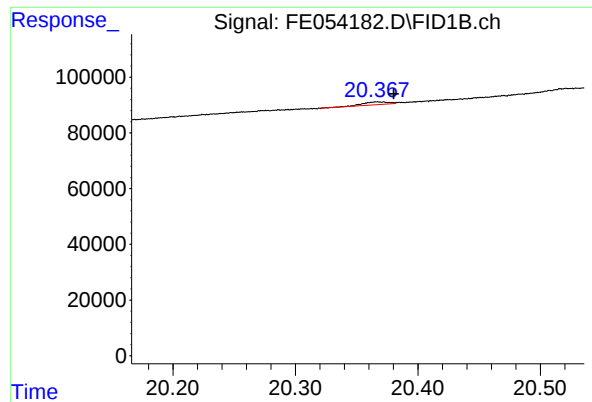

#20 n-Hexatriacontane (C36)

R.T.: 20.368 min
Delta R.T.: -0.013 min
Response: 14684
Conc: 0.13 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK