

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE060523AL\  
 Data File : FE042402.D  
 Signal(s) : FID1B.ch  
 Acq On : 06 Jun 2023 01:09  
 Operator : YP\AJ  
 Sample : 03032-04  
 Misc :  
 ALS Vial : 37 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 TP-21-0A

Integration File: autoint1.e  
 Quant Time: Jun 06 03:35:12 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 051823.M  
 Quant Title : GC Extractables  
 QLast Update : Thu May 18 06:27:12 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.957 | 4475658    | 25.347 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 50.69%       |
| 12) S 1-chlorooctadecane (S... | 13.393 | 3288216    | 24.746 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 49.49%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE060523AL\  
Data File : FE042402.D  
Signal(s) : FID1B.ch  
Acq On : 06 Jun 2023 01:09  
Operator : YP\AJ  
Sample : 03032-04  
Misc :  
ALS Vial : 37 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
TP-21-0A

Integration File: autoint1.e  
Quant Time: Jun 06 03:35:12 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 051823.M  
Quant Title : GC Extractables  
QLast Update : Thu May 18 06:27:12 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

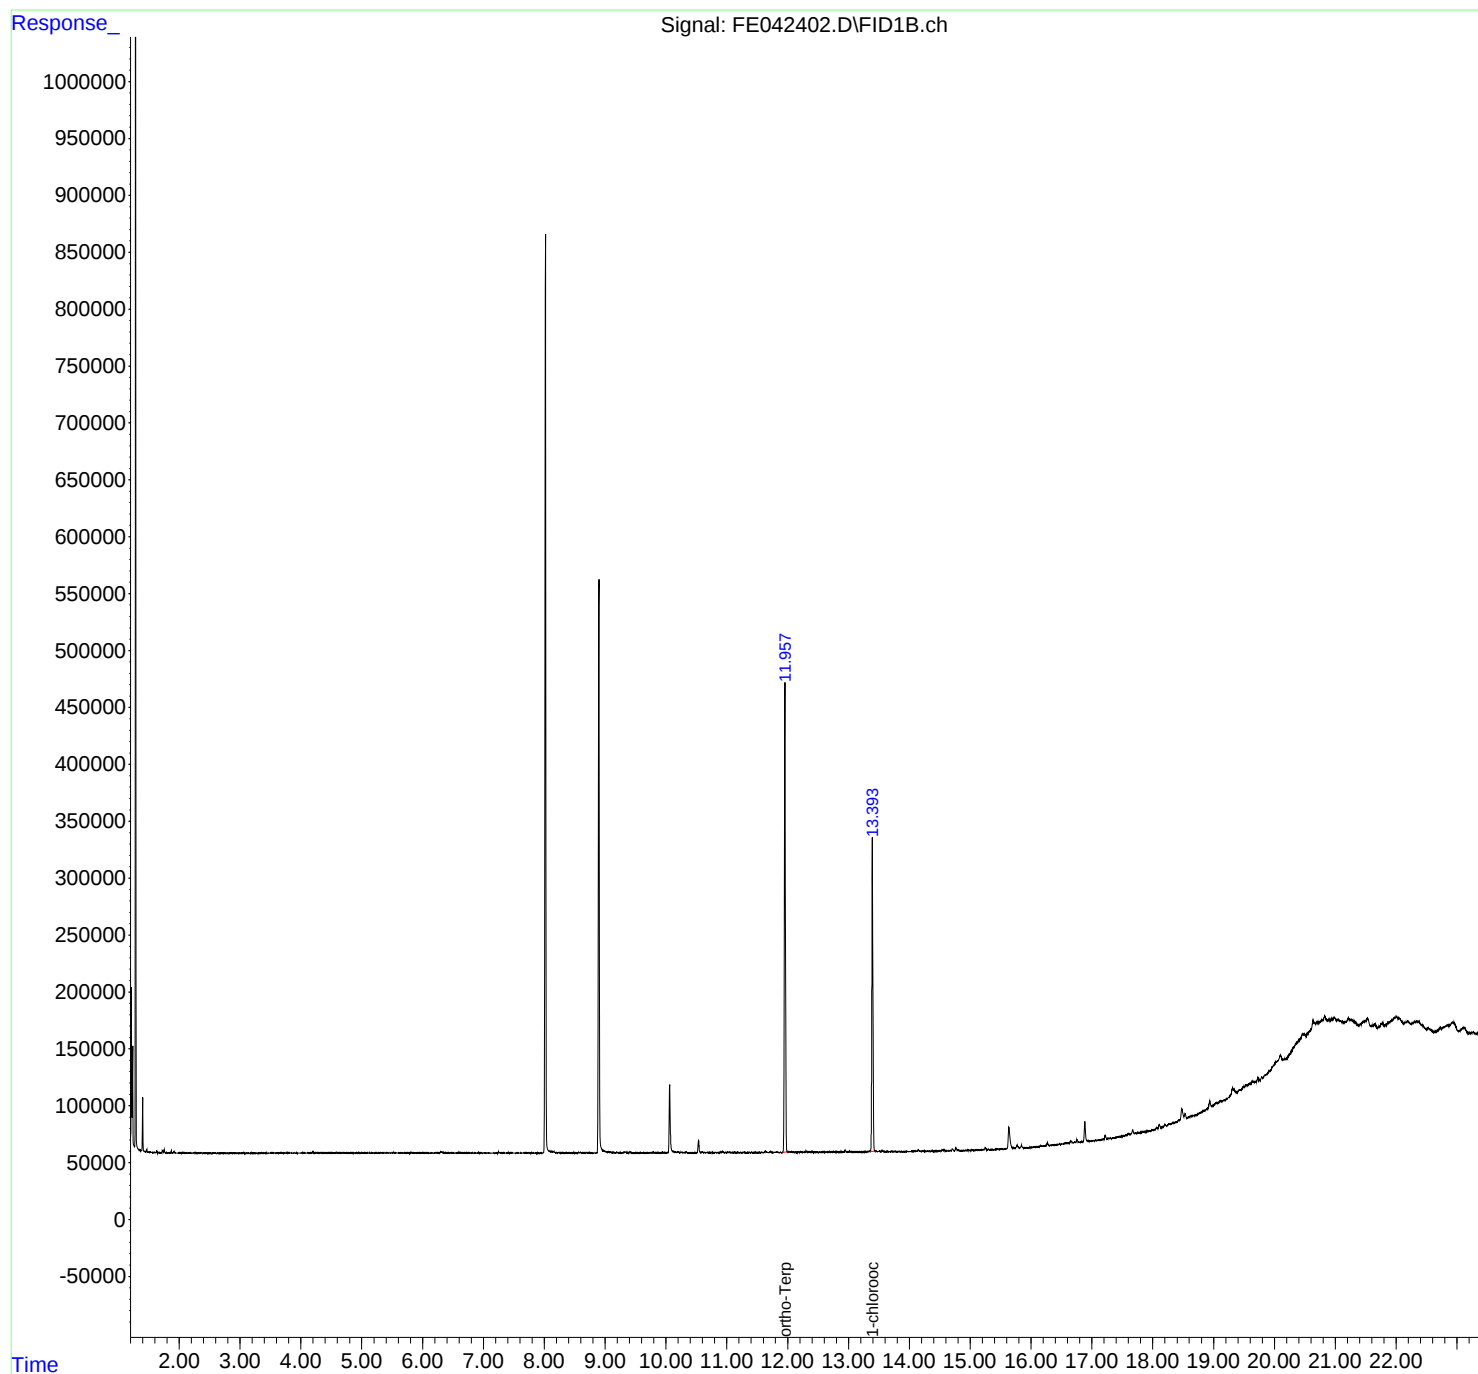


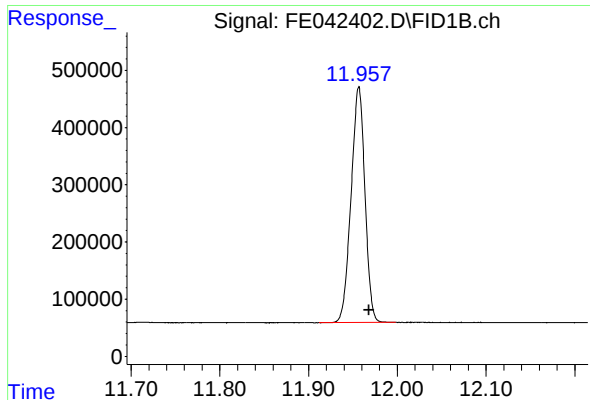

#9 ortho-Terphenyl (SURR)

R.T.: 11.957 min  
Delta R.T.: -0.011 min  
Response: 4475658  
Conc: 25.35 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
TP-21-0A

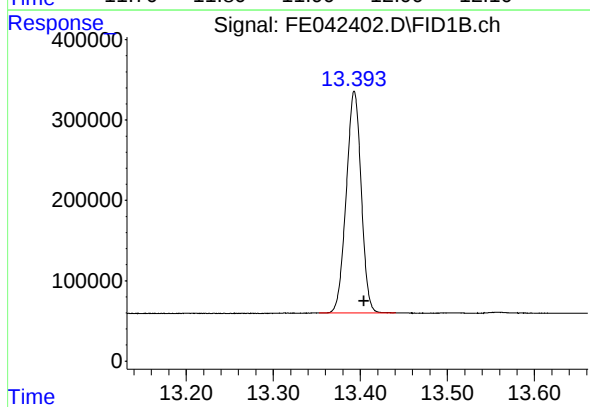

#12 1-chlorooctadecane (SURR)

R.T.: 13.393 min  
Delta R.T.: -0.011 min  
Response: 3288216  
Conc: 24.75 ug/ml