

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060525AL\
Data File : FE054192.D
Signal(s) : FID1B.ch
Acq On : 05 Jun 2025 15:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 06 01:15:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051425.M
Quant Title : GC Extractables
QLast Update : Wed May 14 12:15:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
17) T	n-Tricontane (C30)	18.007	28449	0.228 ug/ml
18) T	n-Dotriacontane (C32)	18.840	29828	0.239 ug/ml
20) T	n-Hexatriacontane (C36)	20.366	17264	0.149 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060525AL\
Data File : FE054192.D
Signal(s) : FID1B.ch
Acq On : 05 Jun 2025 15:12
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 06 01:15:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051425.M
Quant Title : GC Extractables
QLast Update : Wed May 14 12:15:41 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

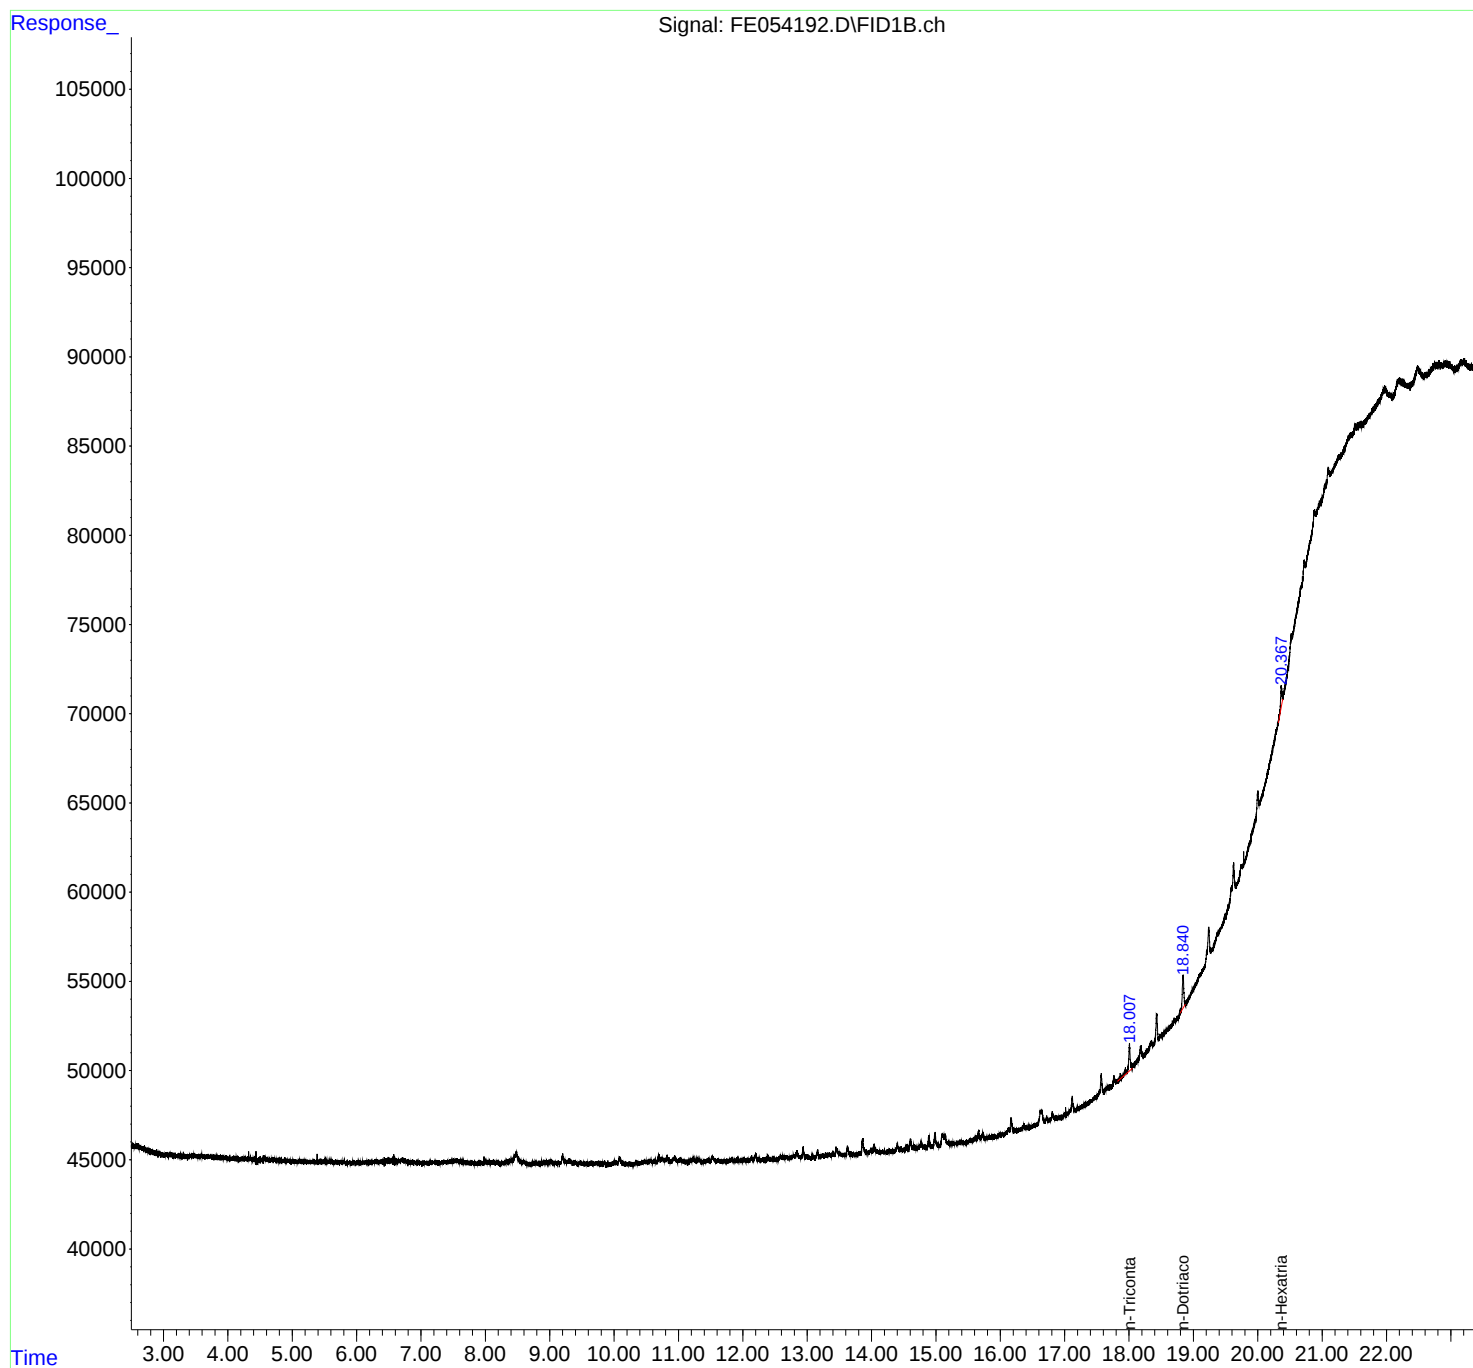


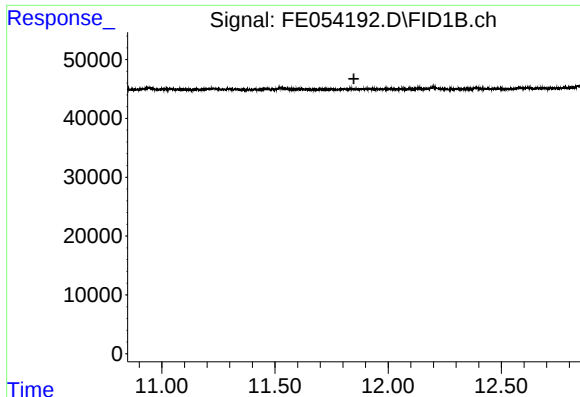

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.849 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
I.BLK

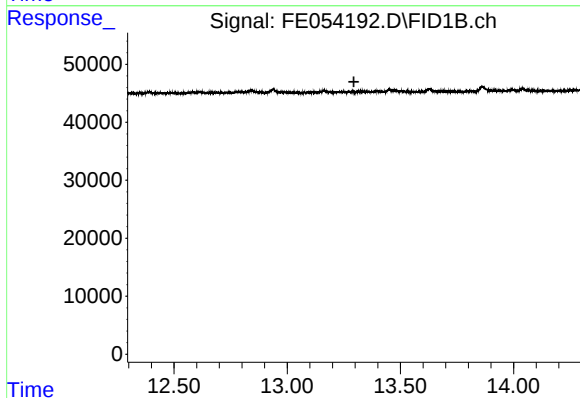


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.295 min
Response: 0
Conc: N.D.

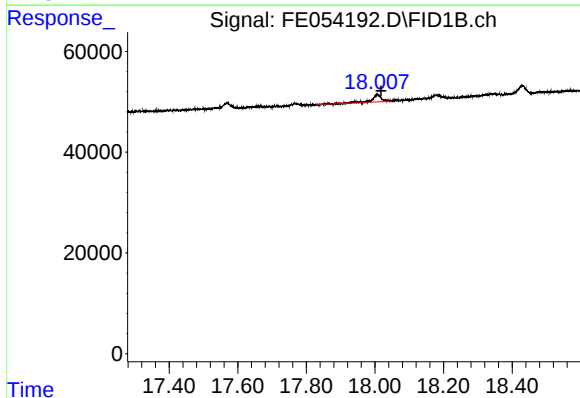


#17 n-Tricontane (C30)

R.T.: 18.007 min
Delta R.T.: -0.011 min
Response: 28449
Conc: 0.23 ug/ml

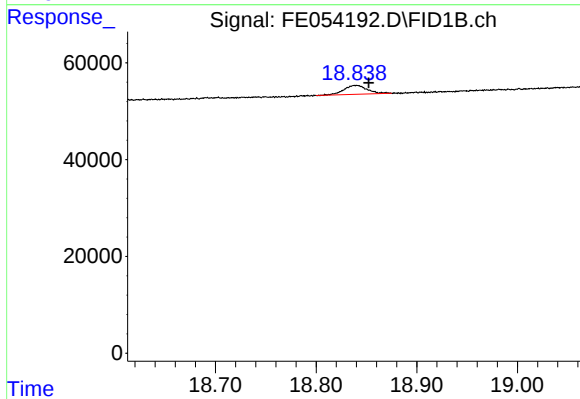

#18 n-Dotriacontane (C32)

R.T.: 18.840 min
Delta R.T.: -0.012 min
Response: 29828
Conc: 0.24 ug/ml

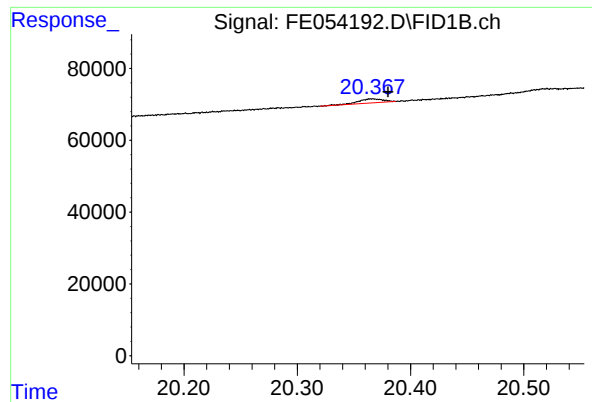

#20 n-Hexatriacontane (C36)

R.T.: 20.366 min
Delta R.T.: -0.014 min
Response: 17264
Conc: 0.15 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK