

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060621\
 Data File : FE033925.D
 Signal(s) : FID1B.CH
 Acq On : 06 Jun 2021 21:04
 Operator : DD\AJ
 Sample : PB136864BSD
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 PB136864BSD

Integration File: autoint1.e
 Quant Time: Jun 07 05:47:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
 Quant Title :
 QLast Update : Mon Jun 07 02:30:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.712	6157894	16.090 ug/ml
Target Compounds			
2) N-DECANE	4.453	6833327	16.754 ug/ml
3) N-DODECANE	6.465	7129103	17.249 ug/ml
4) N-TETRADECANE	8.259	7262787	17.057 ug/ml
5) N-HEXADECANE	9.861	7241599	17.051 ug/ml
6) N-OCTADECANE	11.303	7309735	16.759 ug/ml
7) N-EICOSANE	12.614	7400627	17.034 ug/ml
8) N-DOCOSANE	13.813	7320554	16.772 ug/ml
10) N-TETRACOSANE	14.918	7154455	16.339 ug/ml
11) N-HEXACOSANE	15.940	6952854	16.008 ug/ml
12) N-OCTACOSANE	16.888	6781014	15.584 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060621\
Data File : FE033925.D
Signal(s) : FID1B.CH
Acq On : 06 Jun 2021 21:04
Operator : DD\AJ
Sample : PB136864BSD
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
PB136864BSD

Integration File: autoint1.e
Quant Time: Jun 07 05:47:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
Quant Title :
QLast Update : Mon Jun 07 02:30:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

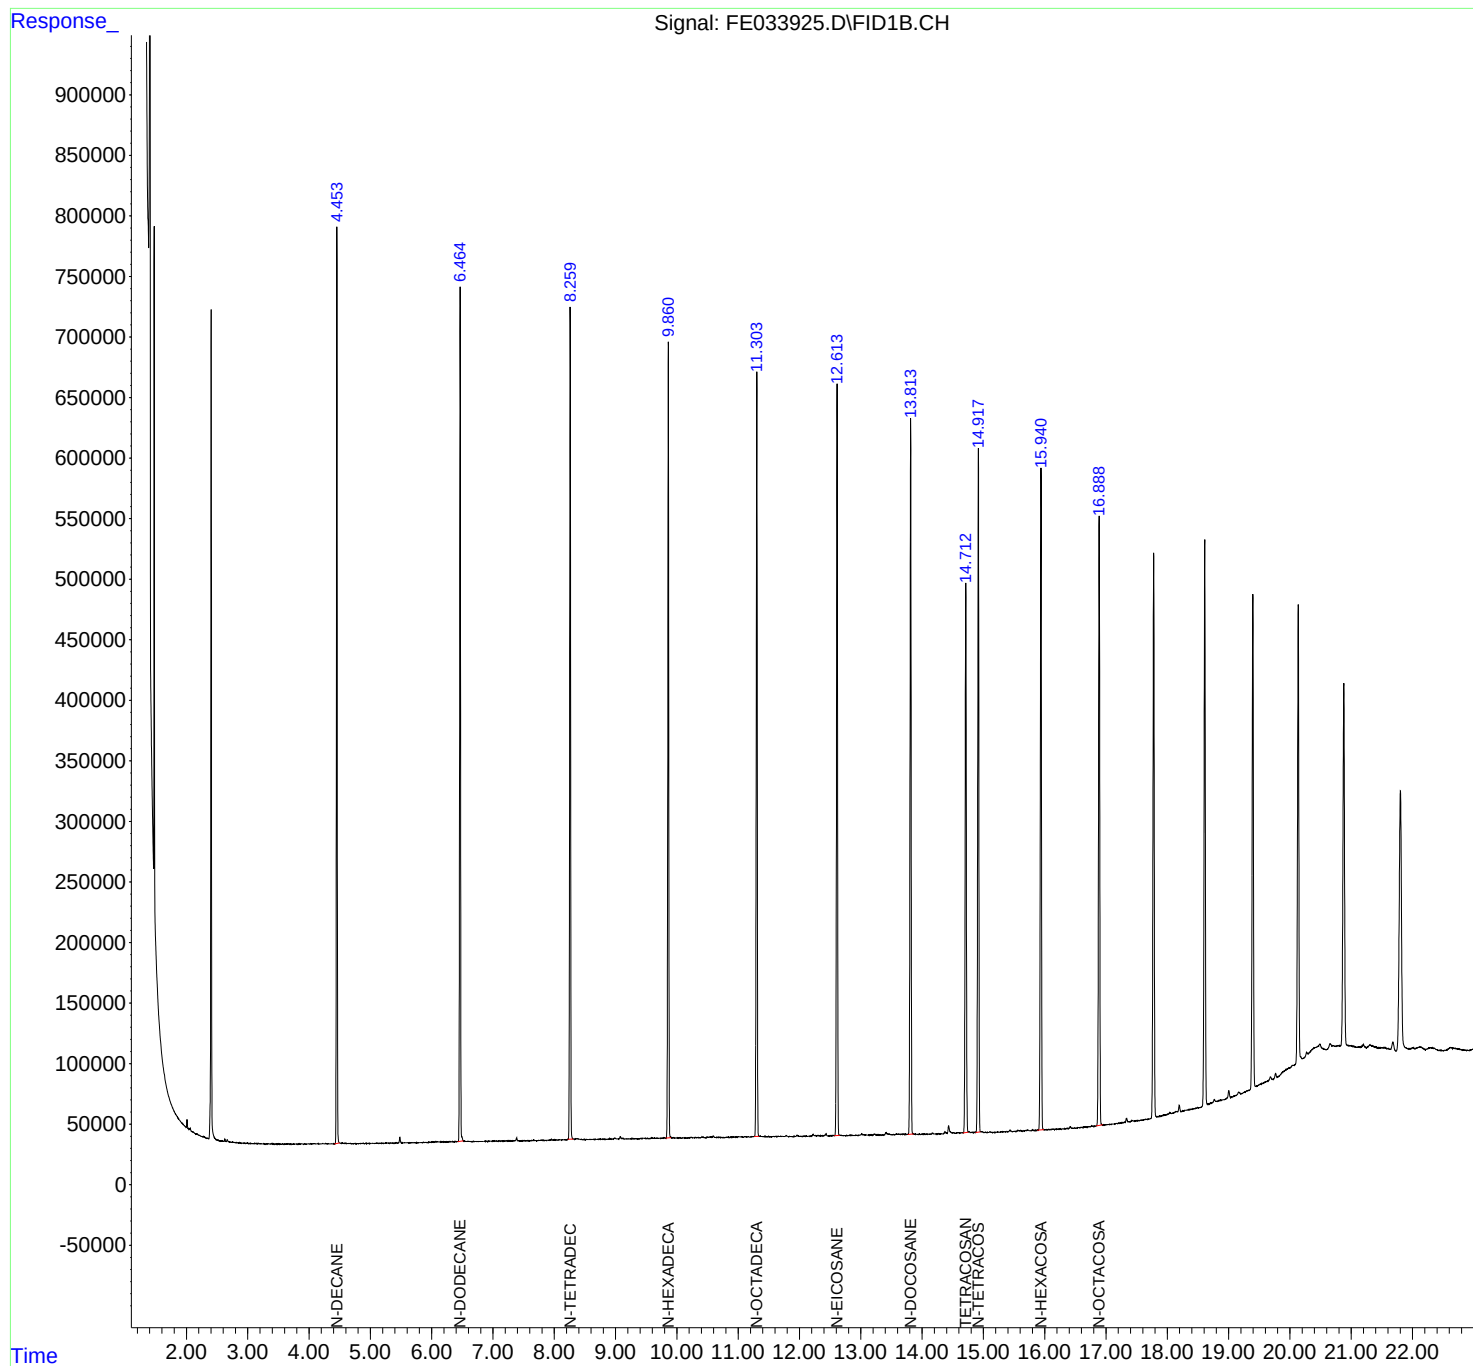


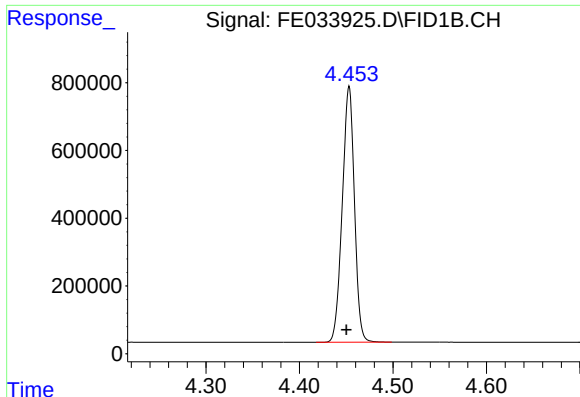

#2 N-DECANE


R.T.: 4.453 min
Delta R.T.: 0.003 min
Response: 6833327
Conc: 16.75 ug/ml

Instrument :
FID_E
ClientSampleId :
PB136864BSD

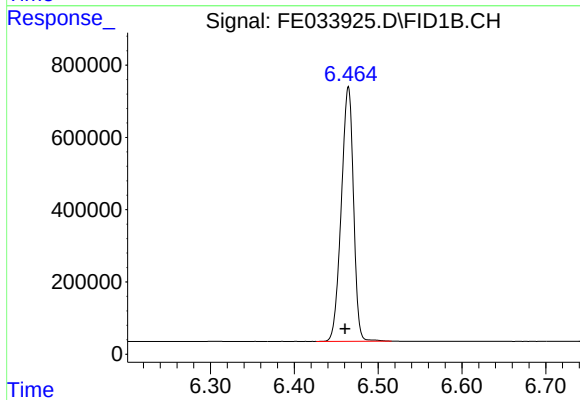


#3 N-DODECANE

R.T.: 6.465 min
Delta R.T.: 0.004 min
Response: 7129103
Conc: 17.25 ug/ml

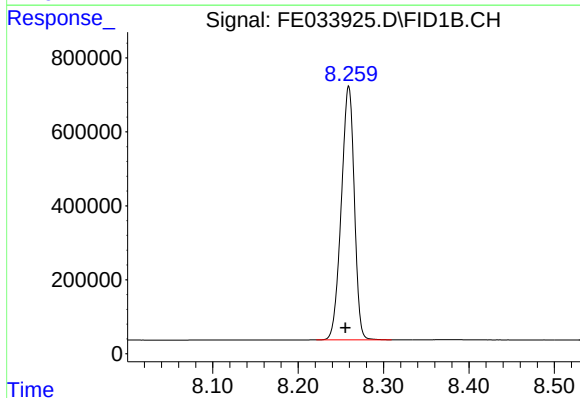


#4 N-TETRADECANE

R.T.: 8.259 min
Delta R.T.: 0.004 min
Response: 7262787
Conc: 17.06 ug/ml

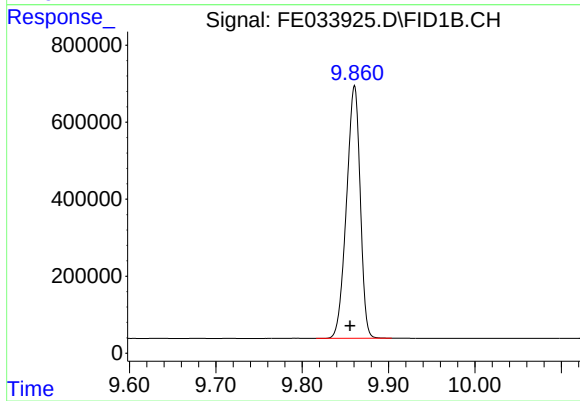

#5 N-HEXADECANE


R.T.: 9.861 min
Delta R.T.: 0.005 min
Response: 7241599
Conc: 17.05 ug/ml

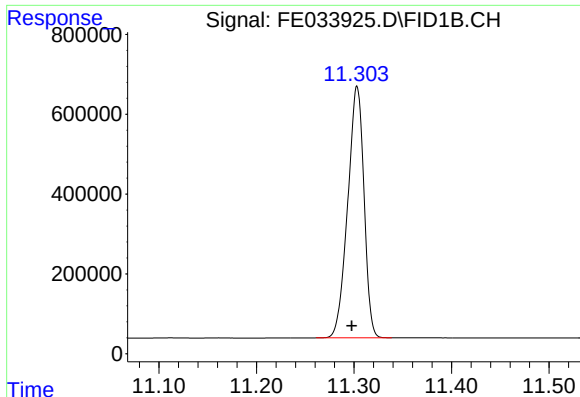

#6 N-OCTADECANE


R.T.: 11.303 min
Delta R.T.: 0.005 min
Response: 7309735
Conc: 16.76 ug/ml

Instrument :
FID_E
ClientSampleId :
PB136864BSD

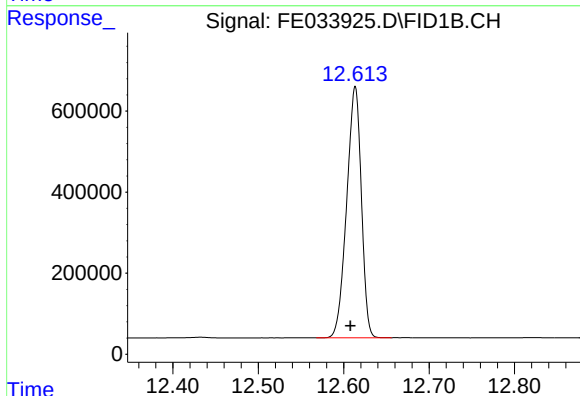


#7 N-EICOSANE

R.T.: 12.614 min
Delta R.T.: 0.006 min
Response: 7400627
Conc: 17.03 ug/ml

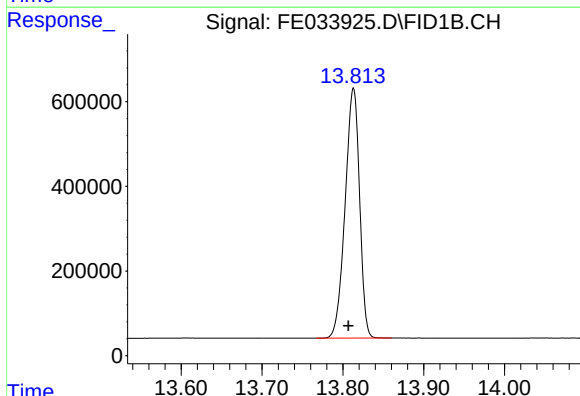


#8 N-DOCOSANE

R.T.: 13.813 min
Delta R.T.: 0.006 min
Response: 7320554
Conc: 16.77 ug/ml

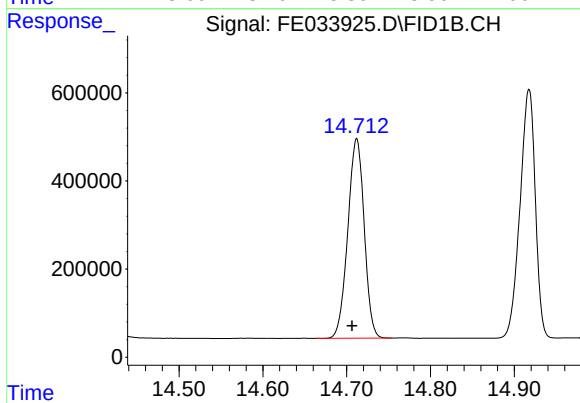

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.712 min
Delta R.T.: 0.006 min
Response: 6157894
Conc: 16.09 ug/ml

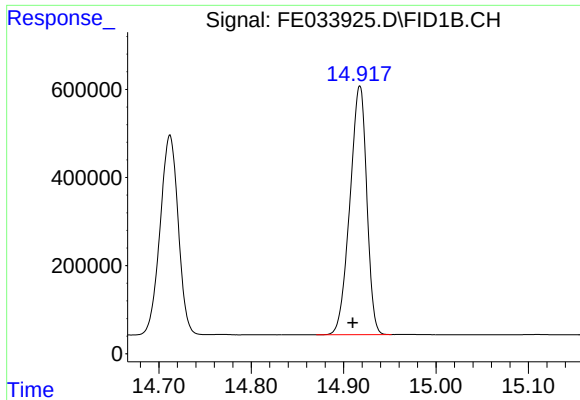

#10 N-TETRACOSANE


R.T.: 14.918 min
Delta R.T.: 0.008 min
Response: 7154455
Conc: 16.34 ug/ml

Instrument :
FID_E
ClientSampleId :
PB136864BSD

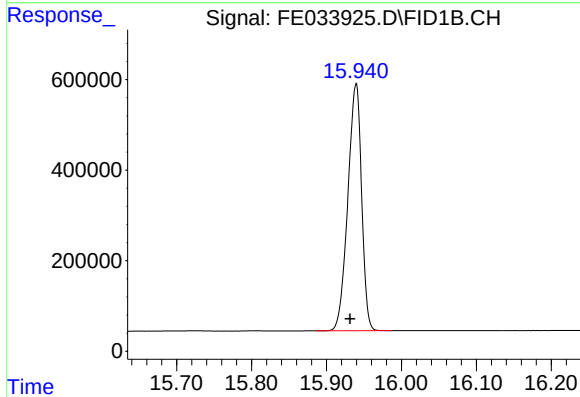

#11 N-HEXACOSANE

R.T.: 15.940 min
Delta R.T.: 0.008 min
Response: 6952854
Conc: 16.01 ug/ml

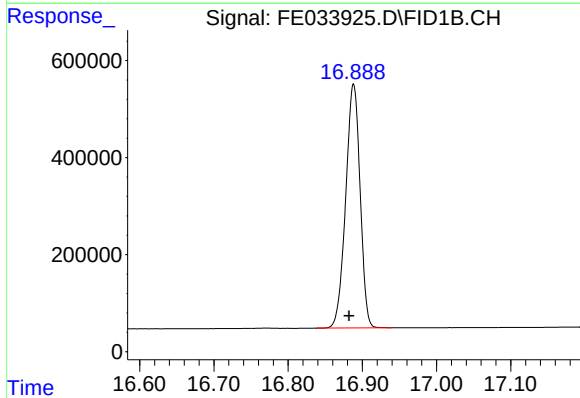

#12 N-OCTACOSANE

R.T.: 16.888 min
Delta R.T.: 0.006 min
Response: 6781014
Conc: 15.58 ug/ml