

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060622AL\
 Data File : FE035917.D
 Signal(s) : FID1B.CH
 Acq On : 06 Jun 2022 17:21
 Operator : YP\AJ
 Sample : N3168-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 HELENS-0602

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File: sample.E
 Quant Time: Jun 07 01:24:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 03:24:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.954	5984764	45.117 ug/ml
Spiked Amount 50.000		Recovery =	90.23%
12) S 1-chlorooctadecane (S...	12.385	4600239	43.977 ug/mlm
Spiked Amount 50.000		Recovery =	87.95%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060622AL\
Data File : FE035917.D
Signal(s) : FID1B.CH
Acq On : 06 Jun 2022 17:21
Operator : YP\AJ
Sample : N3168-01
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
HELENS-0602


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File: sample.E
Quant Time: Jun 07 01:24:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
Quant Title : GC Extractables
QLast Update : Wed May 11 03:24:10 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

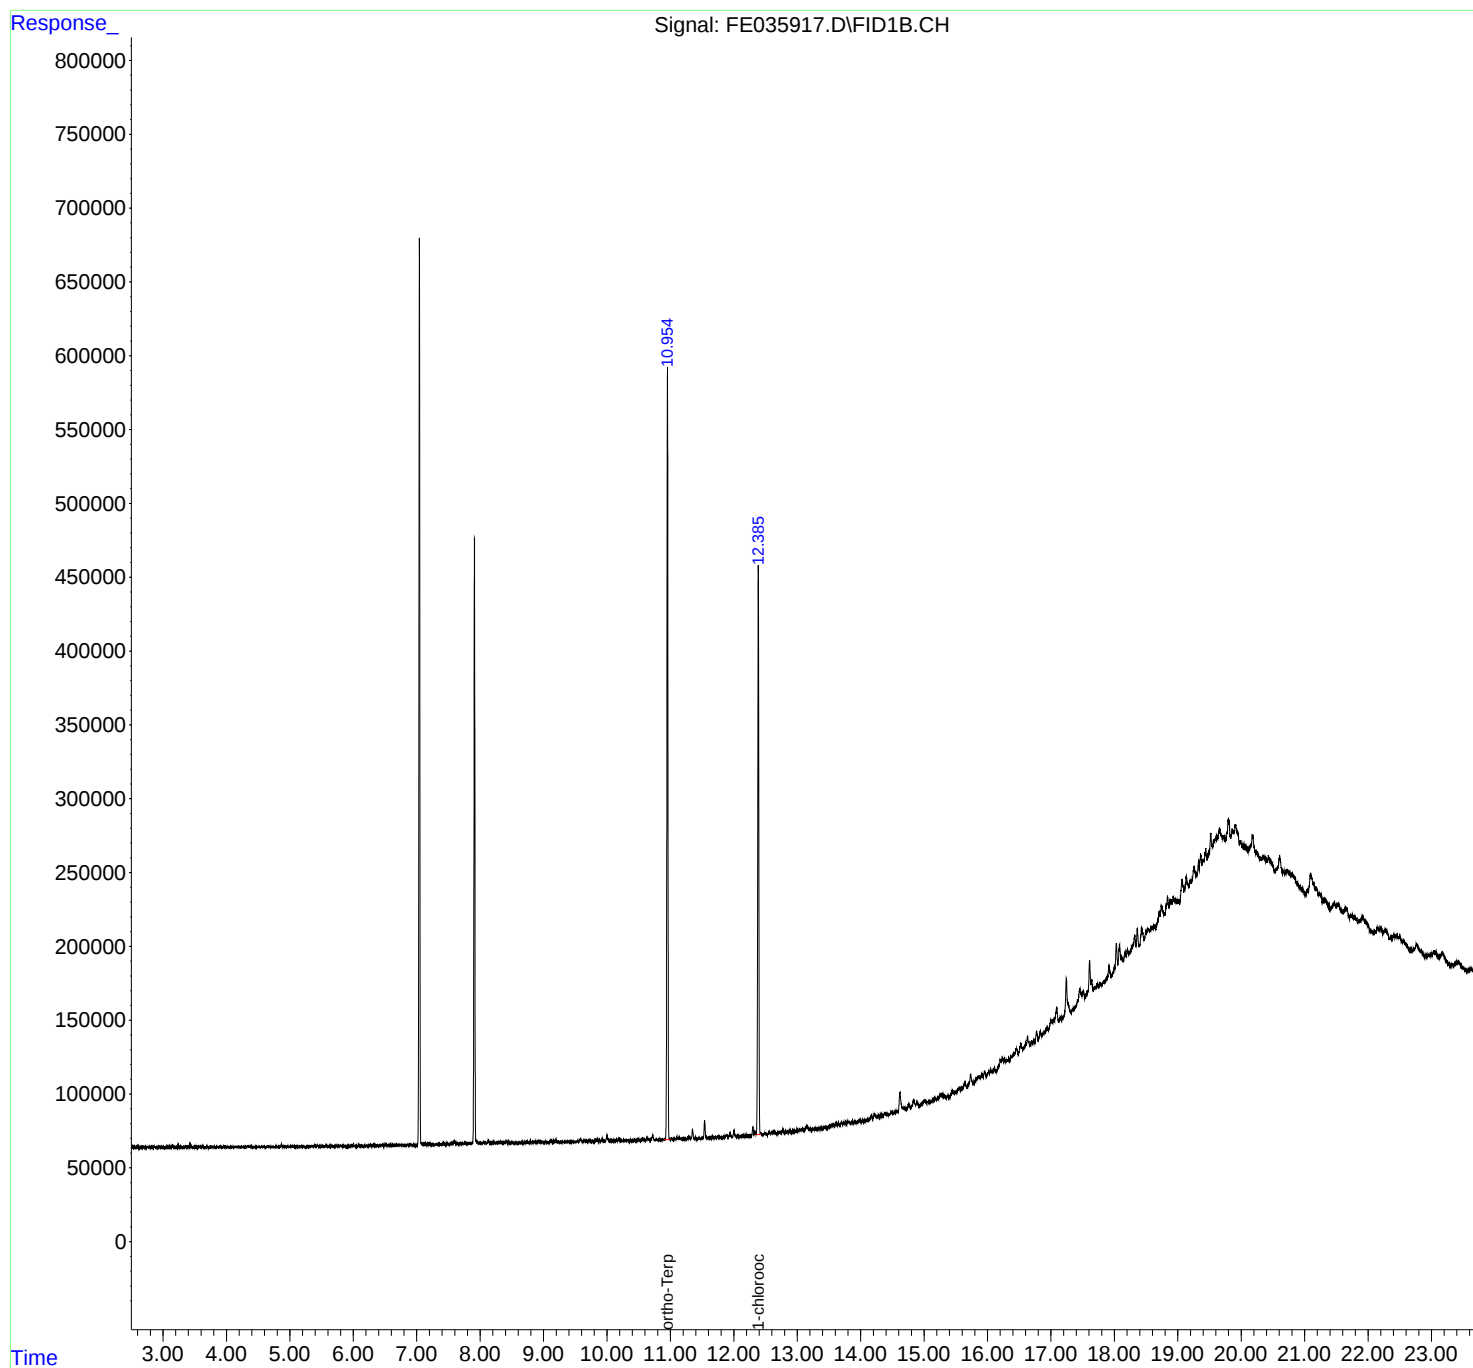

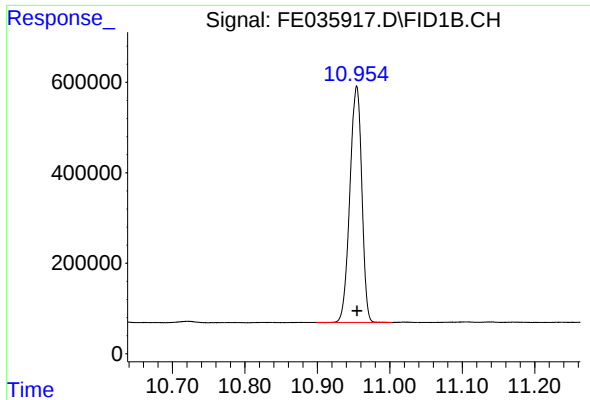


#9 ortho-Terphenyl (SURR)

R.T.: 10.954 min
Delta R.T.: 0.000 min
Response: 5984764
Conc: 45.12 ug/ml

Instrument :
FID_E
ClientSampleId :
HELENS-0602

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

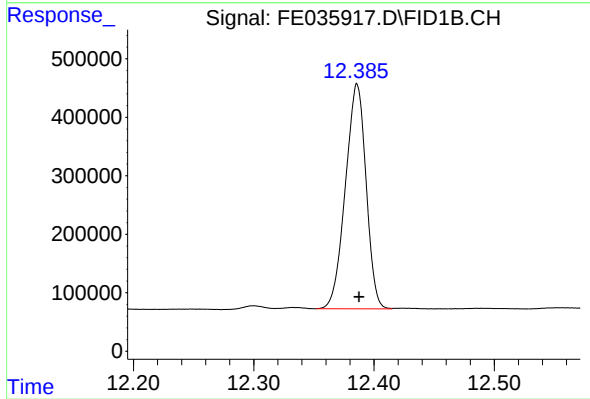

#12 1-chlorooctadecane (SURR)

R.T.: 12.385 min
Delta R.T.: -0.002 min
Response: 4600239
Conc: 43.98 ug/ml m