

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060622AL\
 Data File : FE035930.D
 Signal(s) : FID1B.CH
 Acq On : 07 Jun 2022 00:11
 Operator : YP\AJ
 Sample : N3162-05DL 2X
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 D-14B-9-SB-SW-2(5.5-6.0)DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/07/2022
 Supervised By :Ankita Jodhani 06/07/2022

Integration File: autoint1.e
 Quant Time: Jun 07 01:26:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
 Quant Title : GC Extractables
 QLast Update : Wed May 11 03:24:10 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.951	3518904	26.528 ug/mlm
Spiked Amount	50.000	Recovery	= 53.06%
12) S 1-chlorooctadecane (S...	12.382	2806972	26.834 ug/ml
Spiked Amount	50.000	Recovery	= 53.67%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060622AL\
Data File : FE035930.D
Signal(s) : FID1B.CH
Acq On : 07 Jun 2022 00:11
Operator : YP\AJ
Sample : N3162-05DL 2X
Misc :
ALS Vial : 26 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
D-14B-9-SB-SW-2(5.5-6.0)DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

Integration File: autoint1.e
Quant Time: Jun 07 01:26:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051022.M
Quant Title : GC Extractables
QLast Update : Wed May 11 03:24:10 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

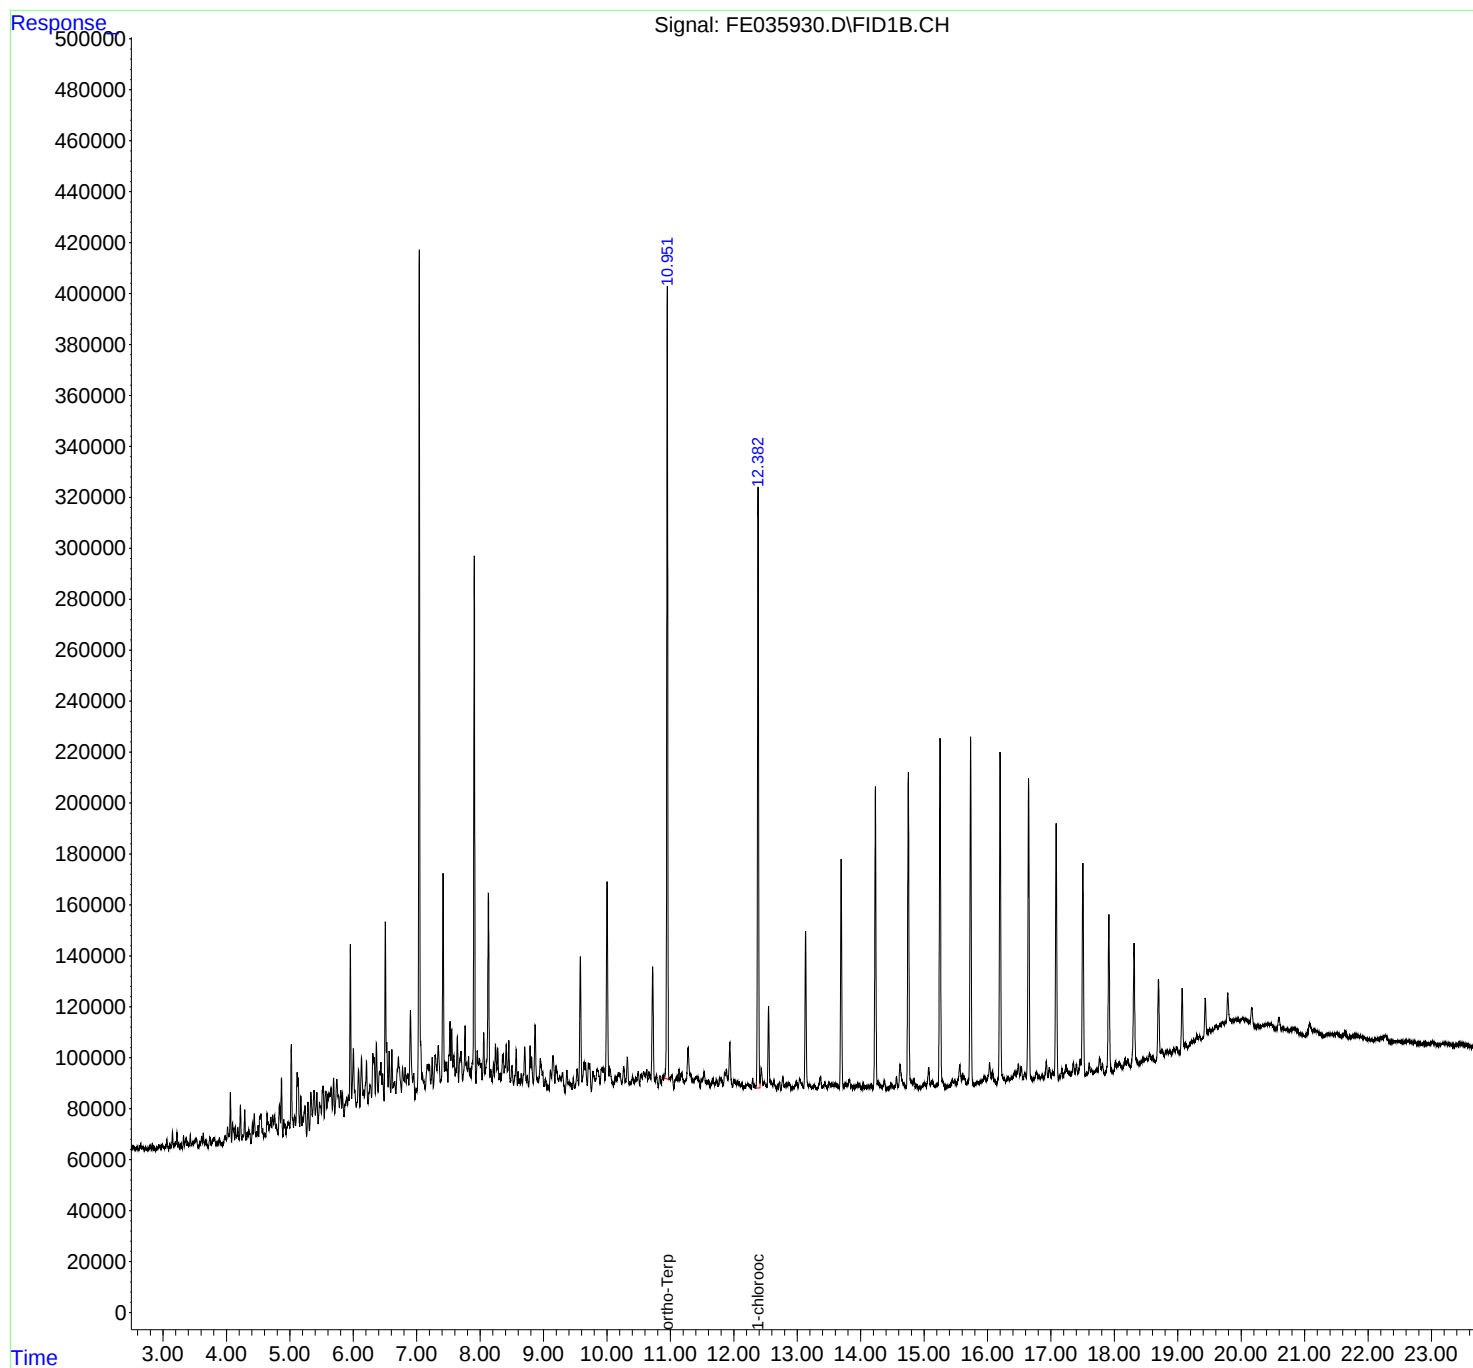

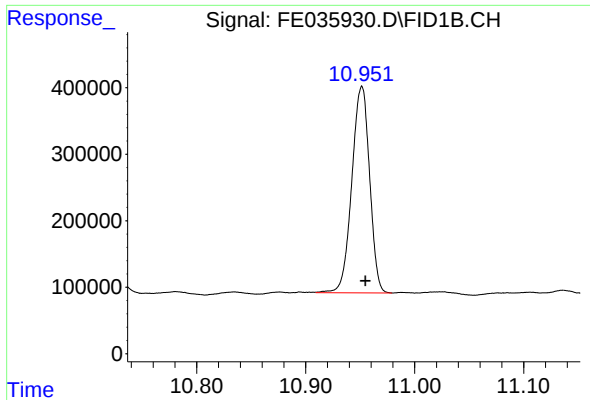


#9 ortho-Terphenyl (SURR)

R.T.: 10.951 min
Delta R.T.: -0.004 min
Response: 3518904
Conc: 26.53 ug/ml

Instrument :
FID_E
ClientSampleId :
D-14B-9-SB-SW-2(5.5-6.0)DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/07/2022
Supervised By :Ankita Jodhani 06/07/2022

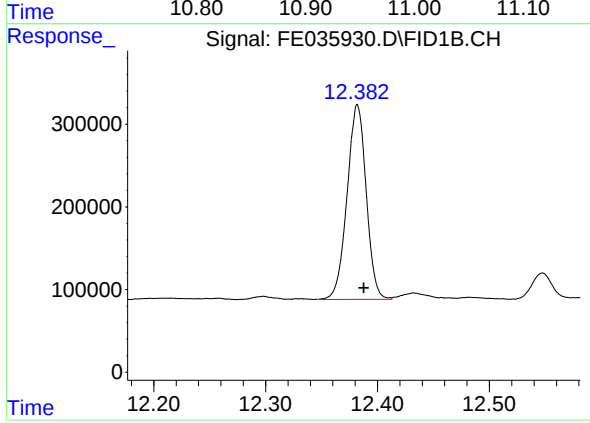

#12 1-chlorooctadecane (SURR)

R.T.: 12.382 min
Delta R.T.: -0.005 min
Response: 2806972
Conc: 26.83 ug/ml