

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060723AL\
 Data File : FE042464.D
 Signal(s) : FID1B.ch
 Acq On : 07 Jun 2023 14:26
 Operator : YP\AJ
 Sample : 03046-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 08 01:44:21 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
 Quant Title : GC Extractables
 QLast Update : Thu May 18 06:27:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.386	412554	3.105 ug/ml
Spiked Amount 50.000		Recovery =	6.21%
Target Compounds			
10) T n-Eicosane (C20)	12.933	226845	1.497 ug/ml
14) T n-Tetracosane (C24)	15.234	138861	0.962 ug/ml
20) T n-Hexatriacontane (C36)	20.498	246427	1.896 ug/ml
22) T n-Tetracontane (C40)	22.181	466798	3.355 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE060723AL\
Data File : FE042464.D
Signal(s) : FID1B.ch
Acq On : 07 Jun 2023 14:26
Operator : YP\AJ
Sample : 03046-13DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 08 01:44:21 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
Quant Title : GC Extractables
QLast Update : Thu May 18 06:27:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

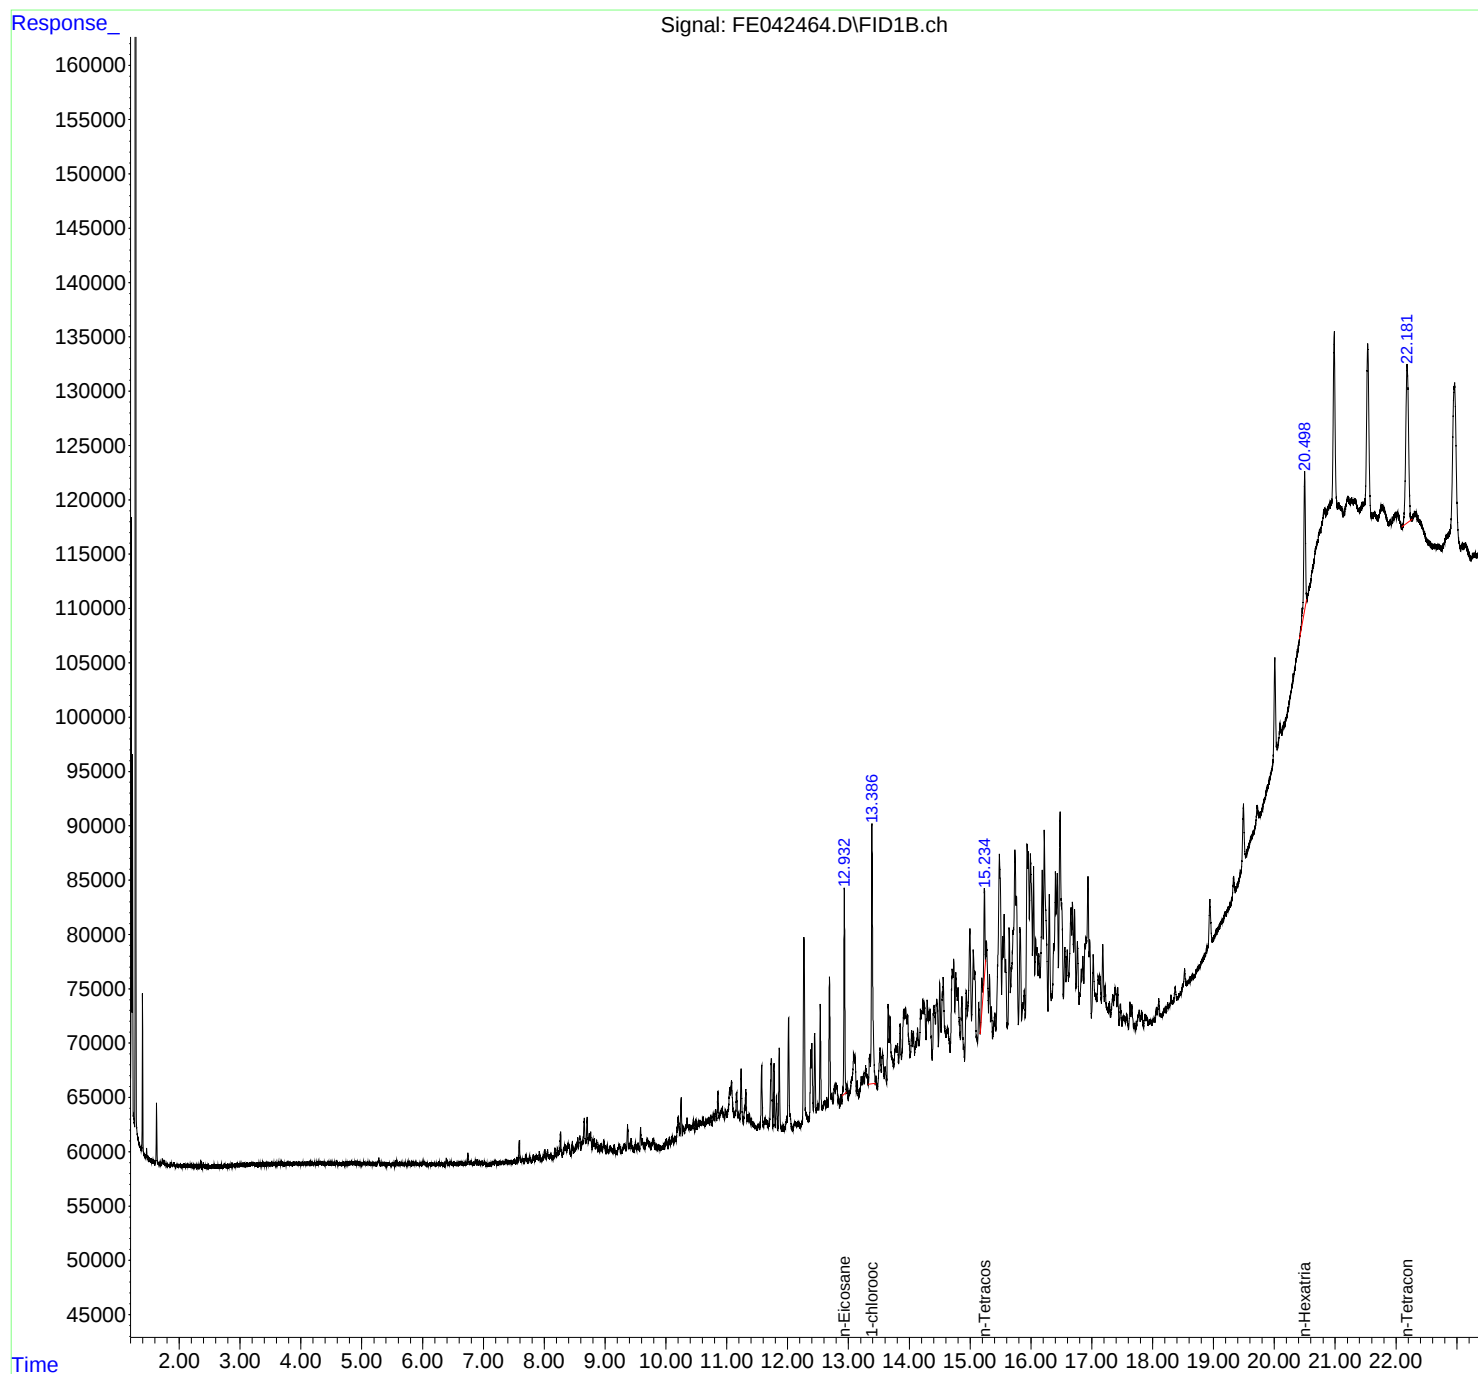


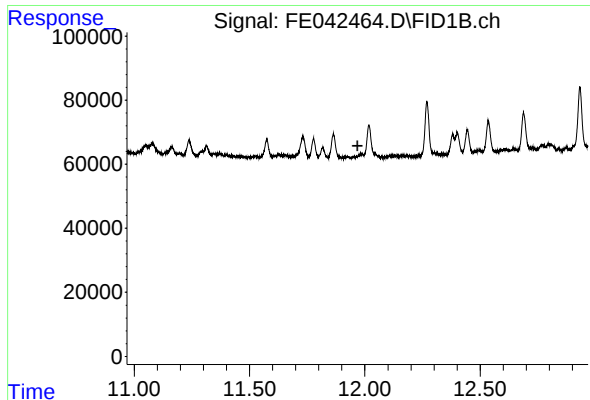

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.968 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

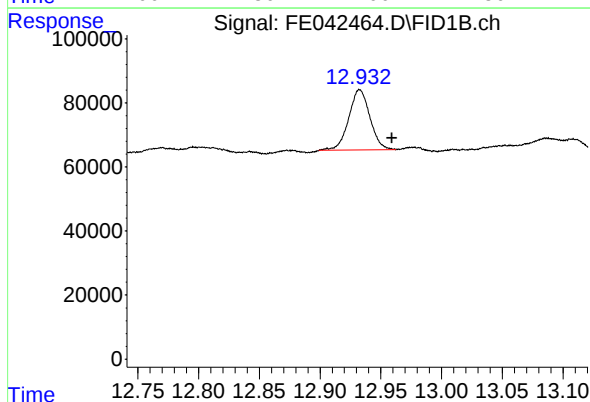


#10 n-Eicosane (C20)

R.T.: 12.933 min
Delta R.T.: -0.027 min
Response: 226845
Conc: 1.50 ug/ml

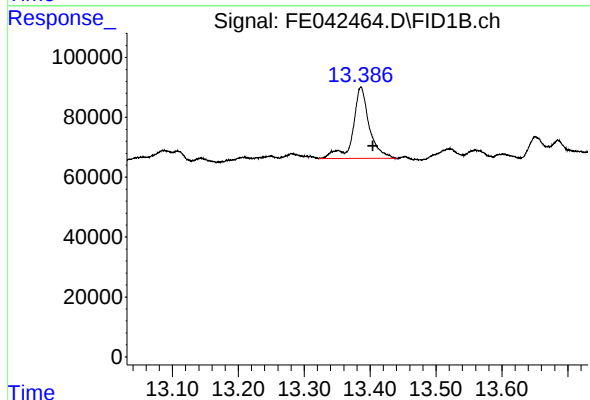


#12 1-chlorooctadecane (SURR)

R.T.: 13.386 min
Delta R.T.: -0.018 min
Response: 412554
Conc: 3.10 ug/ml

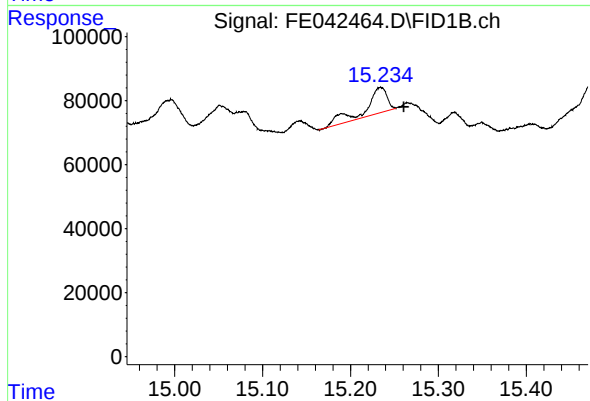

#14 n-Tetracosane (C24)


R.T.: 15.234 min
Delta R.T.: -0.026 min
Response: 138861
Conc: 0.96 ug/ml

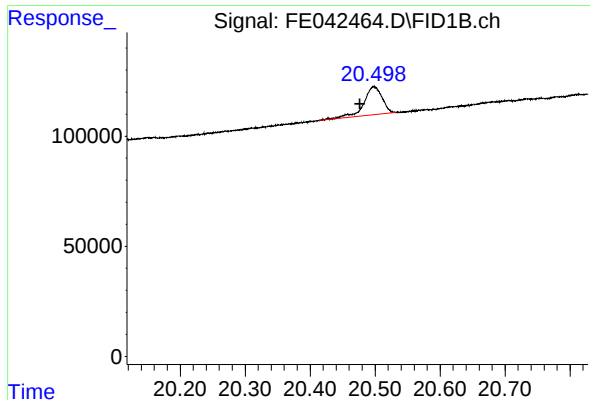

#20 n-Hexatriacontane (C36)

R.T.: 20.498 min
Delta R.T.: 0.022 min
Response: 246427
Conc: 1.90 ug/ml

Instrument :
FID_E
ClientSampleId :

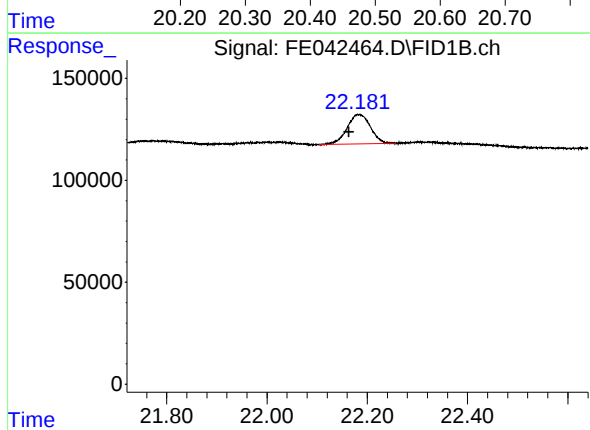

#22 n-Tetracontane (C40)

R.T.: 22.181 min
Delta R.T.: 0.018 min
Response: 466798
Conc: 3.36 ug/ml