

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061021\
 Data File : FE033954.D
 Signal(s) : FID1B.CH
 Acq On : 10 Jun 2021 9:12
 Operator : DD\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 11 02:03:32 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
 Quant Title :
 QLast Update : Mon Jun 07 02:30:45 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.713	19054138	49.788 ug/ml
Target Compounds			
2) N-DECANE	4.453	21643572	53.067 ug/ml
3) N-DODECANE	6.466	22029160	53.299 ug/ml
4) N-TETRADECANE	8.262	22337099	52.459 ug/ml
5) N-HEXADECANE	9.863	22019469	51.847 ug/ml
6) N-OCTADECANE	11.305	22356777	51.257 ug/ml
7) N-EICOSANE	12.616	22071252	50.800 ug/ml
8) N-DOCOSANE	13.814	21943972	50.277 ug/ml
10) N-TETRACOSANE	14.919	21728597	49.623 ug/ml
11) N-HEXACOSANE	15.940	21235773	48.892 ug/ml
12) N-OCTACOSANE	16.890	20886193	48.001 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061021\
Data File : FE033954.D
Signal(s) : FID1B.CH
Acq On : 10 Jun 2021 9:12
Operator : DD\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 11 02:03:32 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
Quant Title :
QLast Update : Mon Jun 07 02:30:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

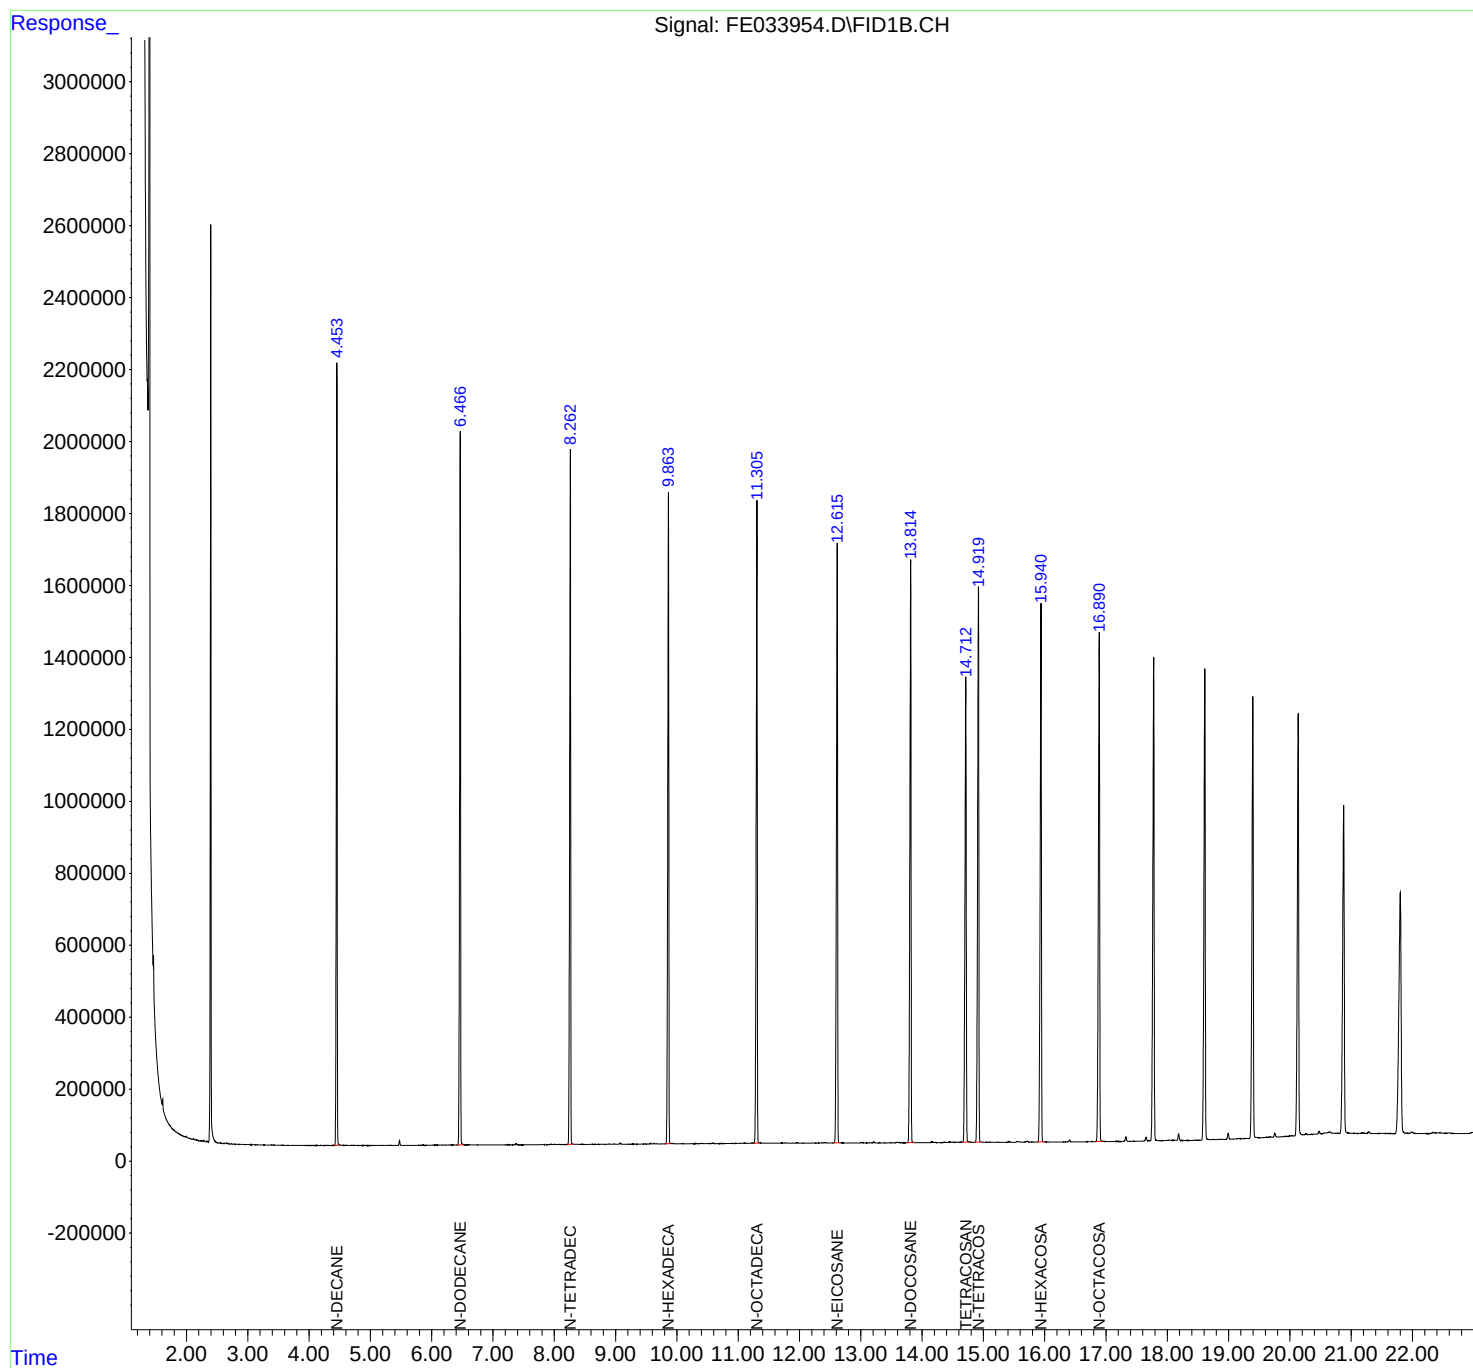

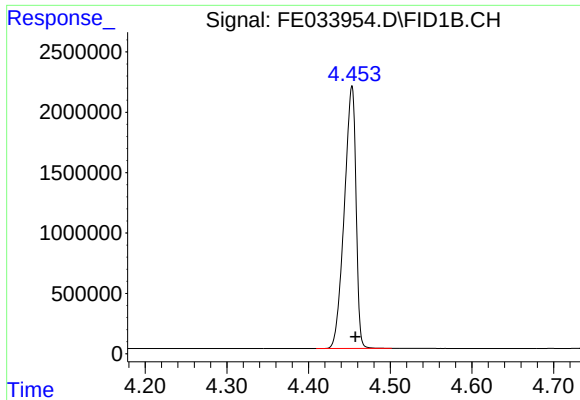


#2 N-DECANE

R.T.: 4.453 min
Delta R.T.: -0.004 min
Response: 21643572
Conc: 53.07 ug/ml

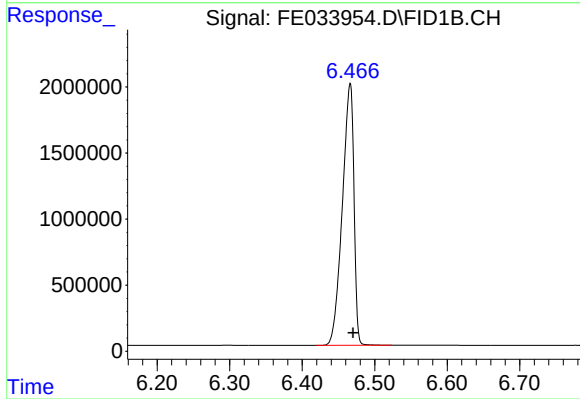


#3 N-DODECANE

R.T.: 6.466 min
Delta R.T.: -0.004 min
Response: 22029160
Conc: 53.30 ug/ml

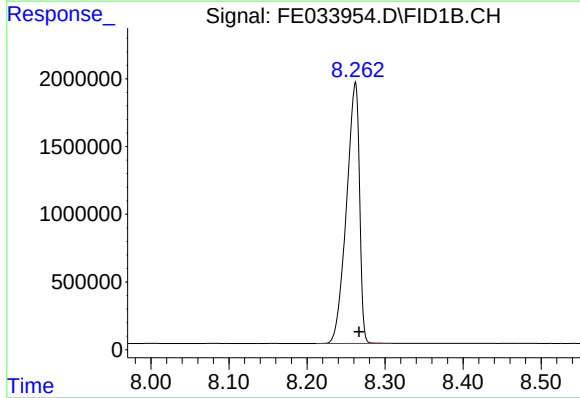


#4 N-TETRADECANE

R.T.: 8.262 min
Delta R.T.: -0.005 min
Response: 22337099
Conc: 52.46 ug/ml

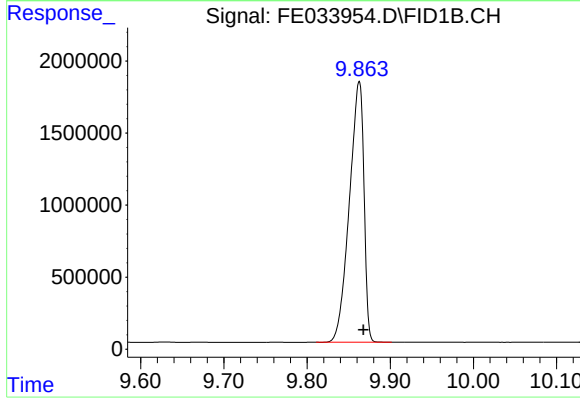


#5 N-HEXADECANE

R.T.: 9.863 min
Delta R.T.: -0.005 min
Response: 22019469
Conc: 51.85 ug/ml

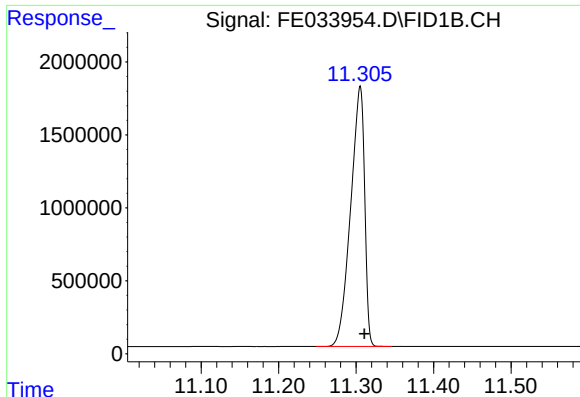


#6 N-OCTADECANE

R.T.: 11.305 min
Delta R.T.: -0.005 min
Response: 22356777
Conc: 51.26 ug/ml

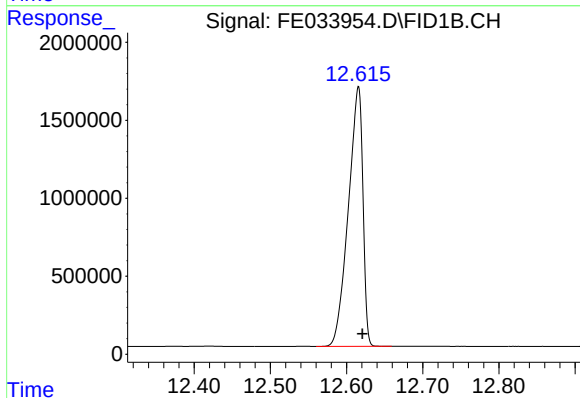


#7 N-EICOSANE

R.T.: 12.616 min
Delta R.T.: -0.005 min
Response: 22071252
Conc: 50.80 ug/ml

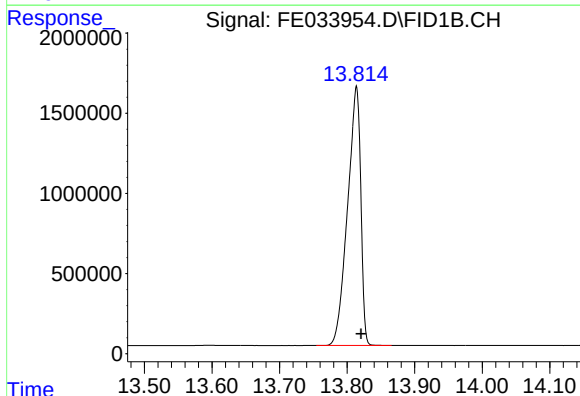


#8 N-DOCOSANE

R.T.: 13.814 min
Delta R.T.: -0.007 min
Response: 21943972
Conc: 50.28 ug/ml

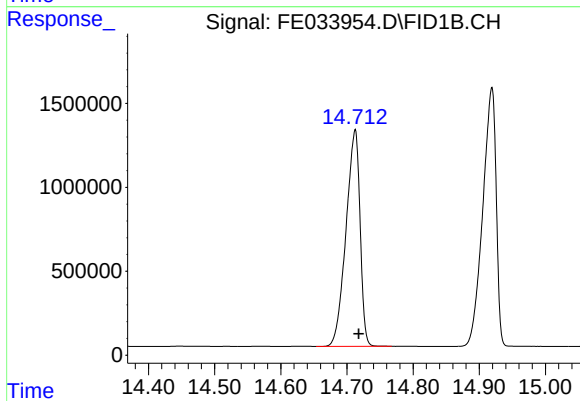


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.713 min
Delta R.T.: -0.005 min
Response: 19054138
Conc: 49.79 ug/ml

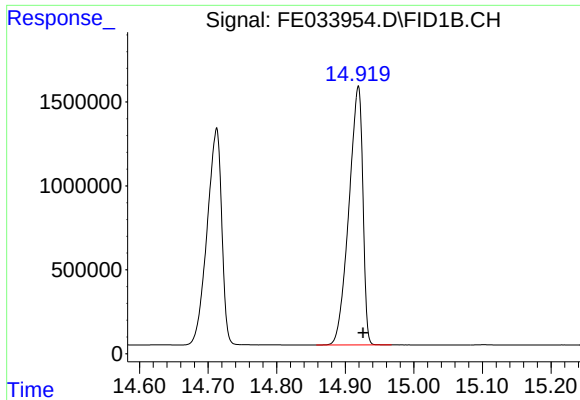


#10 N-TETRACOSANE

R.T.: 14.919 min
Delta R.T.: -0.007 min
Response: 21728597
Conc: 49.62 ug/ml

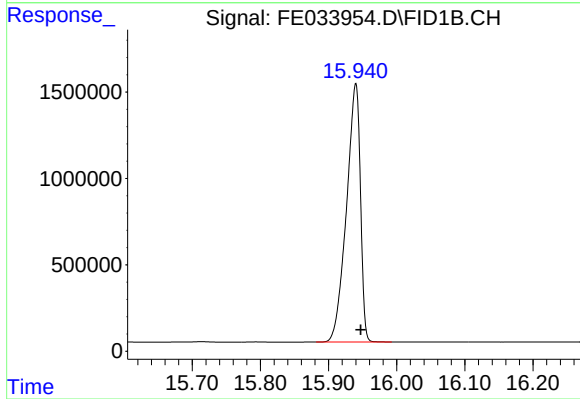

#11 N-HEXACOSANE

R.T.: 15.940 min
Delta R.T.: -0.007 min
Response: 21235773
Conc: 48.89 ug/ml

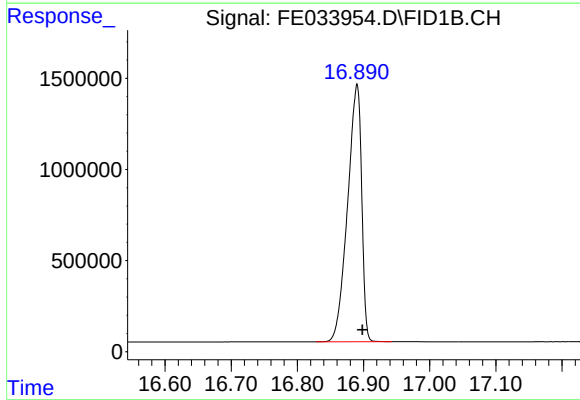

#12 N-OCTACOSANE

R.T.: 16.890 min
Delta R.T.: -0.008 min
Response: 20886193
Conc: 48.00 ug/ml