

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061321\
Data File : FE033973.D
Signal(s) : FID1B.CH
Acq On : 13 Jun 2021 13:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 01:11:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
Quant Title :
QLast Update : Mon Jun 07 02:30:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.701	6463982	16.890 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061321\
Data File : FE033973.D
Signal(s) : FID1B.CH
Acq On : 13 Jun 2021 13:26
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 01:11:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE060521.M
Quant Title :
QLast Update : Mon Jun 07 02:30:45 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

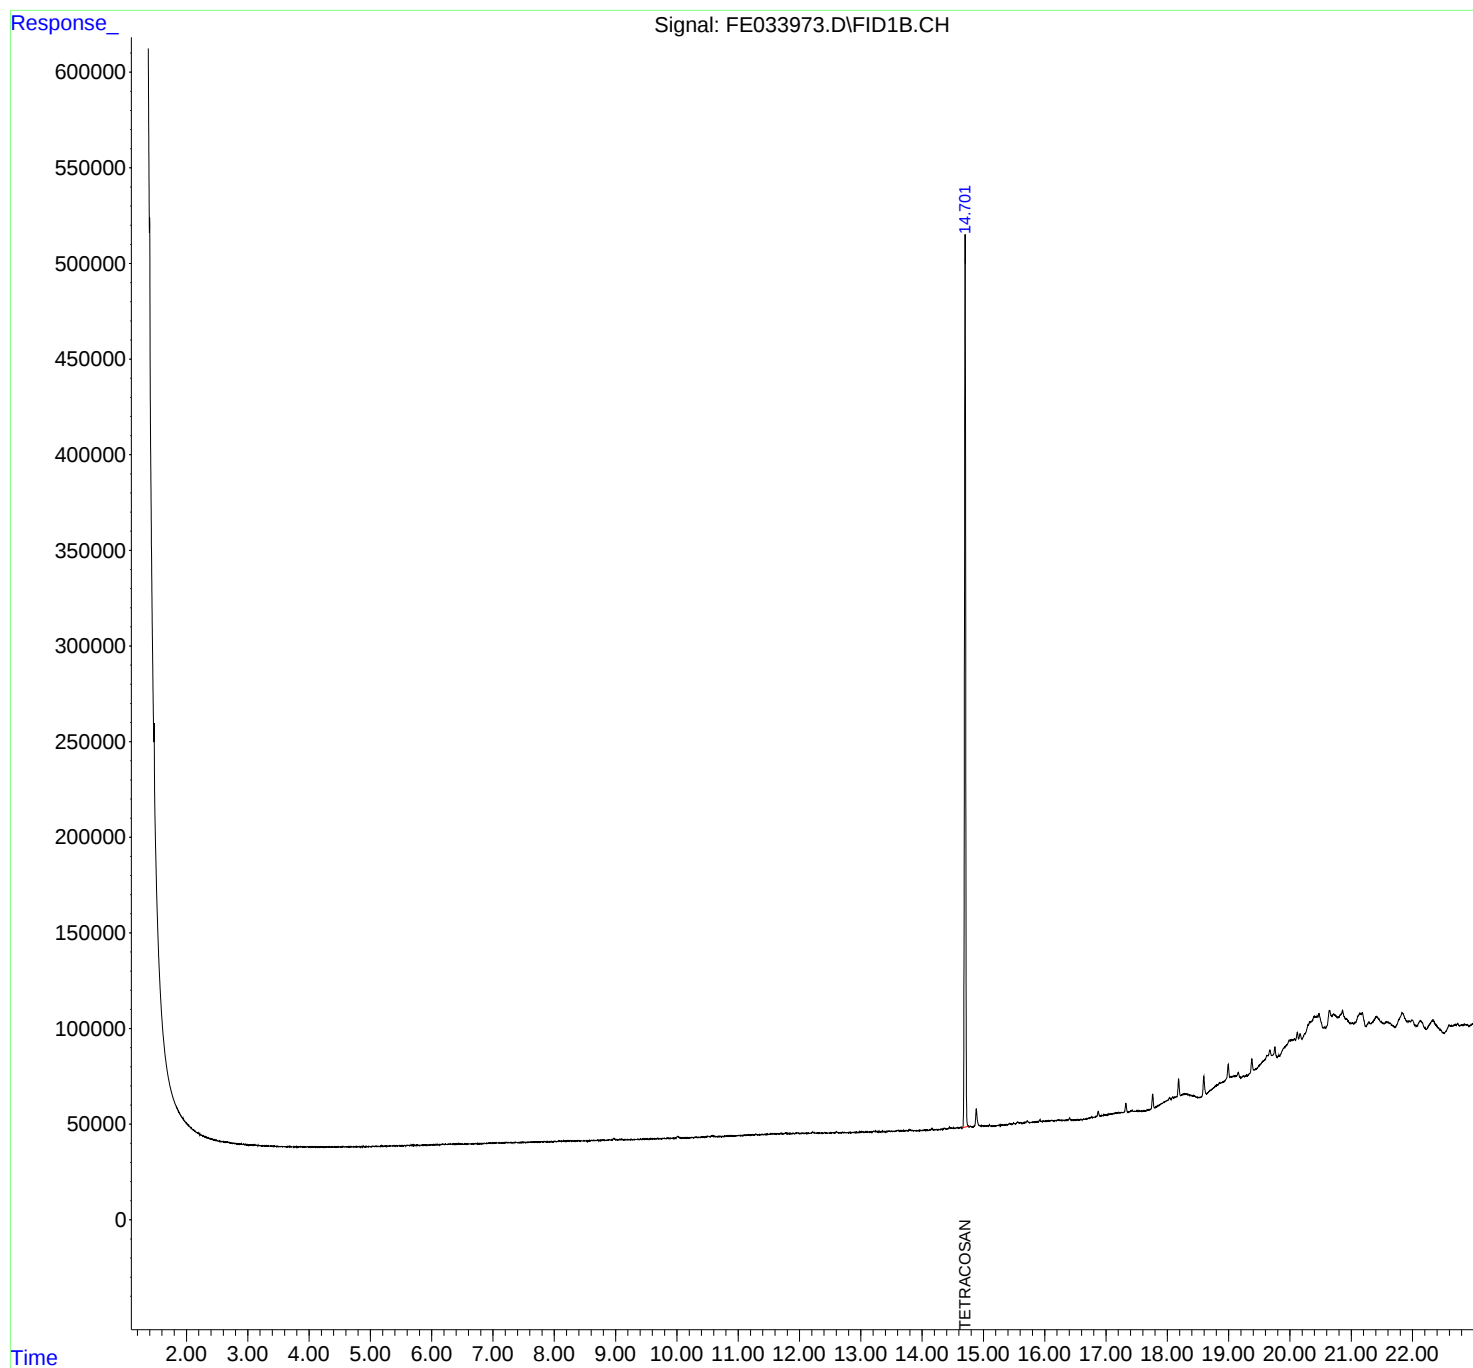

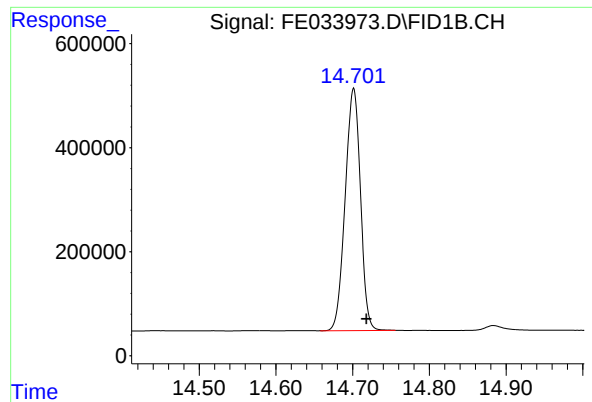

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.701 min
Delta R.T.: -0.017 min
Response: 6463982
Conc: 16.89 ug/ml

Instrument :
FID_E
ClientSampleId :