

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061324AL\
Data File : FE048690.D
Signal(s) : FID1B.ch
Acq On : 13 Jun 2024 05:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 01:17:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.915	56880	0.430 ug/ml
11) T	n-Heneicosane (C21)	13.534	97642	0.754 ug/ml
13) T	n-Docosane (C22)	14.120	66421	0.515 ug/ml
14) T	n-Tetracosane (C24)	15.221	89654	0.692 ug/ml
18) T	n-Dotriacontane (C32)	18.915	127323	0.938 ug/ml
19) T	n-Tetratriacontane (C34)	19.694	103354	0.756 ug/ml
20) T	n-Hexatriacontane (C36)	20.434	55843	0.411 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061324AL\
Data File : FE048690.D
Signal(s) : FID1B.ch
Acq On : 13 Jun 2024 05:58
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 14 01:17:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

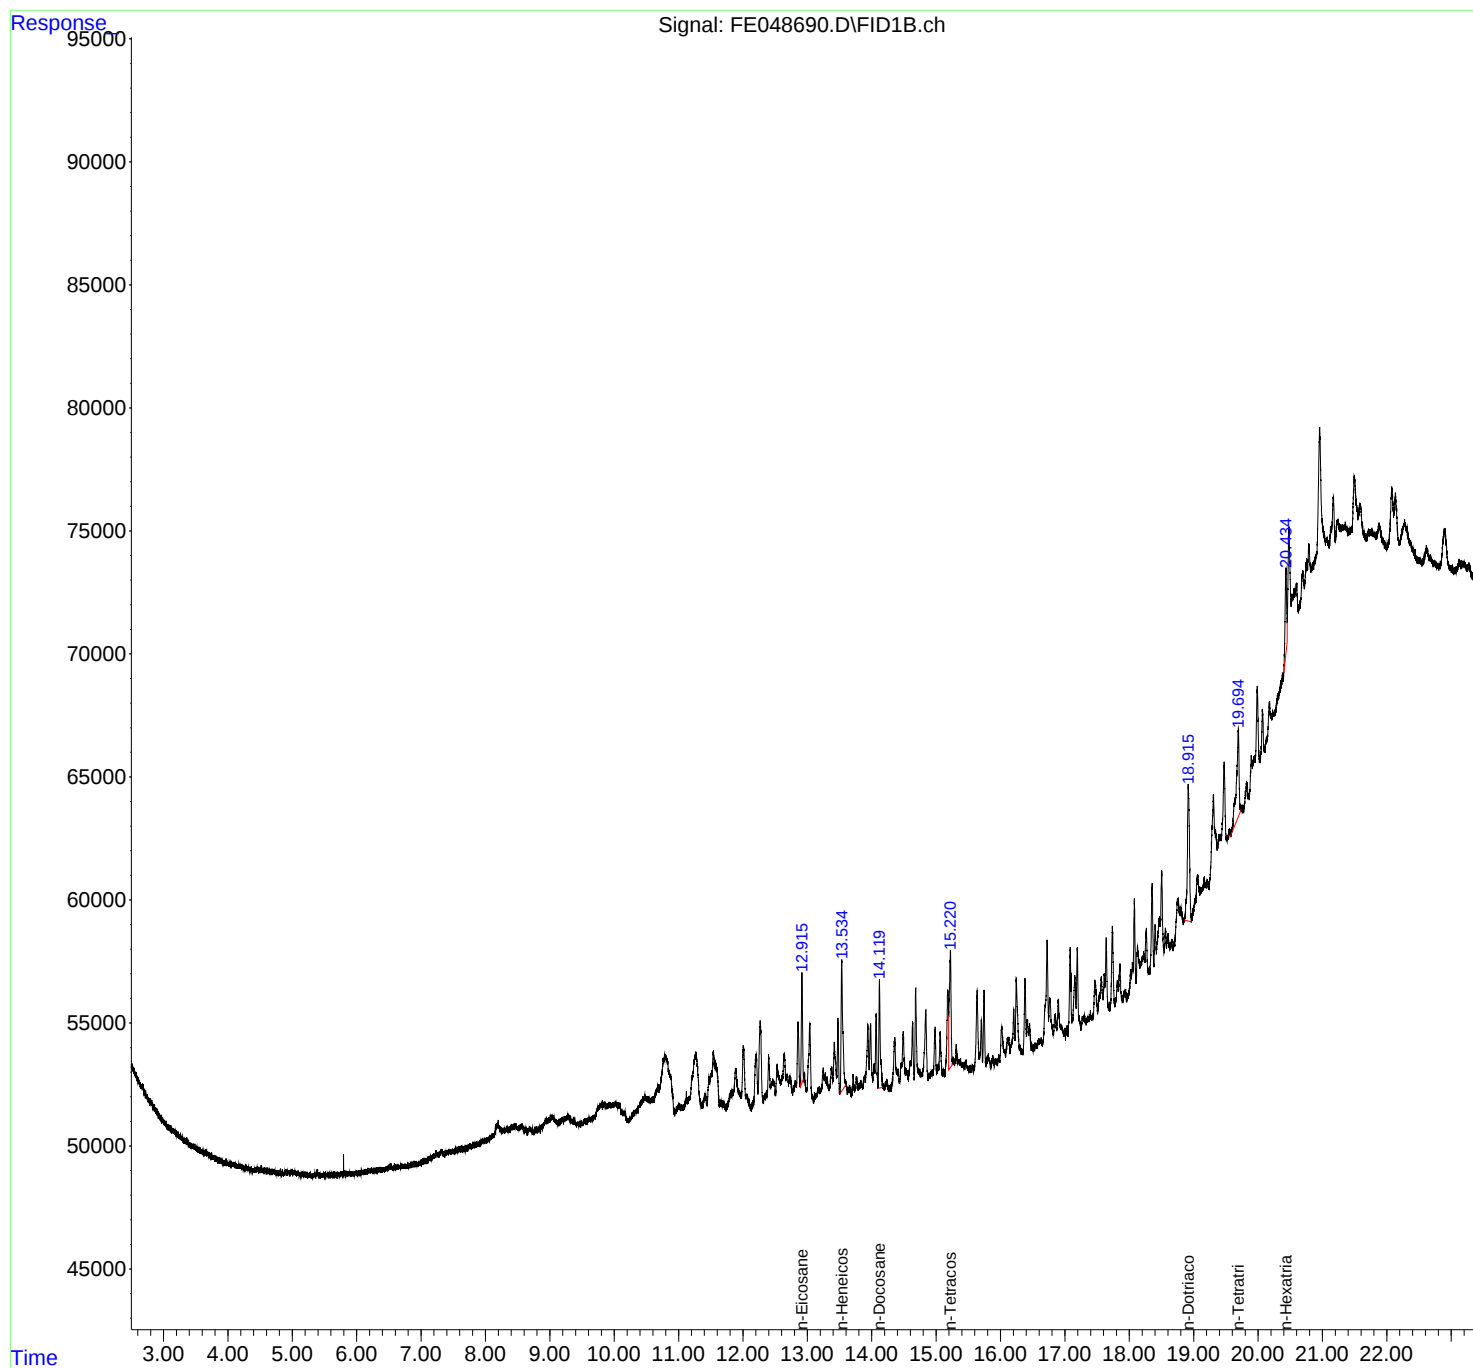


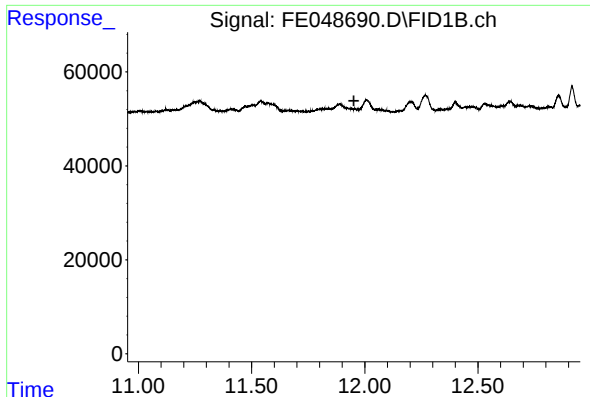

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.952 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

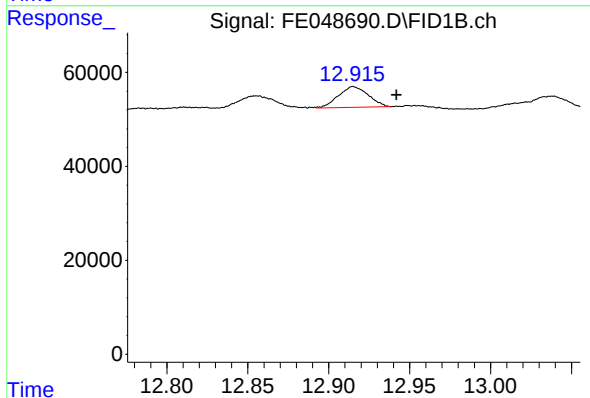


#10 n-Eicosane (C20)

R.T.: 12.915 min
Delta R.T.: -0.027 min
Response: 56880
Conc: 0.43 ug/ml

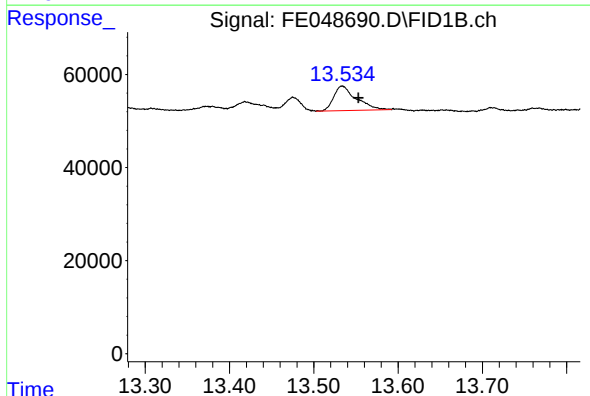


#11 n-Heneicosane (C21)

R.T.: 13.534 min
Delta R.T.: -0.019 min
Response: 97642
Conc: 0.75 ug/ml

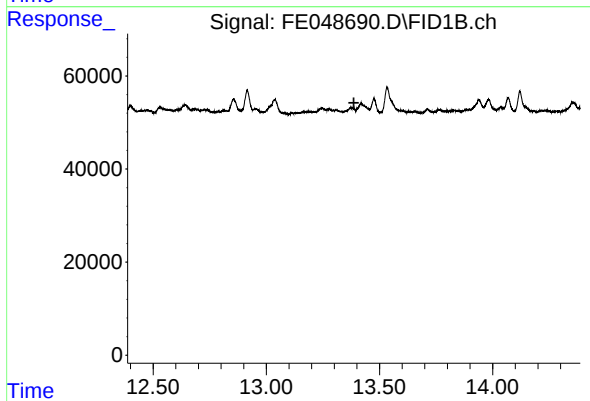

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.387 min
Response: 0
Conc: N.D.

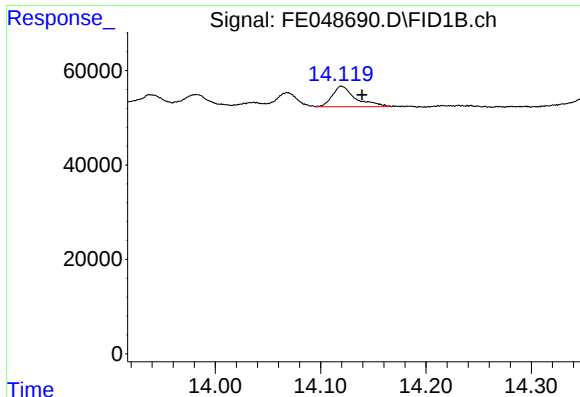

#13 n-Docosane (C22)


R.T.: 14.120 min
Delta R.T.: -0.020 min
Response: 66421
Conc: 0.52 ug/ml

Instrument :
FID_E
ClientSampleId :

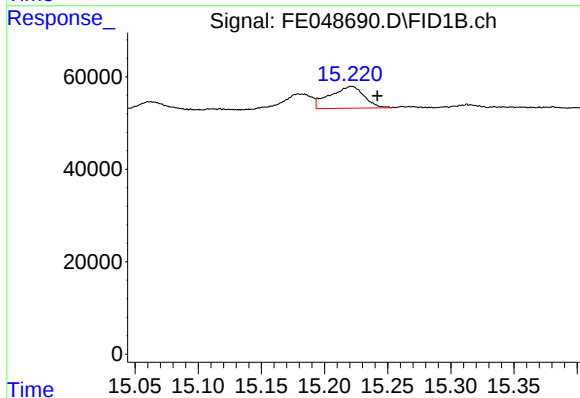


#14 n-Tetracosane (C24)

R.T.: 15.221 min
Delta R.T.: -0.021 min
Response: 89654
Conc: 0.69 ug/ml

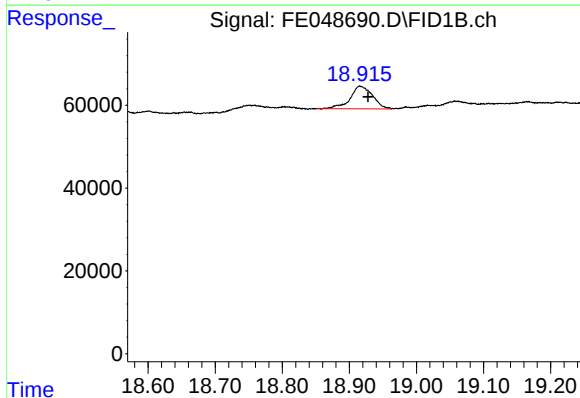


#18 n-Dotriacontane (C32)

R.T.: 18.915 min
Delta R.T.: -0.012 min
Response: 127323
Conc: 0.94 ug/ml

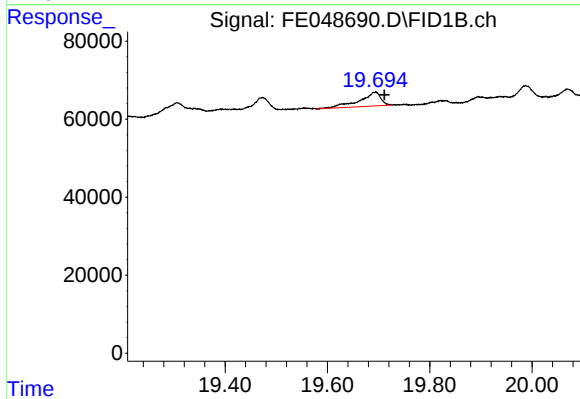

#19 n-Tetratriacontane (C34)

R.T.: 19.694 min
Delta R.T.: -0.017 min
Response: 103354
Conc: 0.76 ug/ml

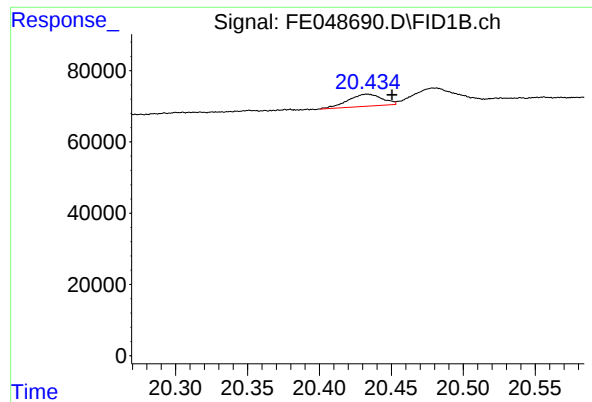

#20 n-Hexatriacontane (C36)

R.T.: 20.434 min
Delta R.T.: -0.017 min
Response: 55843
Conc: 0.41 ug/ml

Instrument :

FID_E

ClientSampleId :