

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061523AL\
 Data File : FE042622.D
 Signal(s) : FID1B.ch
 Acq On : 15 Jun 2023 07:57
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 00:32:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
 Quant Title : GC Extractables
 QLast Update : Thu May 18 06:27:12 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.904f	225590	1.488 ug/ml
11) T n-Heneicosane (C21)	13.531	186956	1.262 ug/ml
13) T n-Docosane (C22)	14.122	199409	1.360 ug/ml
14) T n-Tetracosane (C24)	15.228	186540	1.292 ug/ml
15) T n-Hexacosane (C26)	16.251	125383	0.905 ug/ml
16) T n-Octacosane (C28)	17.202	98492	0.736 ug/ml
18) T n-Dotriacontane (C32)	18.923	216056	1.617 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061523AL\
Data File : FE042622.D
Signal(s) : FID1B.ch
Acq On : 15 Jun 2023 07:57
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 00:32:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 051823.M
Quant Title : GC Extractables
QLast Update : Thu May 18 06:27:12 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

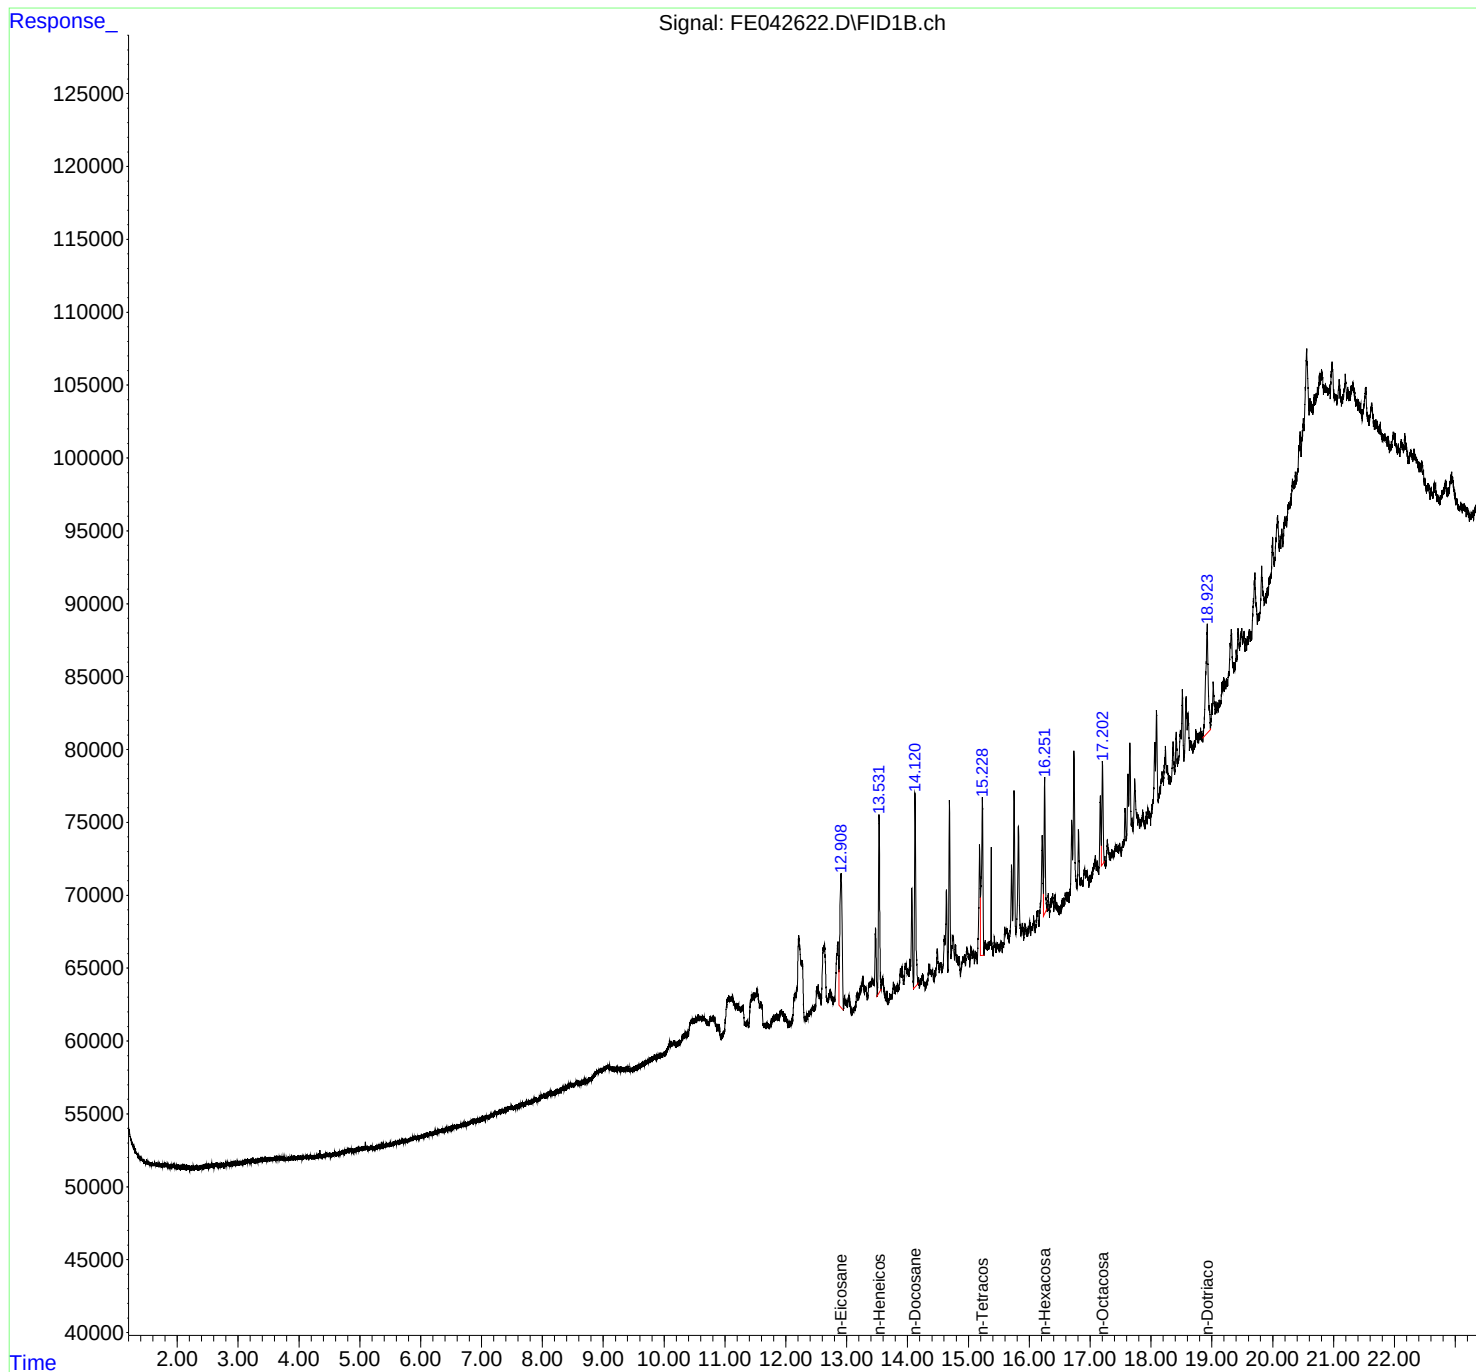


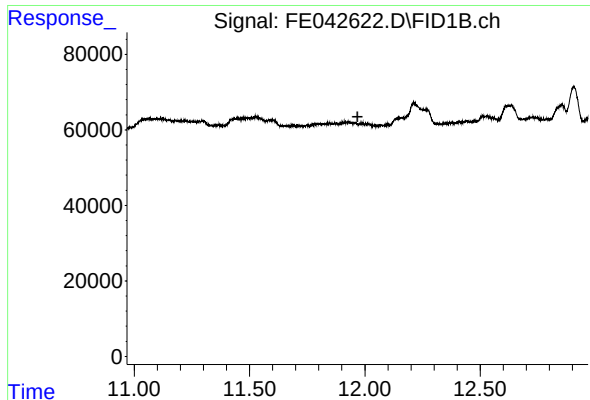

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.968 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

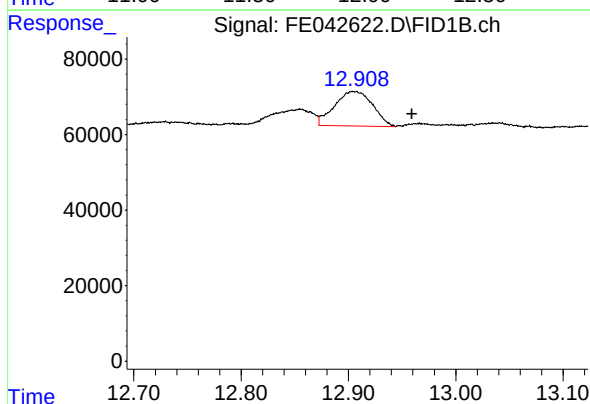


#10 n-Eicosane (C20)

R.T.: 12.904 min
Delta R.T.: -0.055 min
Response: 225590
Conc: 1.49 ug/ml

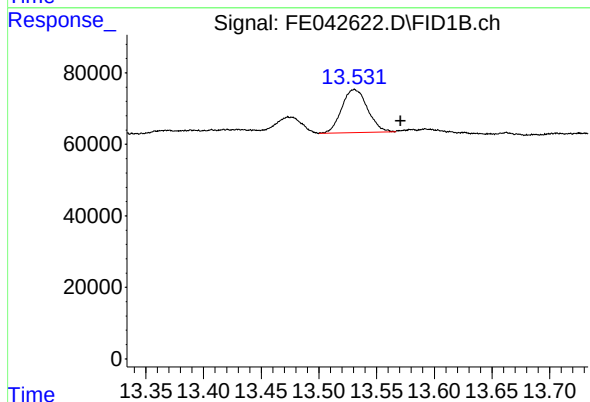


#11 n-Heneicosane (C21)

R.T.: 13.531 min
Delta R.T.: -0.040 min
Response: 186956
Conc: 1.26 ug/ml

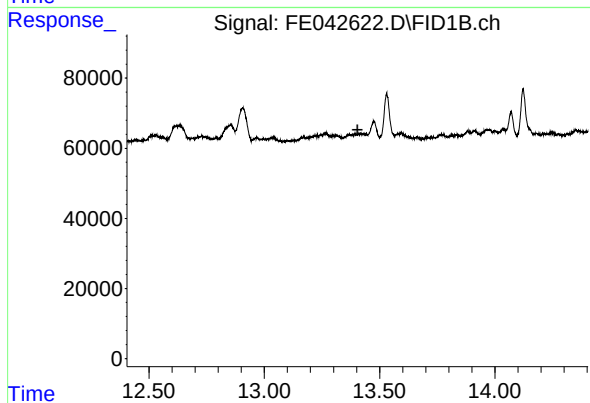

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.404 min
Response: 0
Conc: N.D.

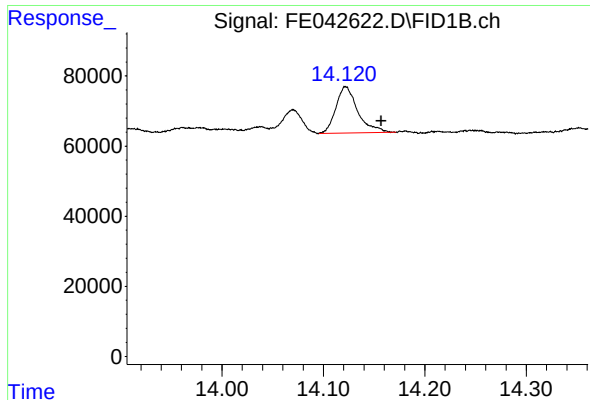

#13 n-Docosane (C22)


R.T.: 14.122 min
Delta R.T.: -0.035 min
Response: 199409
Conc: 1.36 ug/ml

Instrument :
FID_E
ClientSampleId :

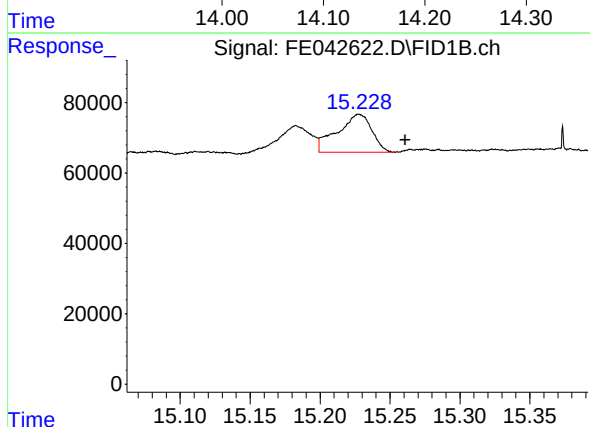


#14 n-Tetracosane (C24)

R.T.: 15.228 min
Delta R.T.: -0.033 min
Response: 186540
Conc: 1.29 ug/ml

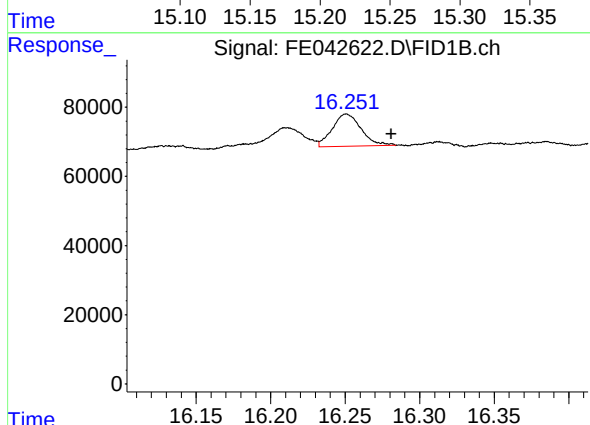


#15 n-Hexacosane (C26)

R.T.: 16.251 min
Delta R.T.: -0.030 min
Response: 125383
Conc: 0.91 ug/ml

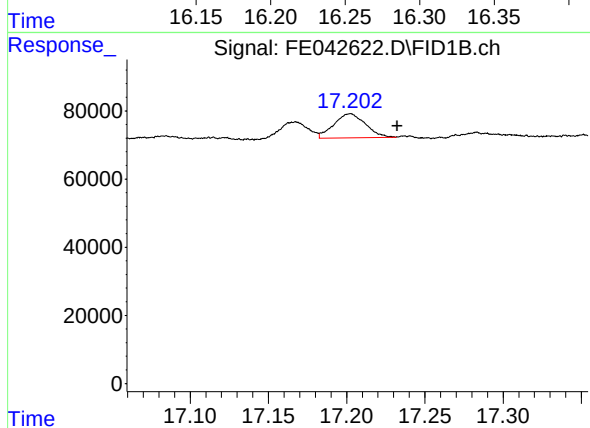

#16 n-Octacosane (C28)

R.T.: 17.202 min
Delta R.T.: -0.030 min
Response: 98492
Conc: 0.74 ug/ml

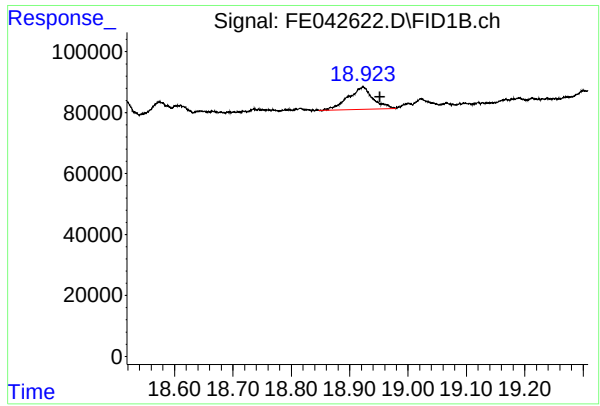

#18 n-Dotriacontane (C32)

R.T.: 18.923 min
Delta R.T.: -0.029 min
Response: 216056
Conc: 1.62 ug/ml

Instrument :
FID_E
ClientSampleId :