

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE061620\  
 Data File : FE032179.D  
 Signal(s) : FID1B.CH  
 Acq On : 16 Jun 2020 10:30  
 Operator : DD\AJ  
 Sample : RT MARKER  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
 Quant Time: Jun 17 00:48:57 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE061120.M  
 Quant Title :  
 QLast Update : Thu Jun 11 13:38:20 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.510  | 7749798  | 20.792 ug/ml |
| 12) N-OCTACOSANE            | 16.922 | 6967501  | 19.064 ug/ml |
| 13) N-TRIACONTANE           | 17.801 | 261777   | 0.719 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.632 | 264137   | 0.771 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.415 | 188714   | 0.662 ug/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE061620\  
Data File : FE032179.D  
Signal(s) : FID1B.CH  
Acq On : 16 Jun 2020 10:30  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Jun 17 00:48:57 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\FE061120.M  
Quant Title :  
QLast Update : Thu Jun 11 13:38:20 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

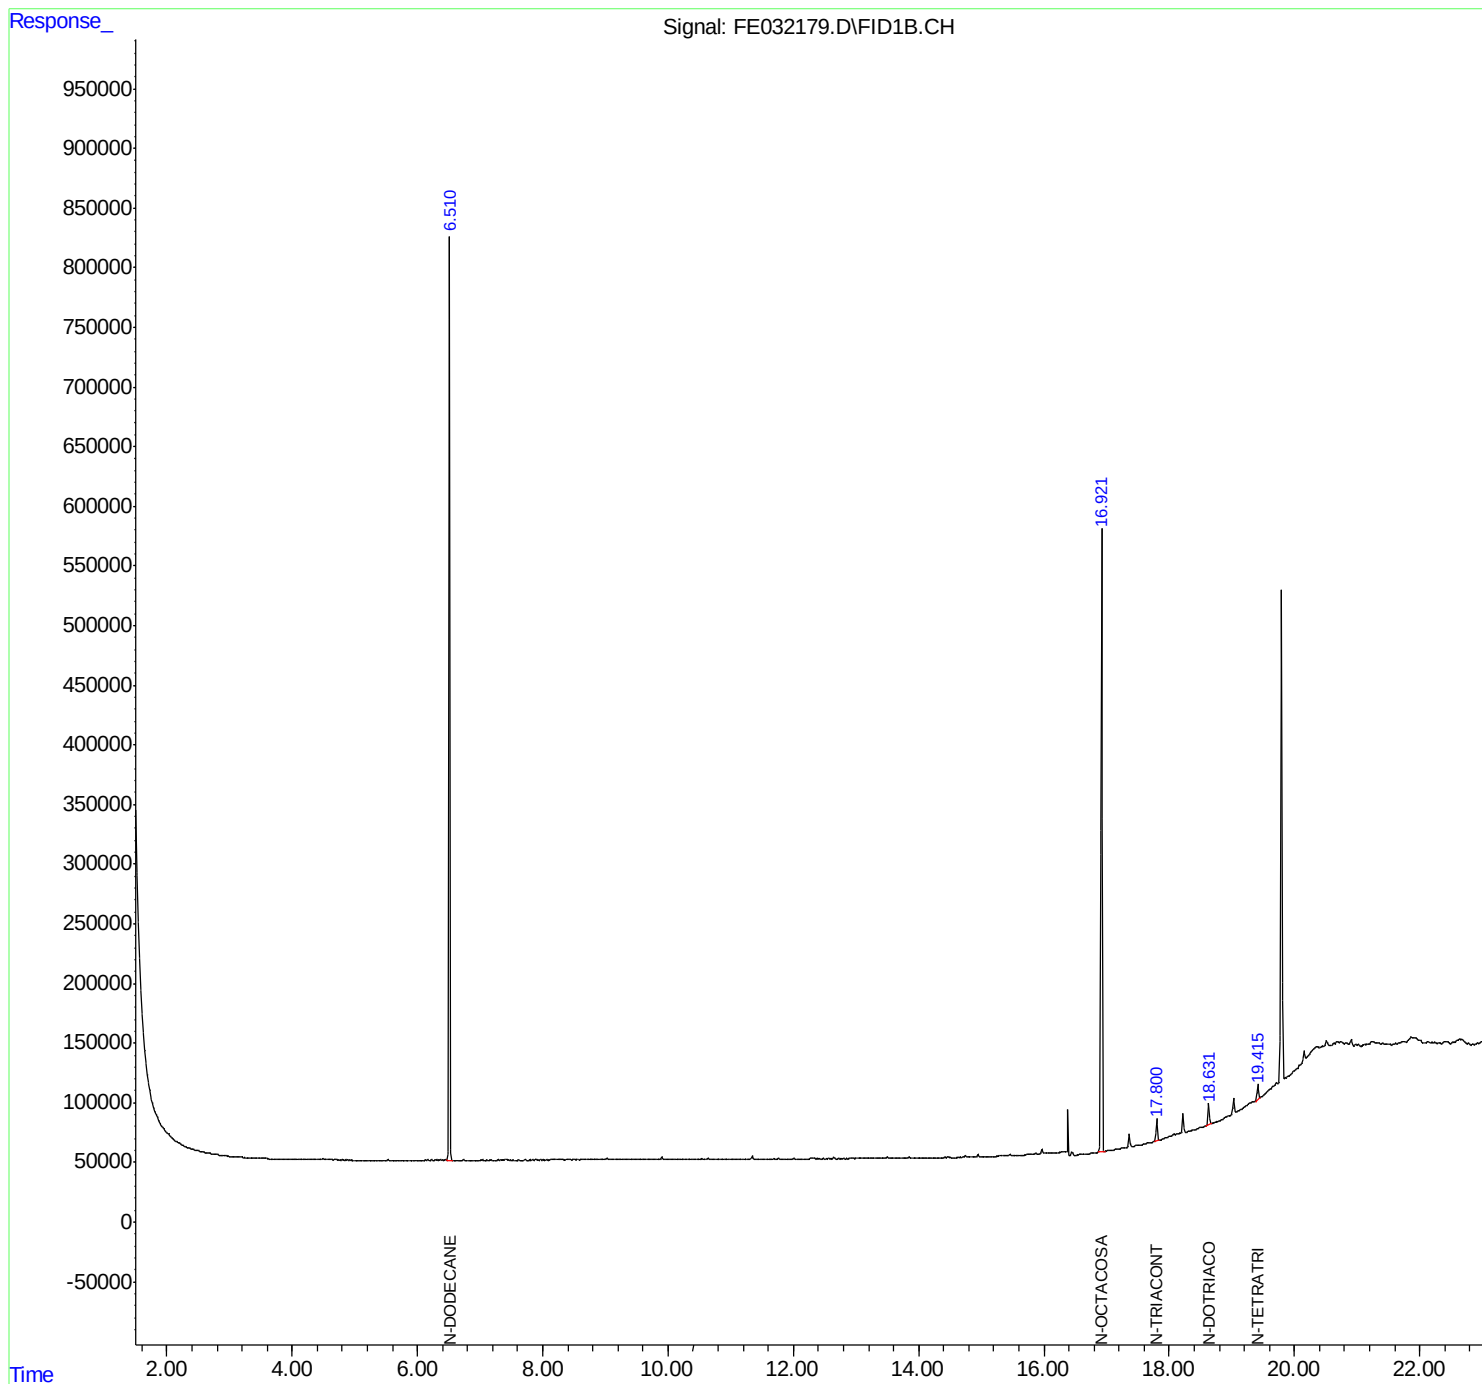

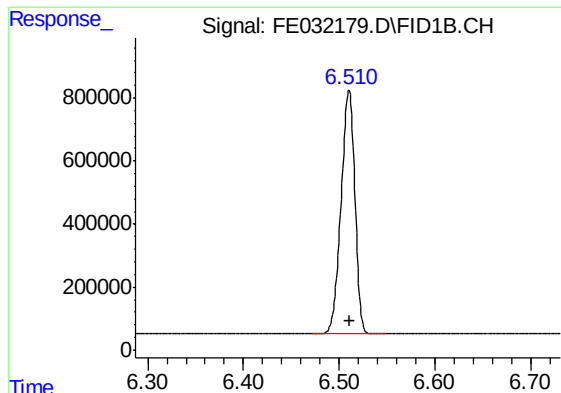


#3 N-DODECANE

R.T.: 6.510 min  
Delta R.T.: 0.000 min  
Response: 7749798  
Conc: 20.79 ug/ml

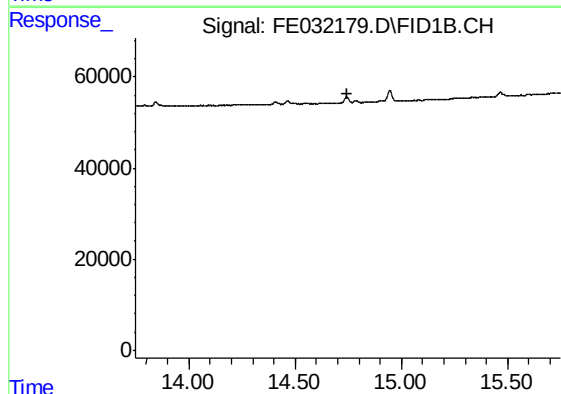


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T. : 14.748 min  
Response: 0  
Conc: N.D.

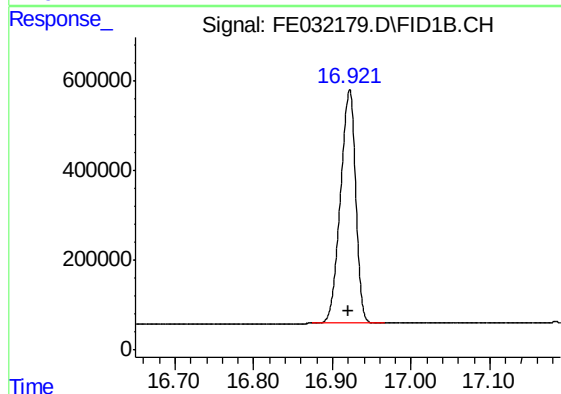


#12 N-OCTACOSANE

R.T.: 16.922 min  
Delta R.T.: 0.000 min  
Response: 6967501  
Conc: 19.06 ug/ml

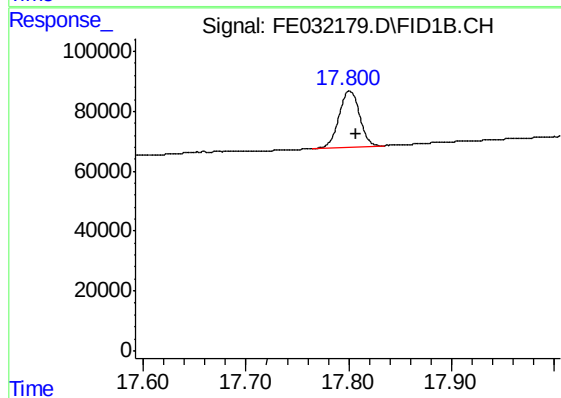


#13 N-TRIACONTANE

R.T.: 17.801 min  
Delta R.T.: -0.007 min  
Response: 261777  
Conc: 0.72 ug/ml

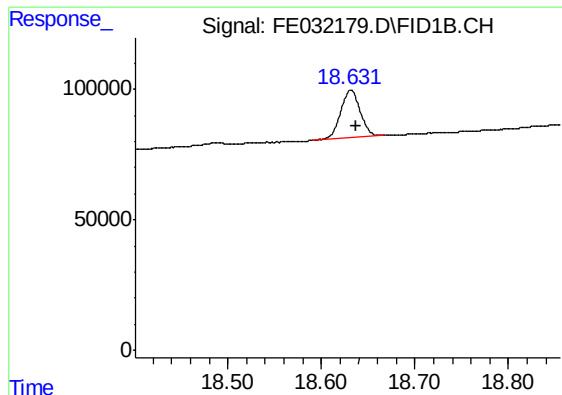

#14 N-DOTRIACONTANE

R.T.: 18.632 min  
Delta R.T.: -0.005 min  
Response: 264137  
Conc: 0.77 ug/ml

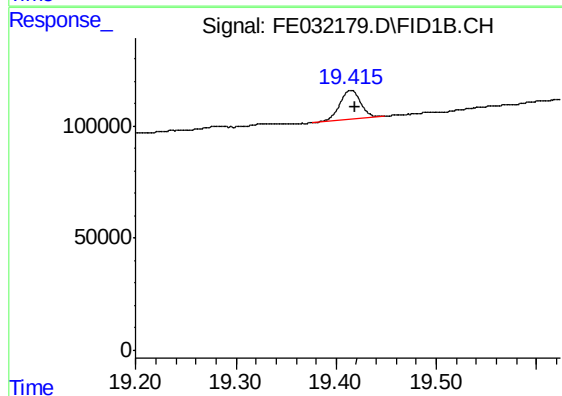

#15 N-TETRATRIACONTANE

R.T.: 19.415 min  
Delta R.T.: -0.004 min  
Response: 188714  
Conc: 0.66 ug/ml