

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061622AL\
 Data File : FE036095.D
 Signal(s) : FID1B.CH
 Acq On : 16 Jun 2022 13:59
 Operator : YP\AJ
 Sample : N3334-19DL2 100X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 16 14:50:32 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 060922.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 09 16:49:15 2022
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	10.849	145772	1.067 ug/ml
Spiked Amount 50.000		Recovery =	2.13%
12) S 1-chlorooctadecane (S...	12.304	118997	1.139 ug/ml
Spiked Amount 50.000		Recovery =	2.28%
Target Compounds			
3) T A~Naphthalene (C11.7)	5.296	59732	<MDL ug/ml
4) T n-Dodecane (C12)	5.722	30053	<MDL ug/ml
5) T A~2-methylnaphthalene...	6.325	46588	<MDL ug/ml
6) T n-Tetradecane (C14)	7.513	155481	1.244 ug/ml
7) T n-Hexadecane (C16)	9.113	61808	<MDL ug/ml
8) T n-Octadecane (C18)	10.551	80874	<MDL ug/ml
10) T n-Eicosane (C20)	11.862	81021	<MDL ug/ml
13) T n-Docosane (C22)	13.056	63941	<MDL ug/ml
14) T n-Tetracosane (C24)	14.166	157660	1.299 ug/ml
15) T n-Hexacosane (C26)	15.221	813655	6.699 ug/ml
16) T n-Octacosane (C28)	16.125	102892	<MDL ug/ml
19) T n-Tetratriacontane (C34)	18.649	105062	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061622AL\
Data File : FE036095.D
Signal(s) : FID1B.CH
Acq On : 16 Jun 2022 13:59
Operator : YP\AJ
Sample : N3334-19DL2 100X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 16 14:50:32 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 060922.M
Quant Title : GC Extractables
QLast Update : Thu Jun 09 16:49:15 2022
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

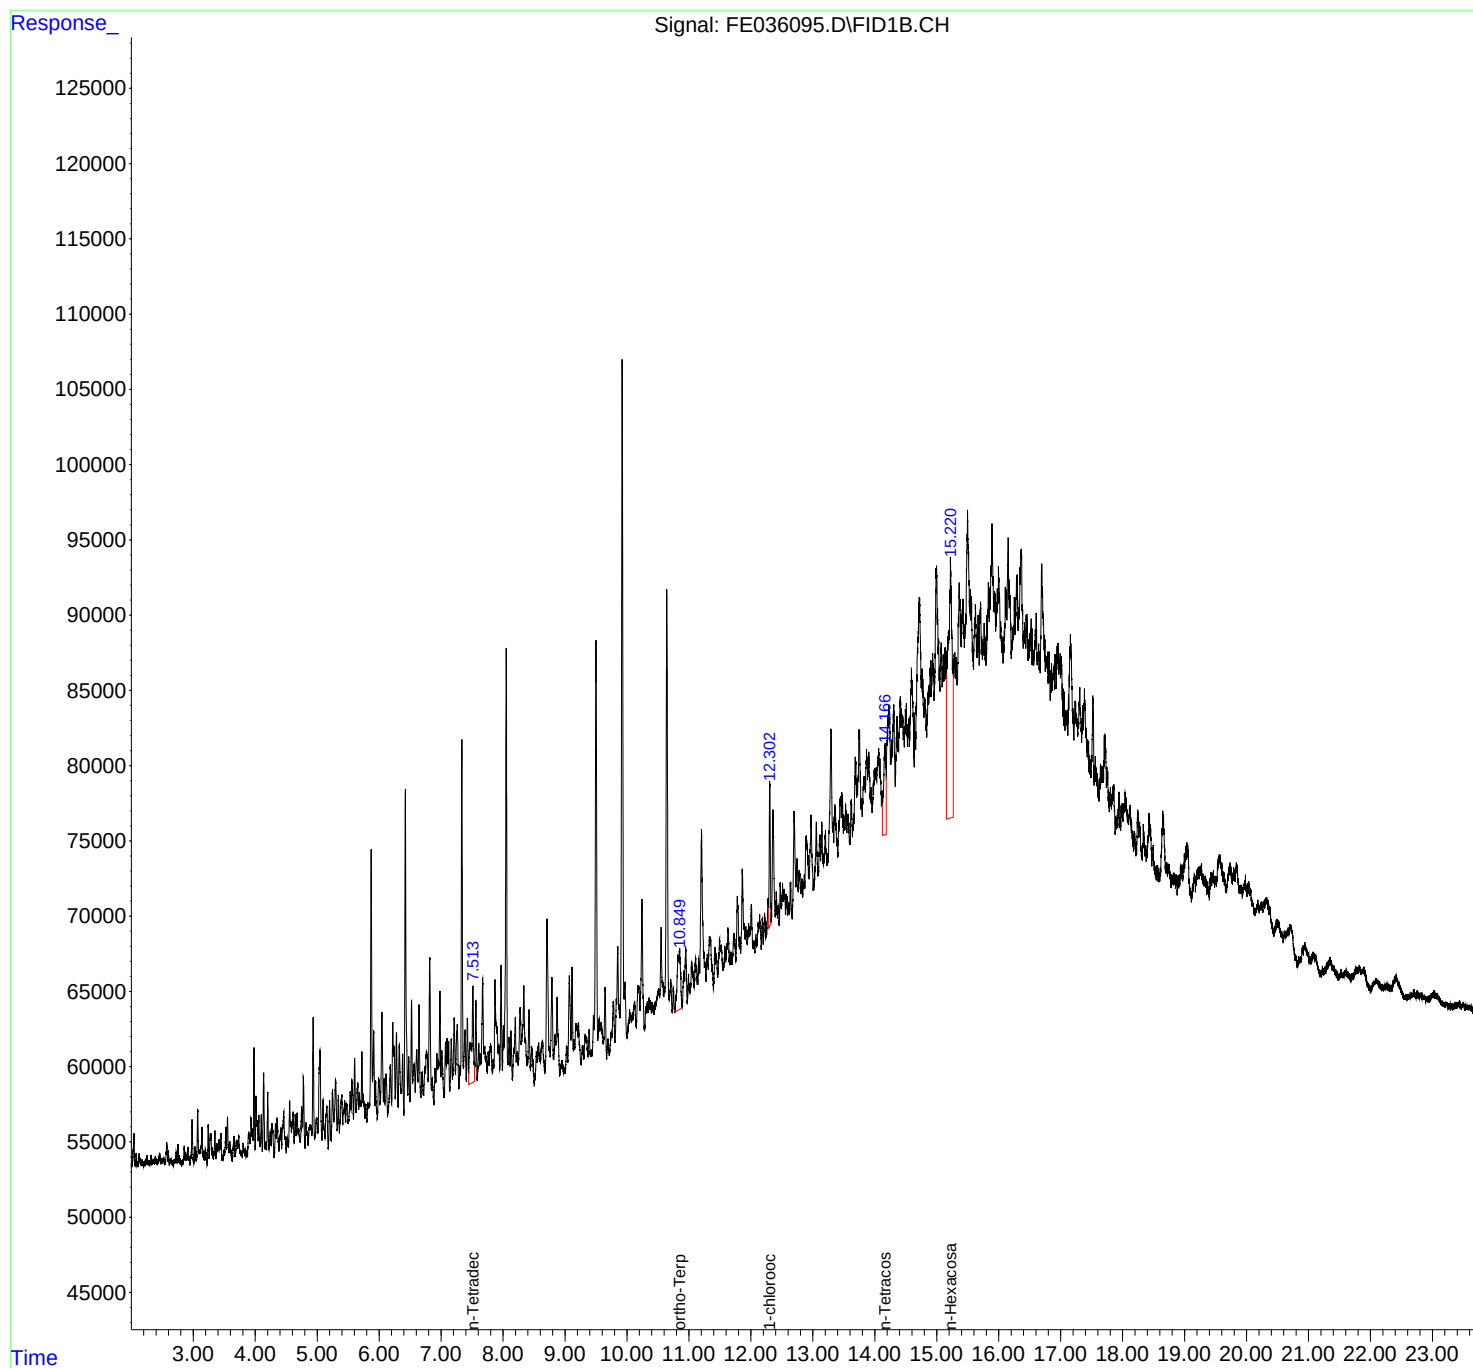


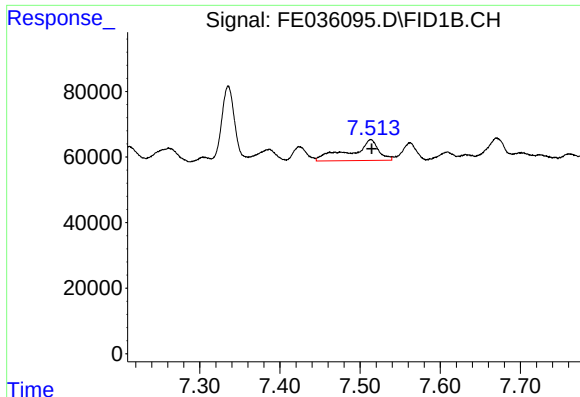

#6 n-Tetradecane (C14)


R.T.: 7.513 min
Delta R.T.: 0.000 min
Response: 155481
Conc: 1.24 ug/ml

Instrument :
FID_E
ClientSampleId :

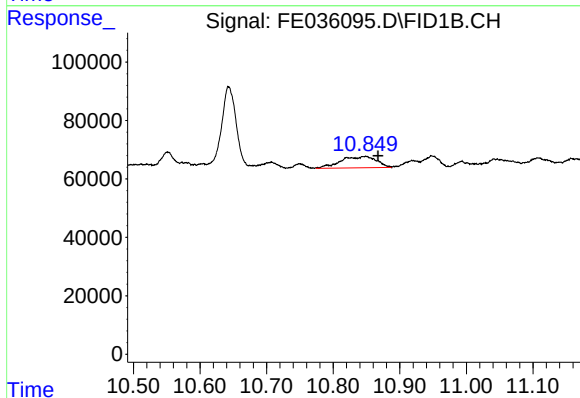


#9 ortho-Terphenyl (SURR)

R.T.: 10.849 min
Delta R.T.: -0.019 min
Response: 145772
Conc: 1.07 ug/ml

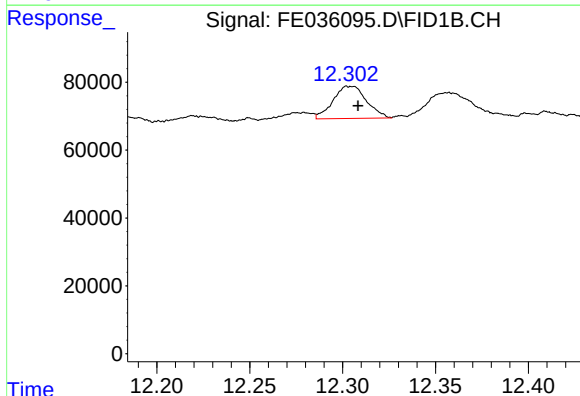


#12 1-chlorooctadecane (SURR)

R.T.: 12.304 min
Delta R.T.: -0.004 min
Response: 118997
Conc: 1.14 ug/ml

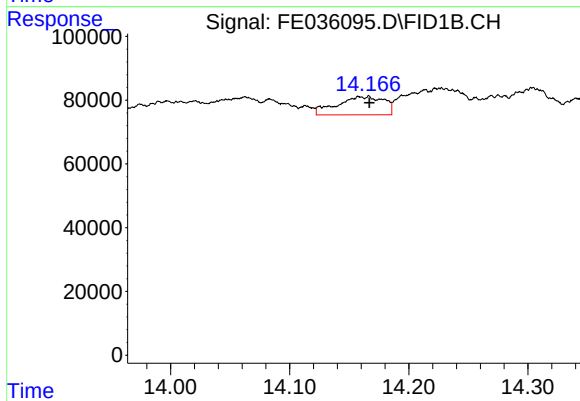

#14 n-Tetracosane (C24)

R.T.: 14.166 min
Delta R.T.: 0.000 min
Response: 157660
Conc: 1.30 ug/ml

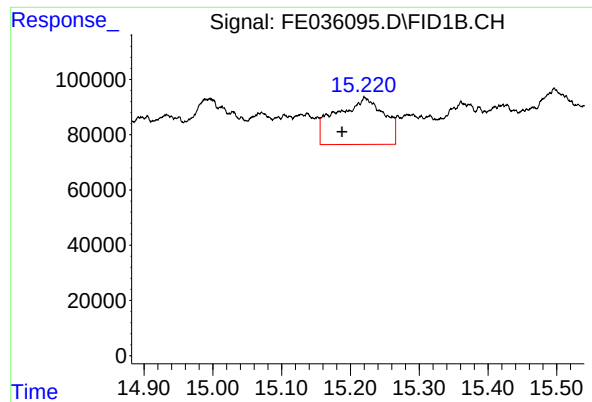

#15 n-Hexacosane (C26)

R.T.: 15.221 min
Delta R.T.: 0.033 min
Response: 813655
Conc: 6.70 ug/ml

Instrument :

FID_E

ClientSampleId :