

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061724AL\
Data File : FE048755.D
Signal(s) : FID1B.ch
Acq On : 18 Jun 2024 02:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 18 02:58:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.914	58280	0.429 ug/ml
19) T	n-Tetratriacontane (C34)	19.698	500901	3.662 ug/ml
22) T	n-Tetracontane (C40)	22.111	410484	2.998 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061724AL\
Data File : FE048755.D
Signal(s) : FID1B.ch
Acq On : 18 Jun 2024 02:20
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 18 02:58:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

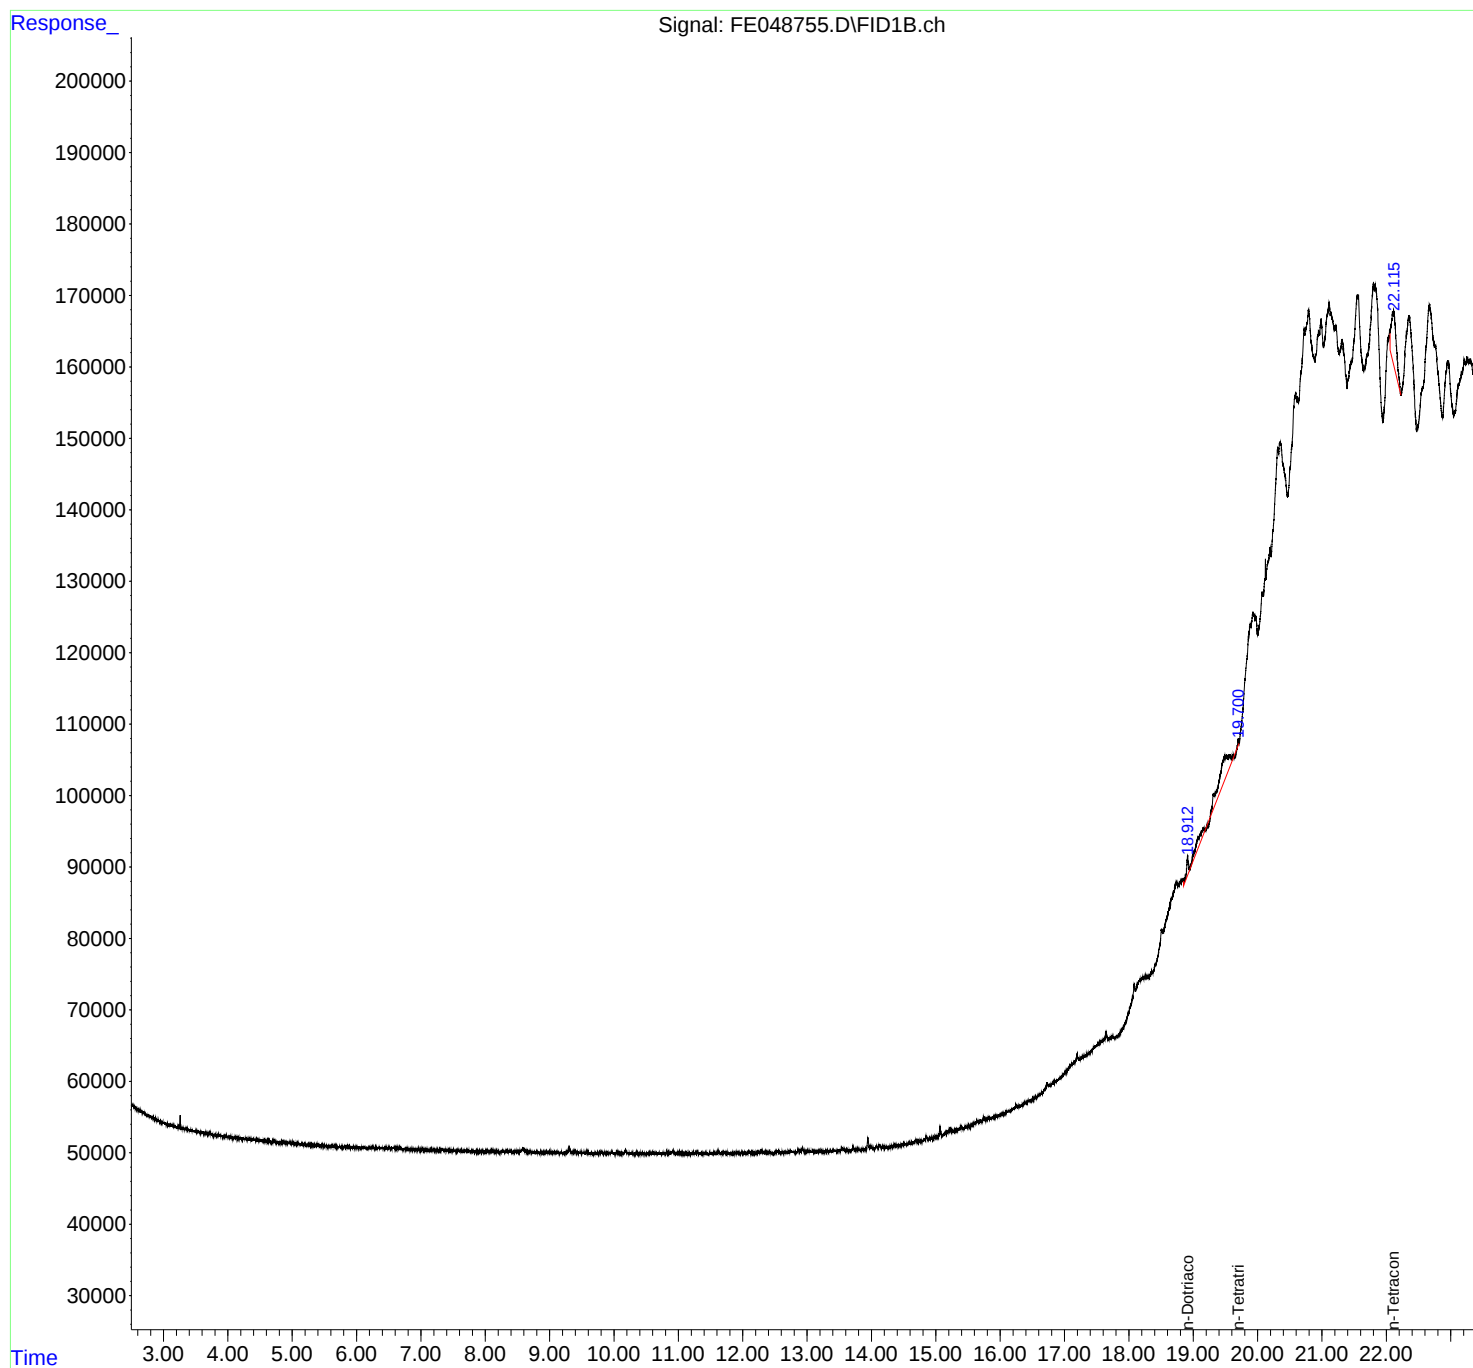


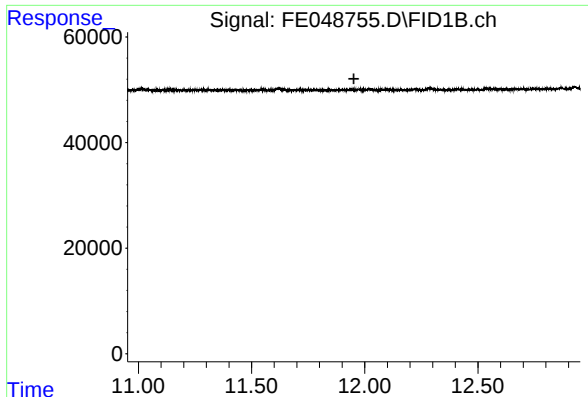

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.952 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

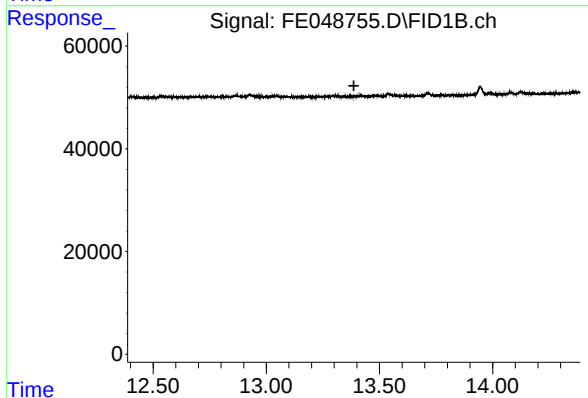


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.387 min
Response: 0
Conc: N.D.

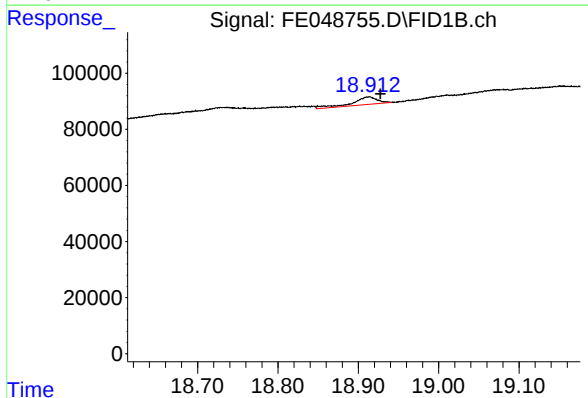


#18 n-Dotriacontane (C32)

R.T.: 18.914 min
Delta R.T.: -0.014 min
Response: 58280
Conc: 0.43 ug/ml

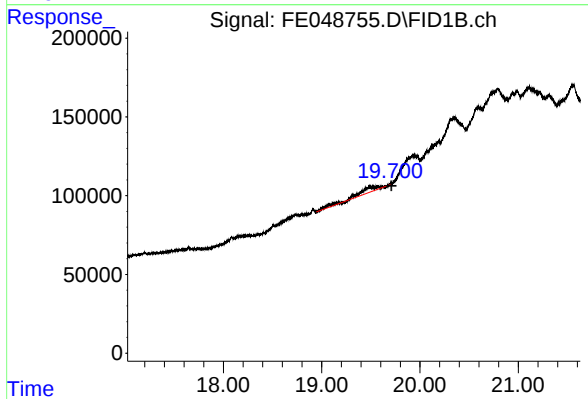

#19 n-Tetratriacontane (C34)

R.T.: 19.698 min
Delta R.T.: -0.013 min
Response: 500901
Conc: 3.66 ug/ml

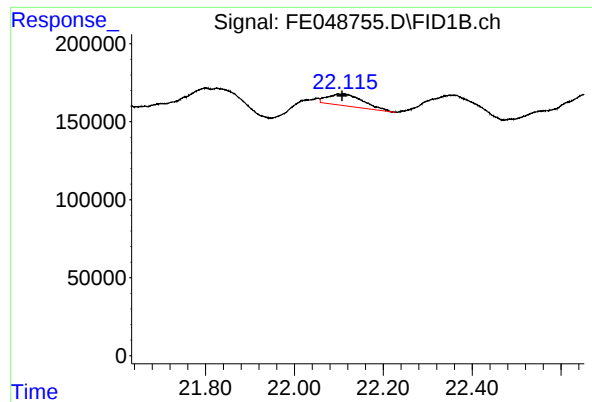

#22 n-Tetracontane (C40)

R.T.: 22.111 min
Delta R.T.: 0.003 min
Response: 410484
Conc: 3.00 ug/ml

Instrument :

FID_E

ClientSampleId :