

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061820\
 Data File : FE032205.D
 Signal(s) : FID1B.CH
 Acq On : 18 Jun 2020 16:11
 Operator : DD\AJ
 Sample : L2812-06 10X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 19 01:15:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
 Quant Title :
 QLast Update : Thu Jun 11 13:38:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.749	455444	1.424 ug/ml
Target Compounds			
4) N-TETRADECANE	8.269	157379	0.425 ug/ml
7) N-EICOSANE	12.722f	333017	0.897 ug/ml
10) N-TETRACOSANE	14.941	284214	0.766 ug/ml
11) N-HEXACOSANE	15.973	124730	0.341 ug/ml
12) N-OCTACOSANE	16.925	393451	1.077 ug/ml
13) N-TRIACONTANE	17.813	781100	2.146 ug/ml
14) N-DOTRIACONTANE	18.643	758238	2.214 ug/ml
15) N-TETRATRIACONTANE	19.429	586008	2.054 ug/ml
16) N-HEXATRIACONTANE	20.172	1151228	5.340 ug/ml
17) N-OCTATRIACONTANE	20.917	212854	1.245 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061820\
Data File : FE032205.D
Signal(s) : FID1B.CH
Acq On : 18 Jun 2020 16:11
Operator : DD\AJ
Sample : L2812-06 10X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 19 01:15:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
Quant Title :
QLast Update : Thu Jun 11 13:38:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

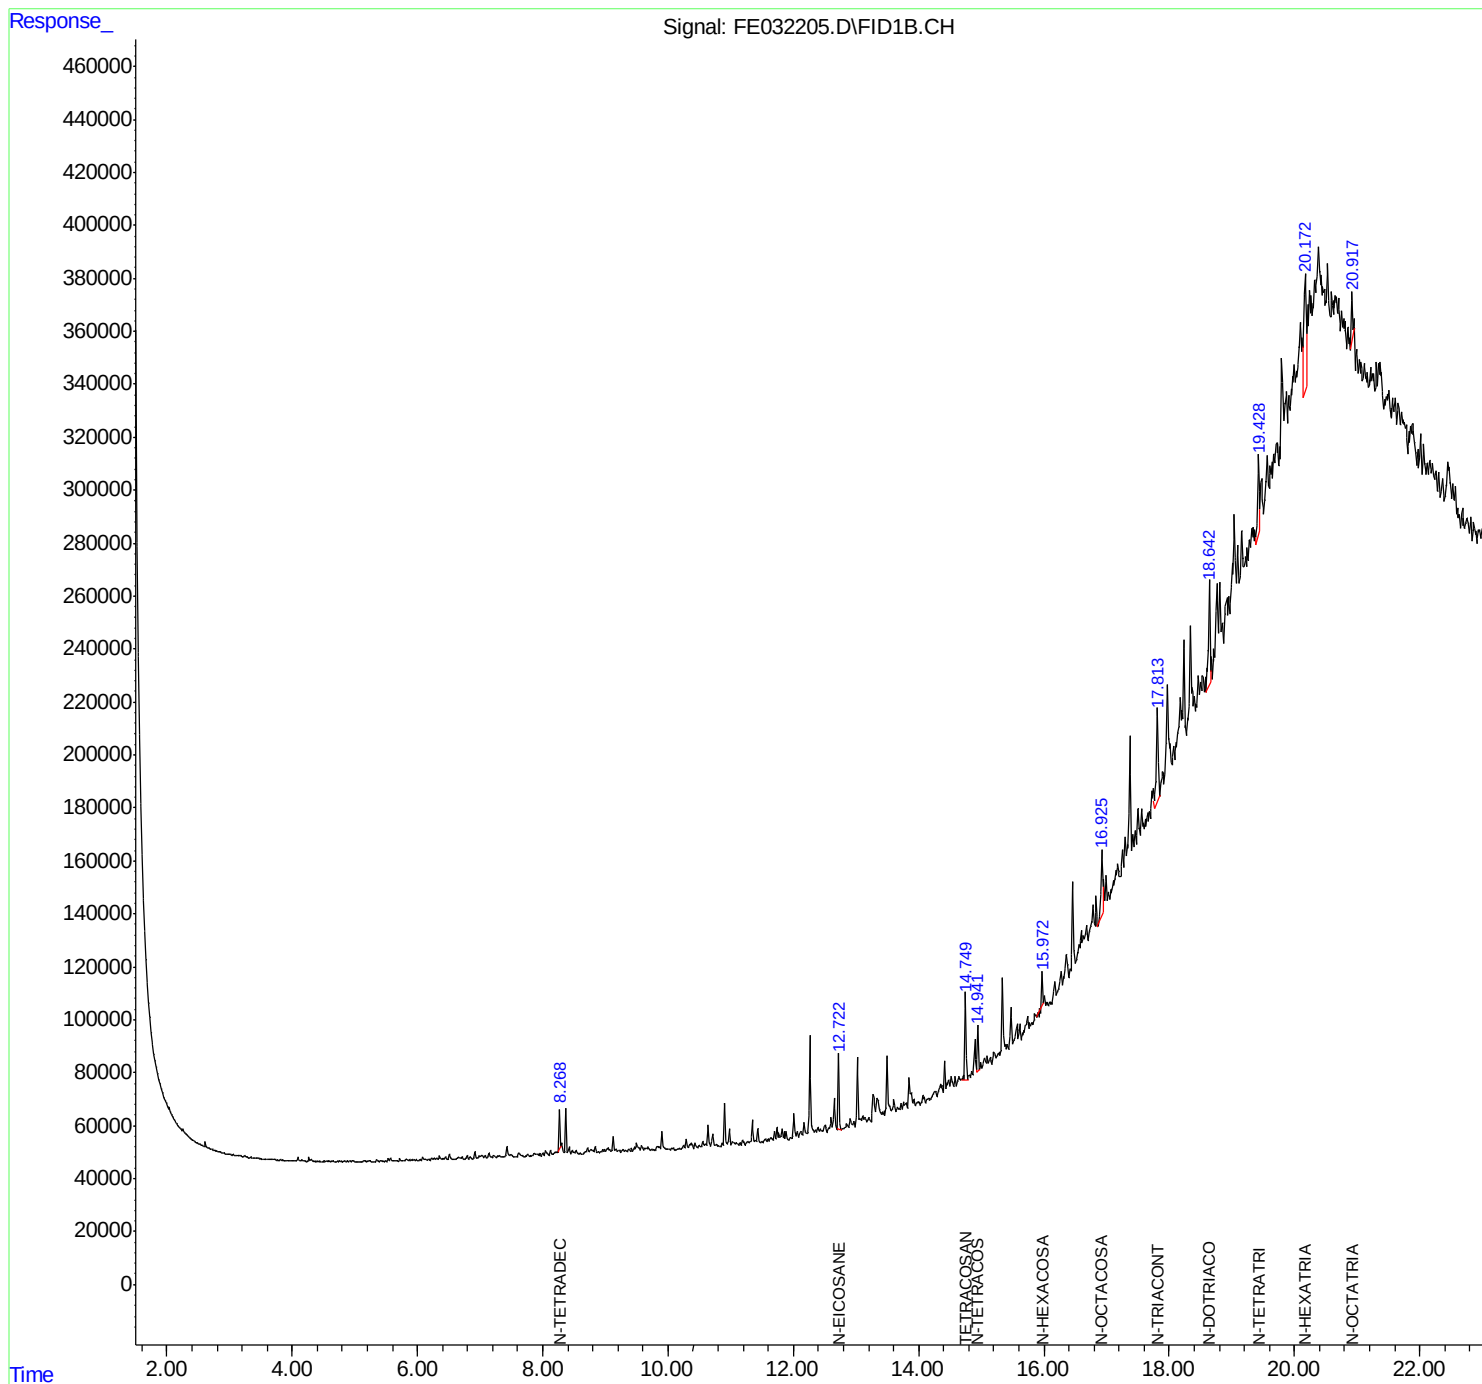

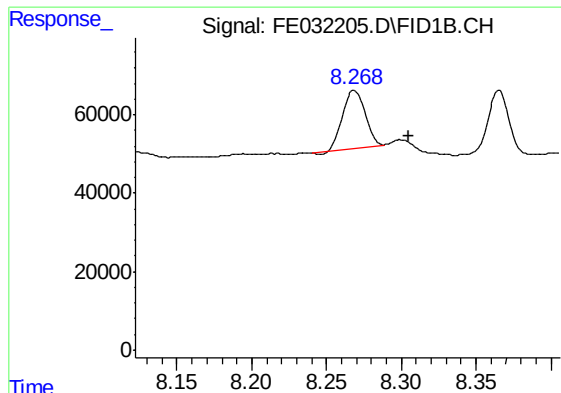


#4 N-TETRADECANE

R.T.: 8.269 min
Delta R.T.: -0.036 min
Response: 157379
Conc: 0.42 ug/ml

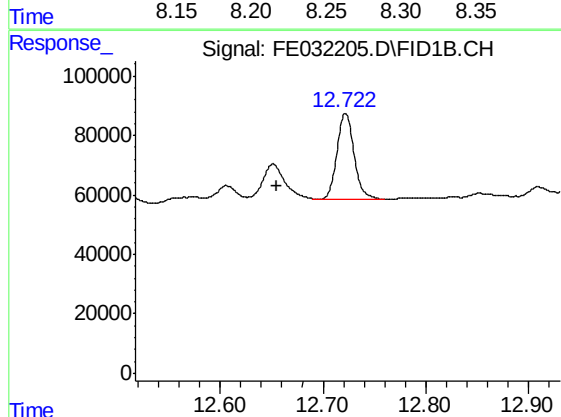


#7 N-EICOSANE

R.T.: 12.722 min
Delta R.T.: 0.067 min
Response: 333017
Conc: 0.90 ug/ml

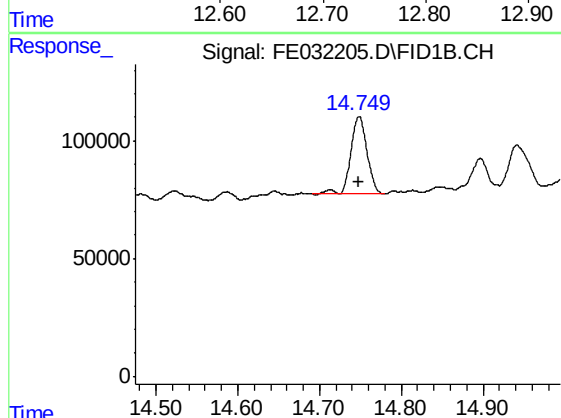


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.749 min
Delta R.T.: 0.000 min
Response: 455444
Conc: 1.42 ug/ml

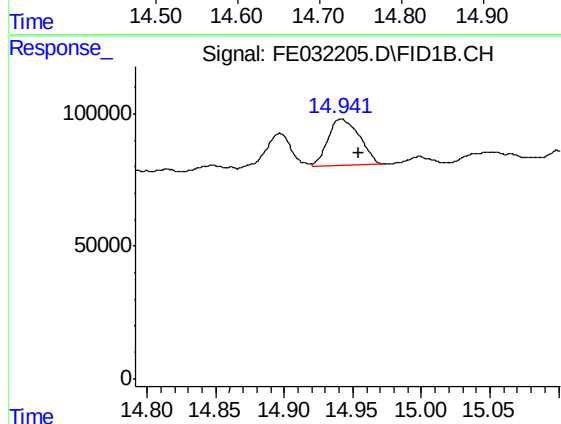


#10 N-TETRACOSANE

R.T.: 14.941 min
Delta R.T.: -0.013 min
Response: 284214
Conc: 0.77 ug/ml

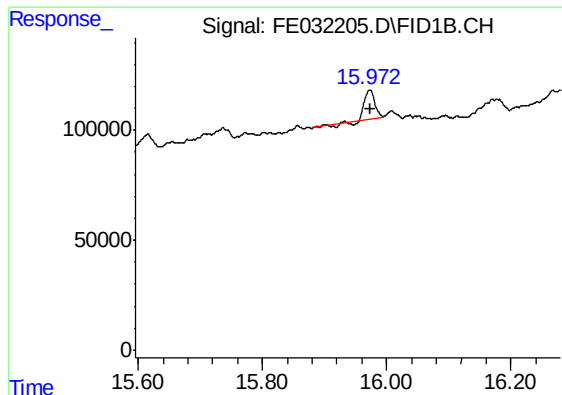


#11 N-HEXACOSANE

R.T.: 15.973 min
Delta R.T.: 0.000 min
Response: 124730
Conc: 0.34 ug/ml

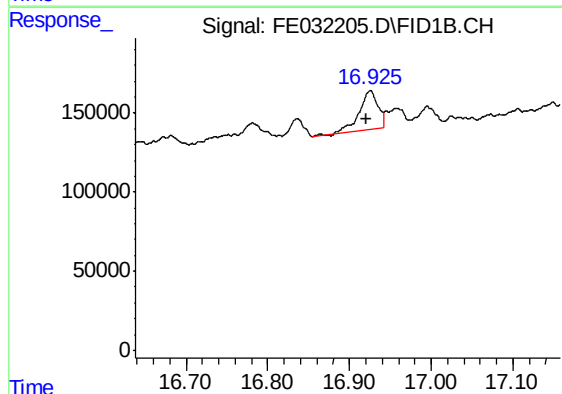


#12 N-OCTACOSANE

R.T.: 16.925 min
Delta R.T.: 0.004 min
Response: 393451
Conc: 1.08 ug/ml

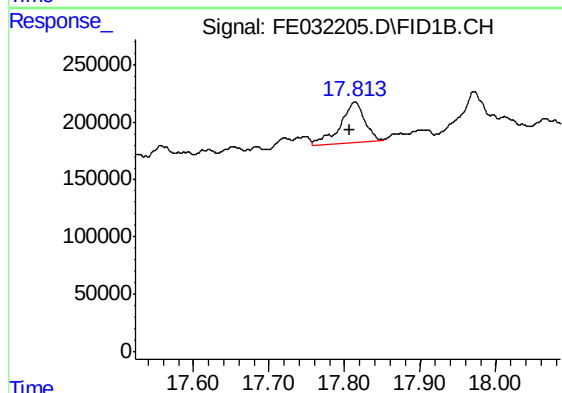


#13 N-TRIACONTANE

R.T.: 17.813 min
Delta R.T.: 0.006 min
Response: 781100
Conc: 2.15 ug/ml

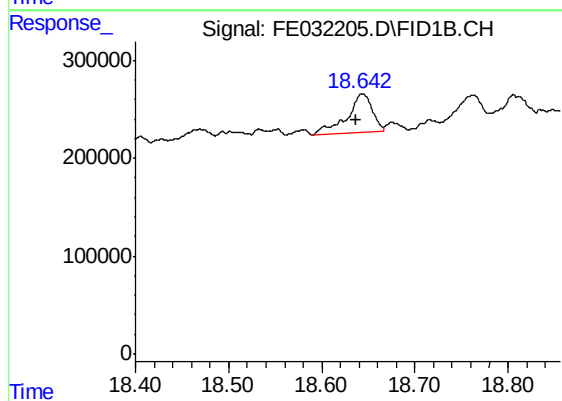


#14 N-DOTRIACONTANE

R.T.: 18.643 min
Delta R.T.: 0.006 min
Response: 758238
Conc: 2.21 ug/ml

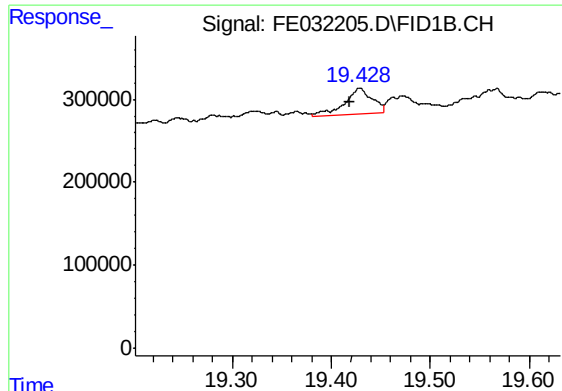


#15 N-TETRATRIACONTANE

R.T.: 19.429 min
Delta R.T.: 0.009 min
Response: 586008
Conc: 2.05 ug/ml

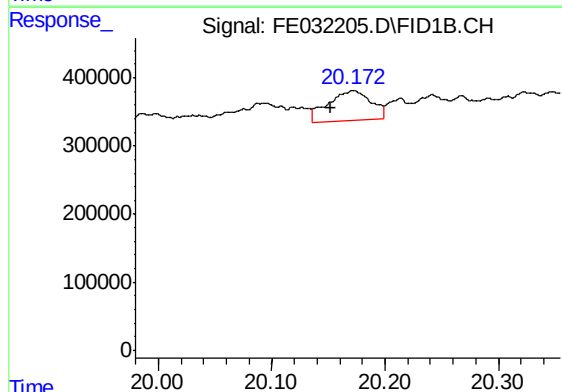

#16 N-HEXATRIACONTANE

R.T.: 20.172 min
Delta R.T.: 0.020 min
Response: 1151228
Conc: 5.34 ug/ml

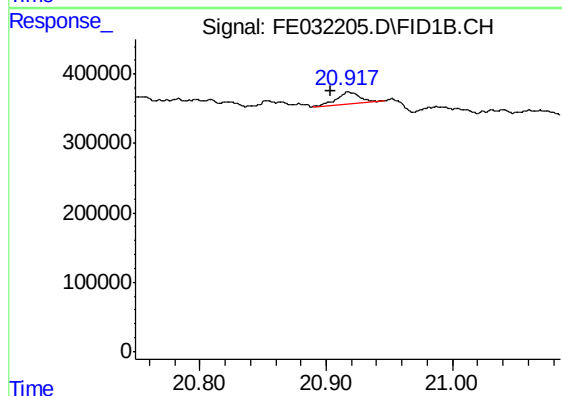

#17 N-OCTATRIACONTANE

R.T.: 20.917 min
Delta R.T.: 0.014 min
Response: 212854
Conc: 1.25 ug/ml