

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061923AL\
 Data File : FE042692.D
 Signal(s) : FID1B.ch
 Acq On : 19 Jun 2023 08:25
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 20 01:52:45 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 061723.M
 Quant Title : GC Extractables
 QLast Update : Mon Jun 19 02:33:05 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
13) T n-Docosane (C22)	14.100	301998	1.873 ug/ml
14) T n-Tetracosane (C24)	15.215	263863	1.670 ug/ml
15) T n-Hexacosane (C26)	16.240	221708	1.467 ug/ml
16) T n-Octacosane (C28)	17.192	185982	1.299 ug/ml
17) T n-Tricontane (C30)	18.081	137667	0.976 ug/ml
18) T n-Dotriacontane (C32)	18.914	241386	1.773 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061923AL\
Data File : FE042692.D
Signal(s) : FID1B.ch
Acq On : 19 Jun 2023 08:25
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 01:52:45 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 061723.M
Quant Title : GC Extractables
QLast Update : Mon Jun 19 02:33:05 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

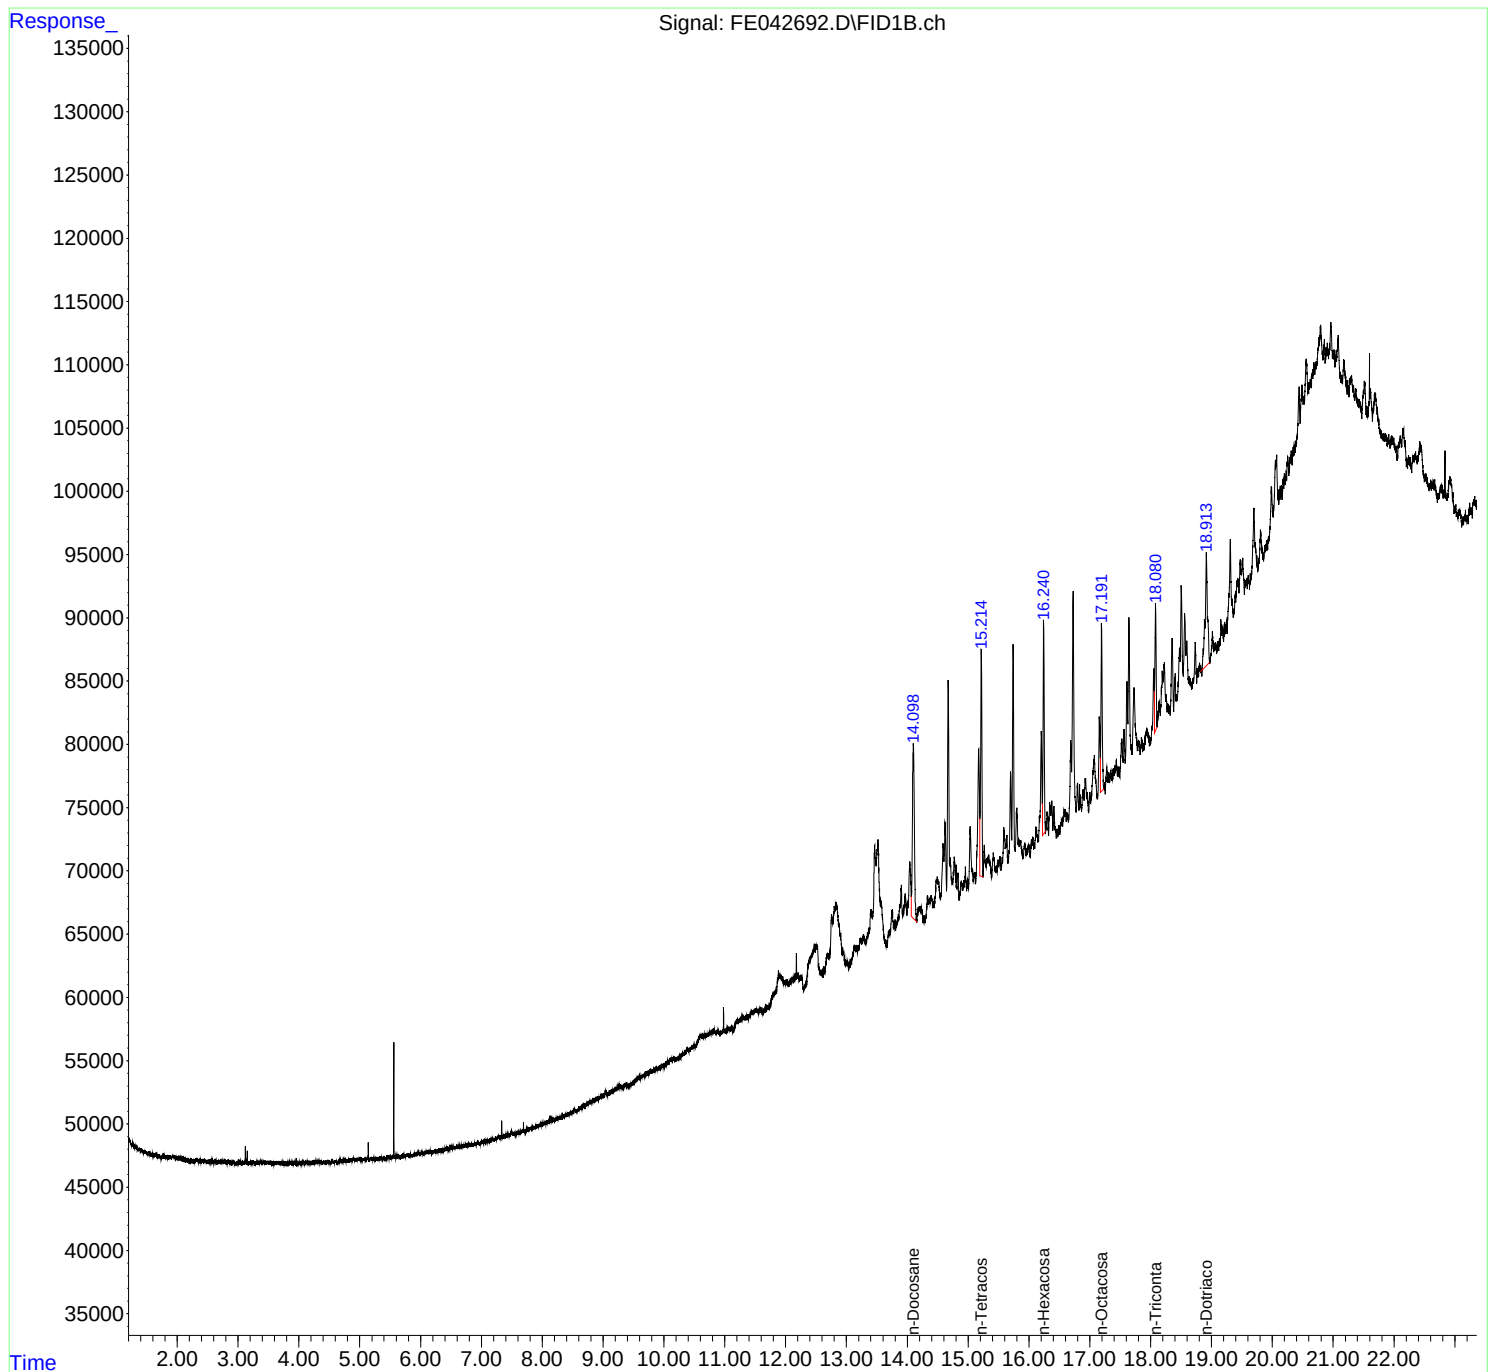


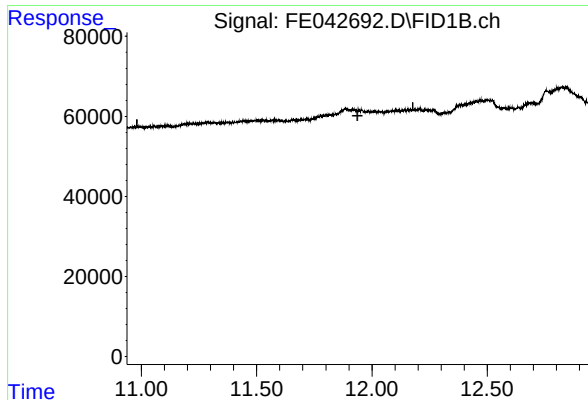

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.937 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

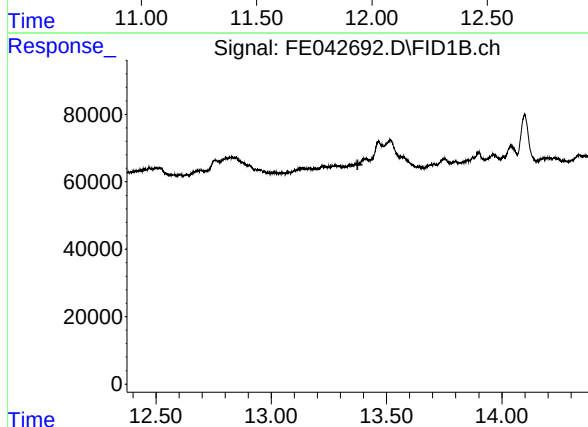


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.374 min
Response: 0
Conc: N.D.

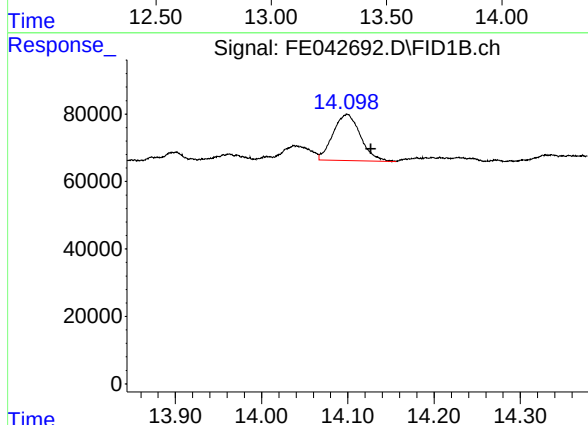


#13 n-Docosane (C22)

R.T.: 14.100 min
Delta R.T.: -0.027 min
Response: 301998
Conc: 1.87 ug/ml

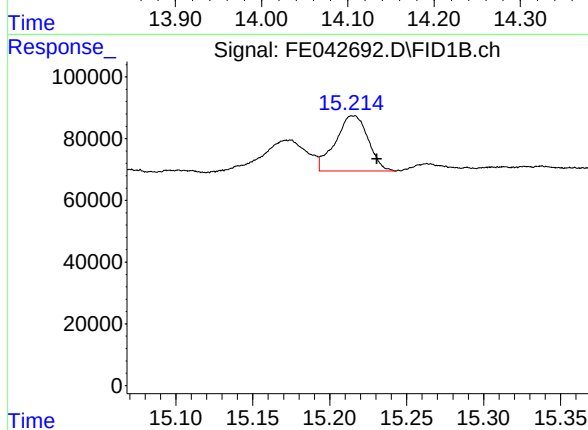

#14 n-Tetracosane (C24)


R.T.: 15.215 min
Delta R.T.: -0.016 min
Response: 263863
Conc: 1.67 ug/ml

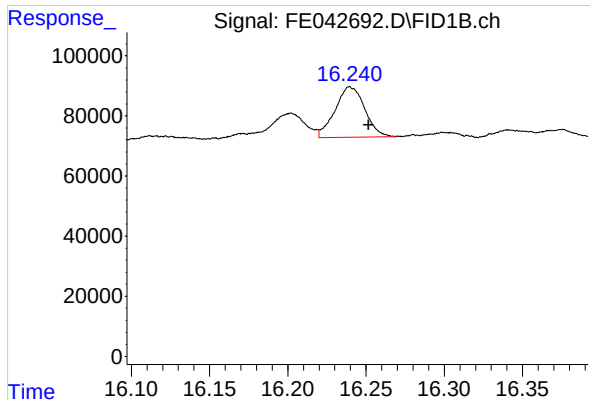

#15 n-Hexacosane (C26)


R.T.: 16.240 min
Delta R.T.: -0.012 min
Response: 221708
Conc: 1.47 ug/ml

Instrument :
FID_E
ClientSampleId :

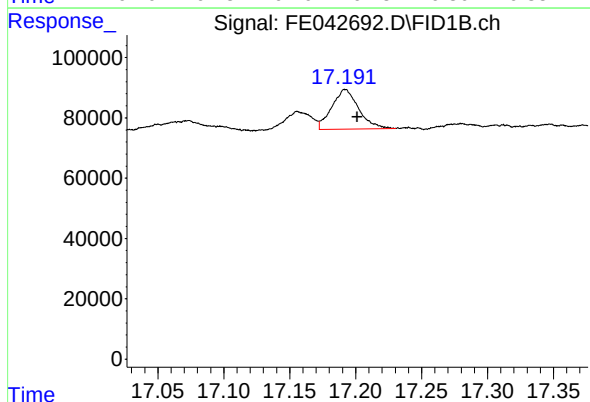


#16 n-Octacosane (C28)

R.T.: 17.192 min
Delta R.T.: -0.009 min
Response: 185982
Conc: 1.30 ug/ml

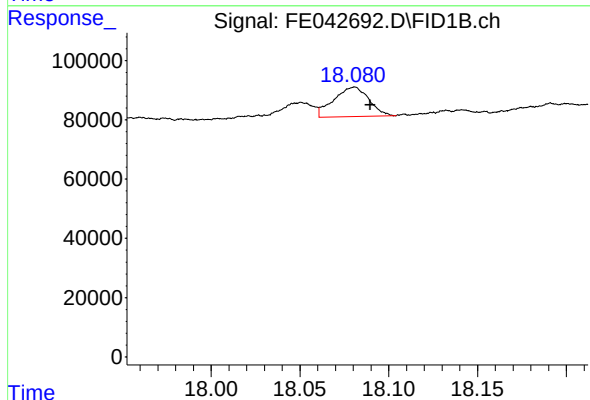

#17 n-Tricontane (C30)

R.T.: 18.081 min
Delta R.T.: -0.009 min
Response: 137667
Conc: 0.98 ug/ml

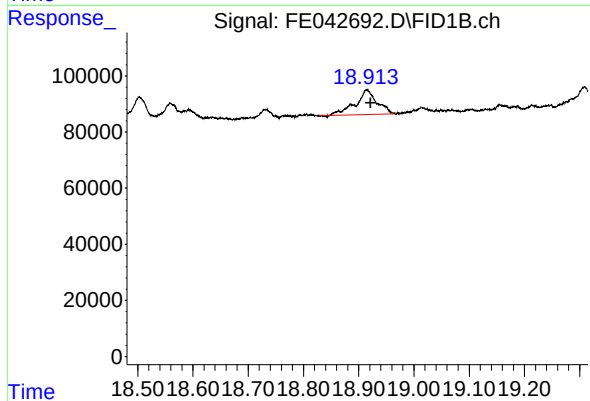

#18 n-Dotriacontane (C32)

R.T.: 18.914 min
Delta R.T.: -0.008 min
Response: 241386
Conc: 1.77 ug/ml