

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061924AL\
Data File : FE048800.D
Signal(s) : FID1B.ch
Acq On : 19 Jun 2024 22:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 01:30:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.909	44072	0.325 ug/ml
19) T	n-Tetratriacontane (C34)	19.774f	154884	1.132 ug/ml
22) T	n-Tetracontane (C40)	22.129	106284	0.776 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE061924AL\
Data File : FE048800.D
Signal(s) : FID1B.ch
Acq On : 19 Jun 2024 22:44
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 20 01:30:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 052524.M
Quant Title : GC Extractables
QLast Update : Fri May 24 16:28:51 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

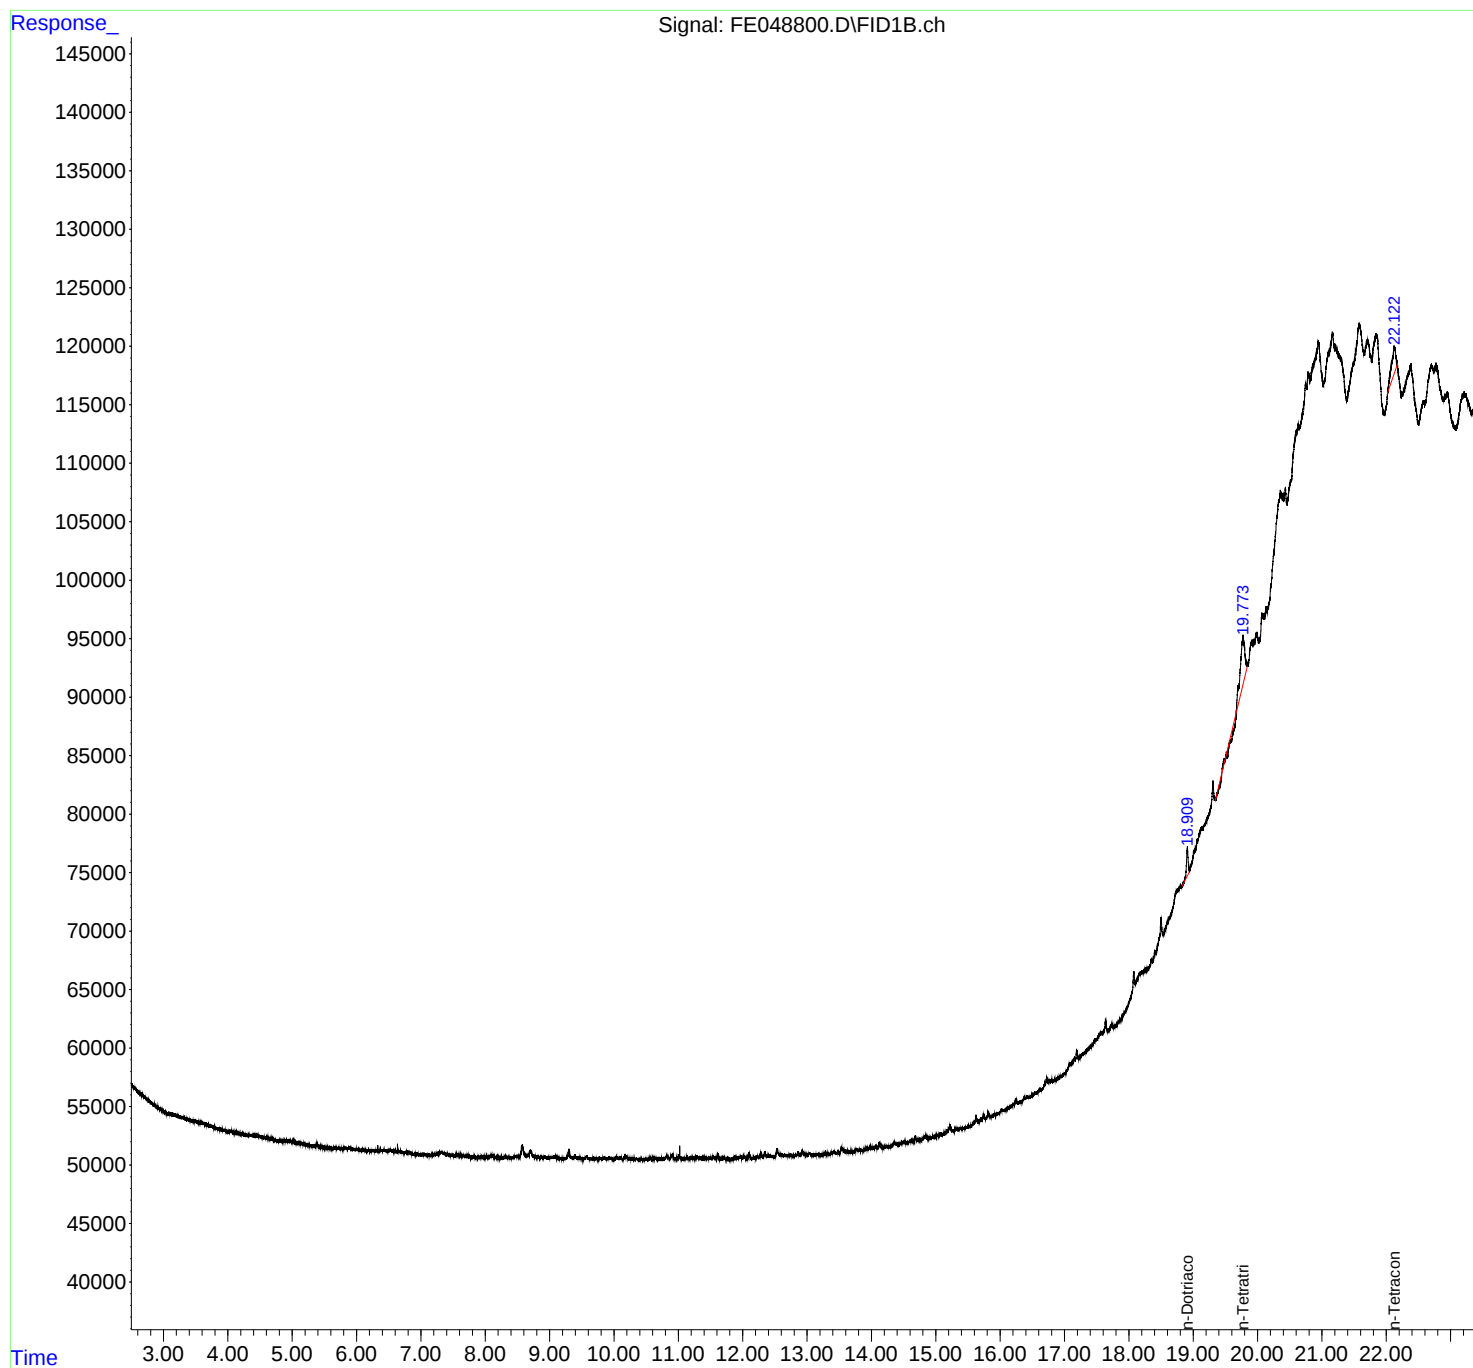


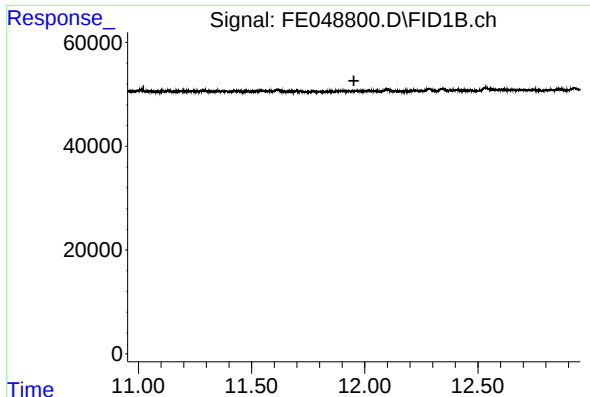

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T. : 11.952 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

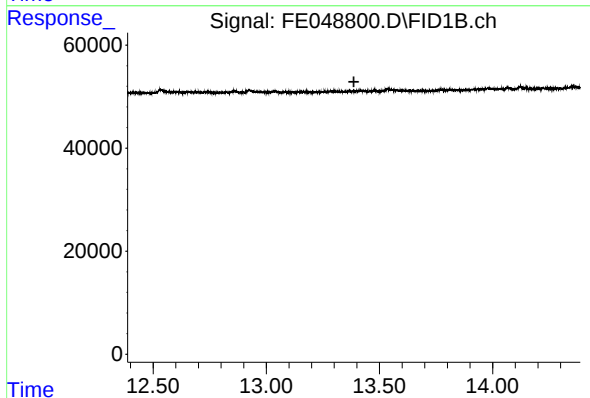


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T. : 13.387 min
Response: 0
Conc: N.D.

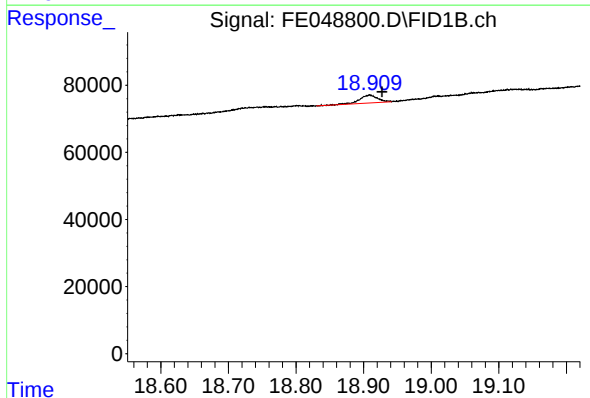


#18 n-Dotriacontane (C32)

R.T.: 18.909 min
Delta R.T.: -0.018 min
Response: 44072
Conc: 0.32 ug/ml

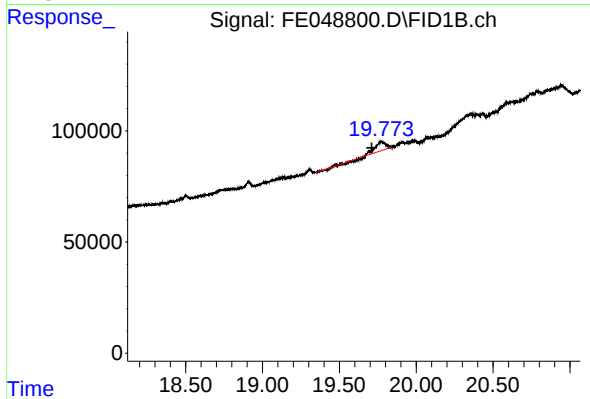

#19 n-Tetratriacontane (C34)

R.T.: 19.774 min
Delta R.T.: 0.063 min
Response: 154884
Conc: 1.13 ug/ml

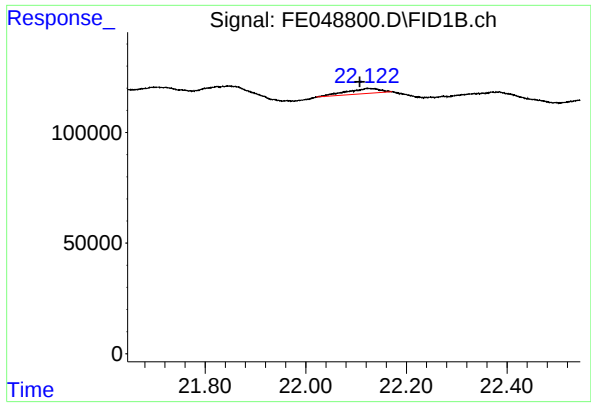

#22 n-Tetracontane (C40)

R.T.: 22.129 min
Delta R.T.: 0.021 min
Response: 106284
Conc: 0.78 ug/ml

Instrument :

FID_E

ClientSampleId :