

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062019\
Data File : FE030110.D
Signal(s) : FID1B.CH
Acq On : 20 Jun 2019 8:15
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 20 11:41:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062019.M
Quant Title :
QLast Update : Thu Jun 20 11:40:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
12)	N-DOTRIACONTANE	18.518	62995	0.337 ug/ml
14)	N-HEXATRIACONTANE	20.072	70446	0.411 ug/ml
15)	N-TETRACONTANE	21.668	182482	1.259 ug/ml
16)	N-TETRTETRACOOCTANE	24.294	279077	2.406 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062019\
Data File : FE030110.D
Signal(s) : FID1B.CH
Acq On : 20 Jun 2019 8:15
Operator : AJ\SJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 20 11:41:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062019.M
Quant Title :
QLast Update : Thu Jun 20 11:40:42 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 uL
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

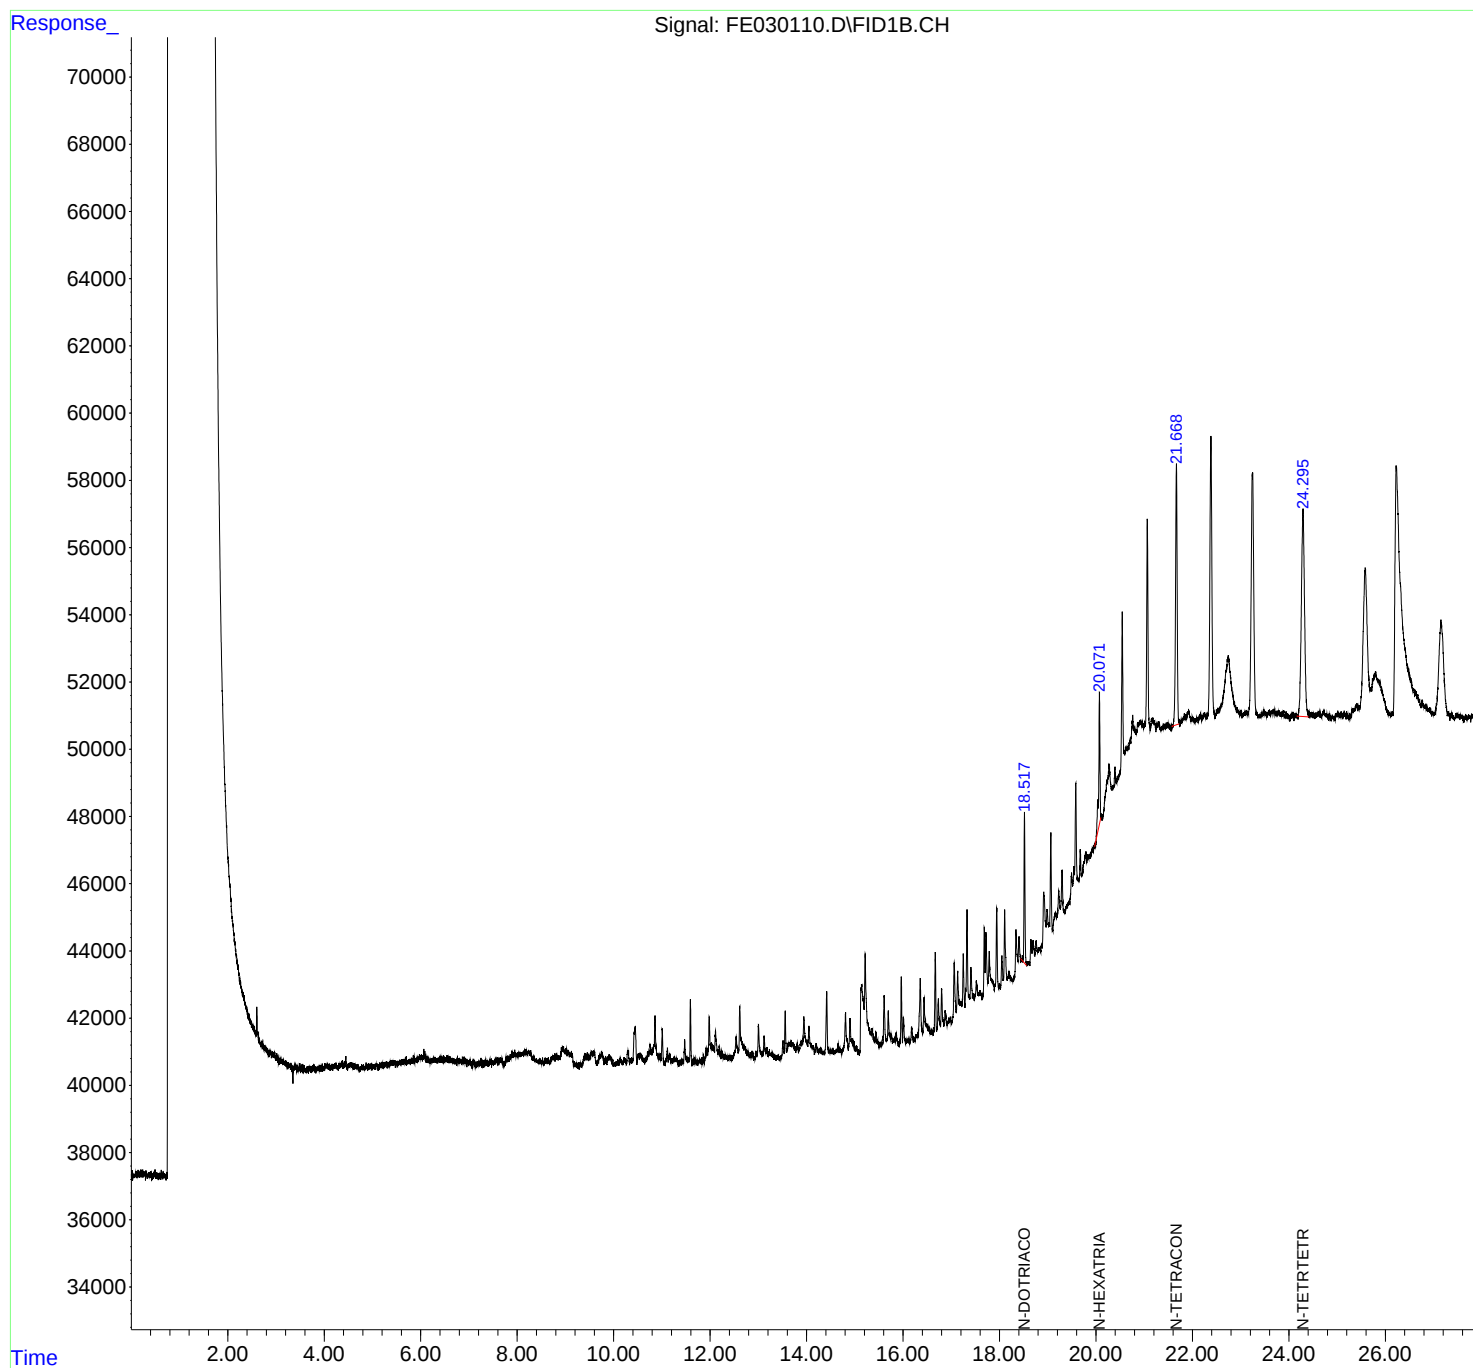

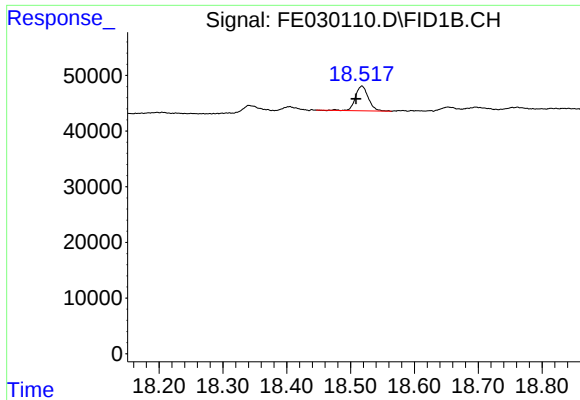


#12 N-DOTRIACONTANE

R.T.: 18.518 min
Delta R.T.: 0.009 min
Response: 62995
Conc: 0.34 ug/ml

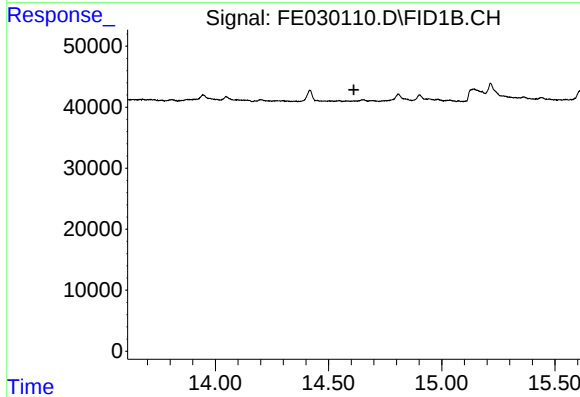


#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.612 min
Response: 0
Conc: N.D.

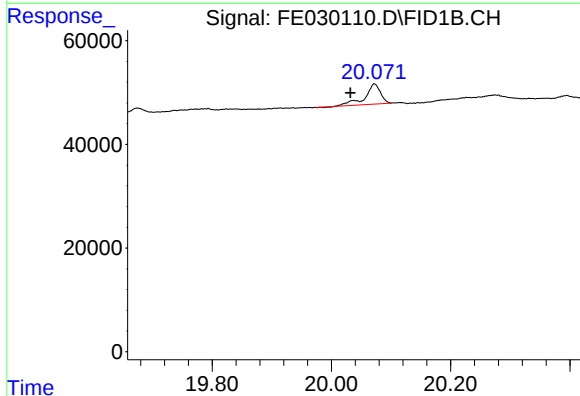


#14 N-HEXATRIACONTANE

R.T.: 20.072 min
Delta R.T.: 0.040 min
Response: 70446
Conc: 0.41 ug/ml

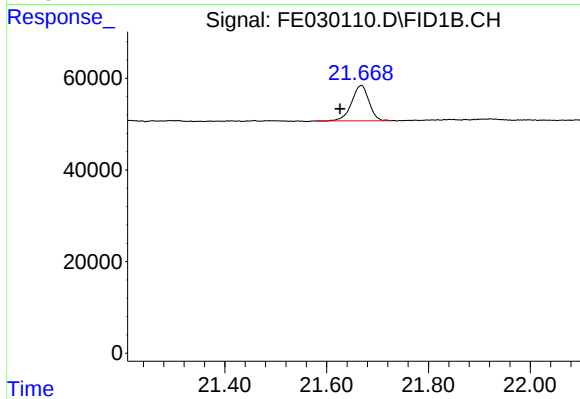

#15 N-TETRACONTANE

R.T.: 21.668 min
Delta R.T.: 0.042 min
Response: 182482
Conc: 1.26 ug/ml

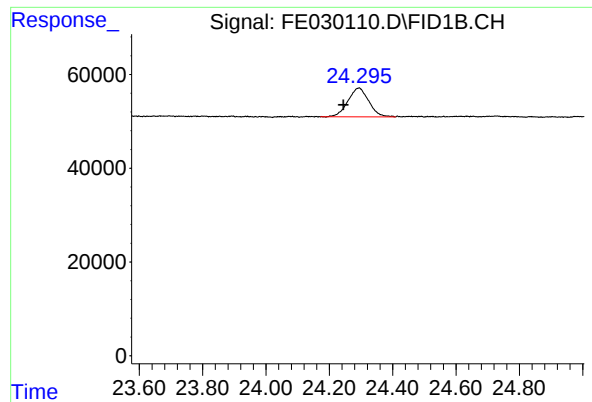

#16 N-TETRTETRACOCTANE

R.T.: 24.294 min

Delta R.T.: 0.049 min

Response: 279077

Conc: 2.41 ug/ml