

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062122\
Data File : FE036140.D
Signal(s) : FID1B.ch
Acq On : 21 Jun 2022 16:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 22 08:59:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.962	2794820	19.326 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062122\
Data File : FE036140.D
Signal(s) : FID1B.ch
Acq On : 21 Jun 2022 16:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Jun 22 08:59:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

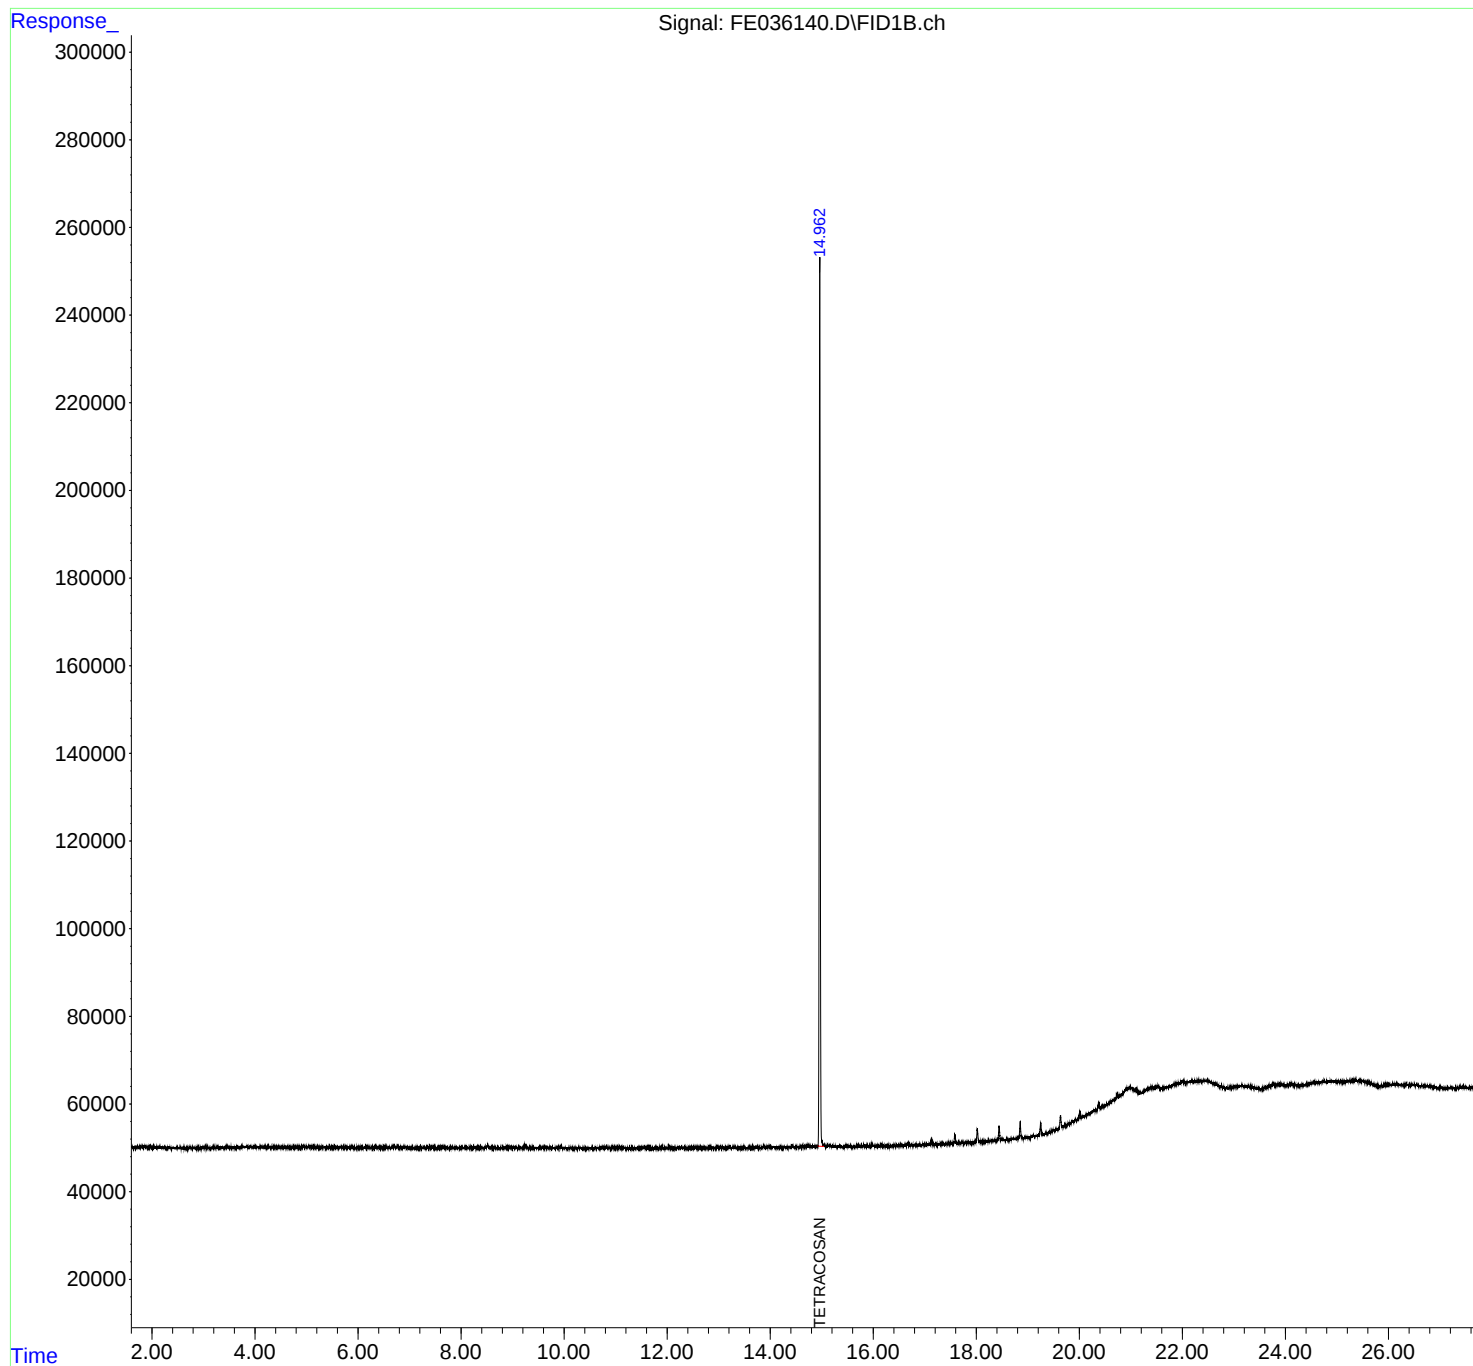

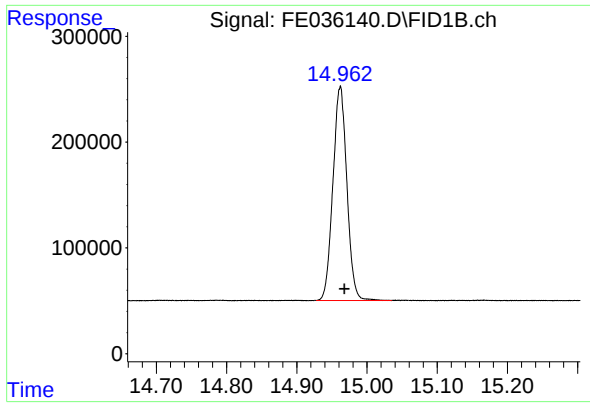

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.962 min
Delta R.T.: -0.006 min
Response: 2794820
Conc: 19.33 ug/ml

Instrument :
FID_E
ClientSampleId :
I.BLK