

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062124AL\
 Data File : FE048822.D
 Signal(s) : FID1B.ch
 Acq On : 20 Jun 2024 18:59
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 21 07:49:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 20 17:53:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

17) T	n-Tricontane (C30)	18.074	124229	0.849 ug/ml
18) T	n-Dotriacontane (C32)	18.906	243678	1.704 ug/ml
19) T	n-Tetratriacontane (C34)	19.687	230448	1.665 ug/ml
20) T	n-Hexatriacontane (C36)	20.426	201419	1.550 ug/ml
21) T	n-Octatriacontane (C38)	21.161	171120	1.335 ug/ml
22) T	n-Tetracontane (C40)	22.071	72464	0.592 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062124AL\
Data File : FE048822.D
Signal(s) : FID1B.ch
Acq On : 20 Jun 2024 18:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 21 07:49:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
Quant Title : GC Extractables
QLast Update : Thu Jun 20 17:53:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

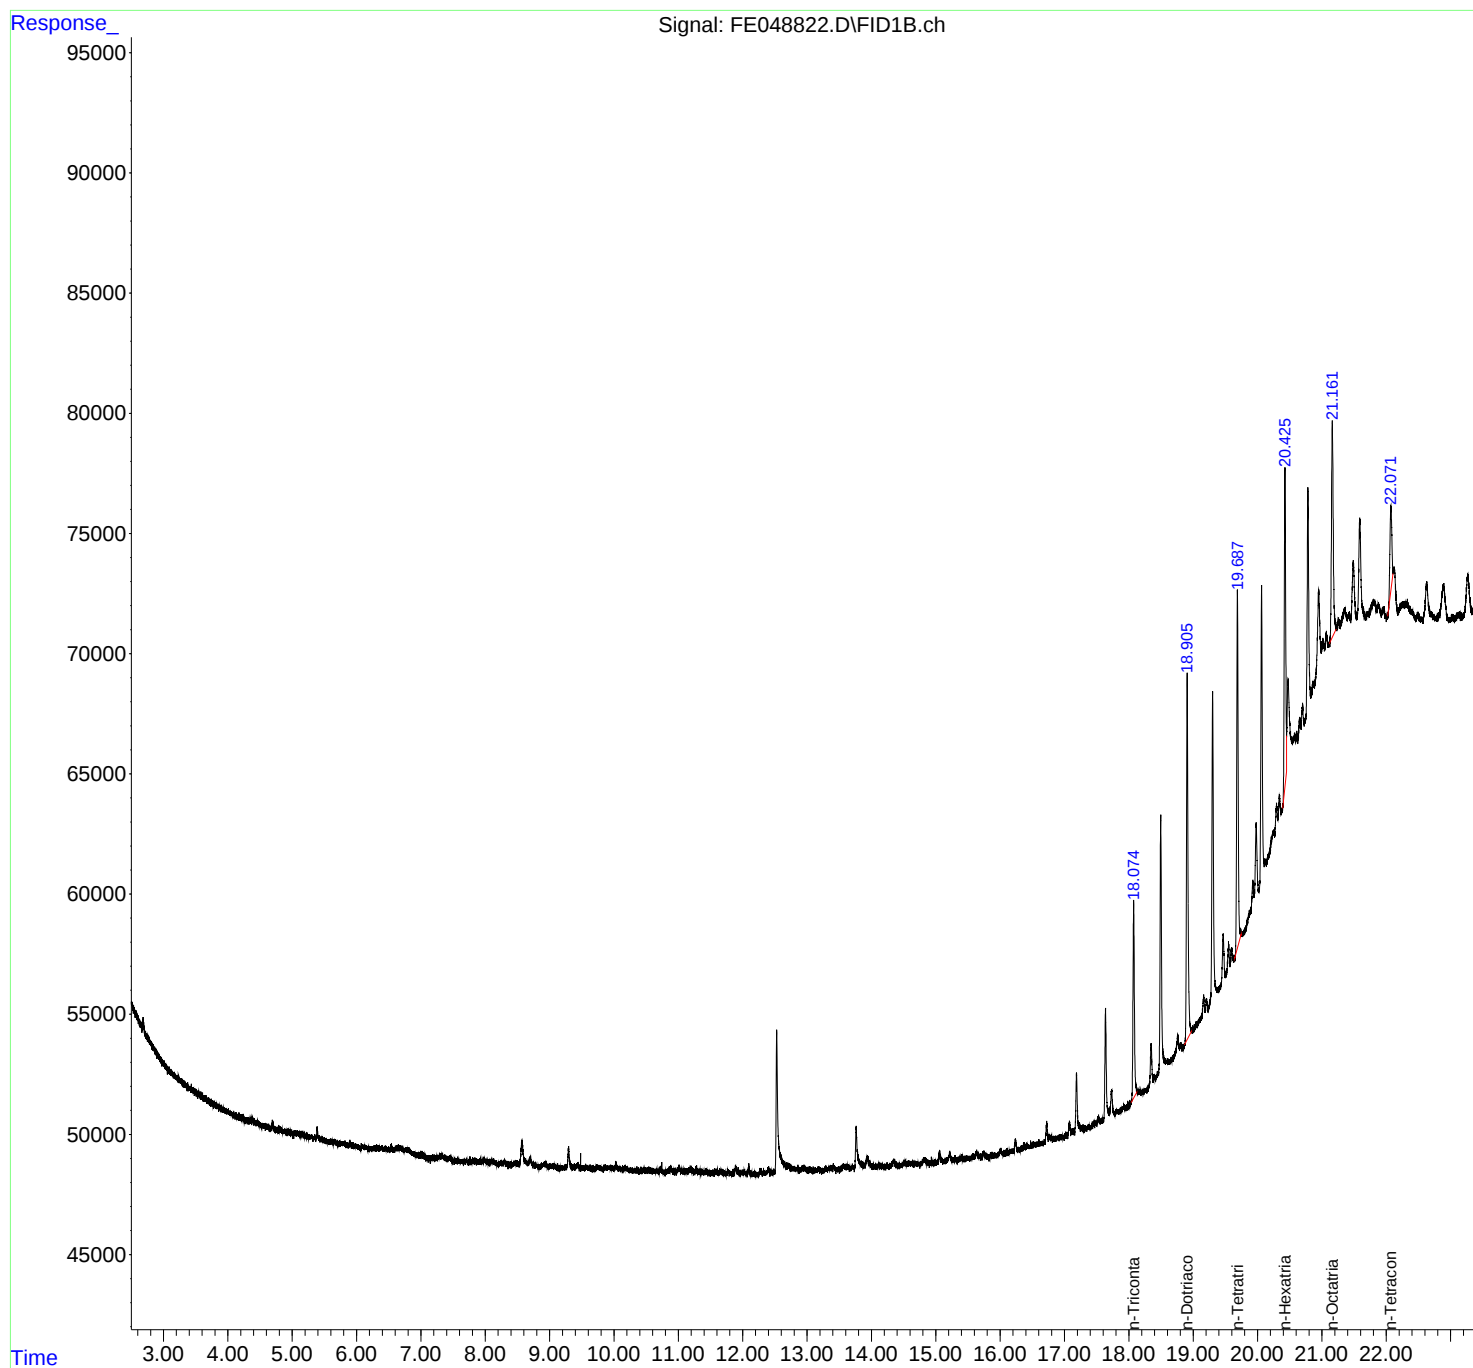


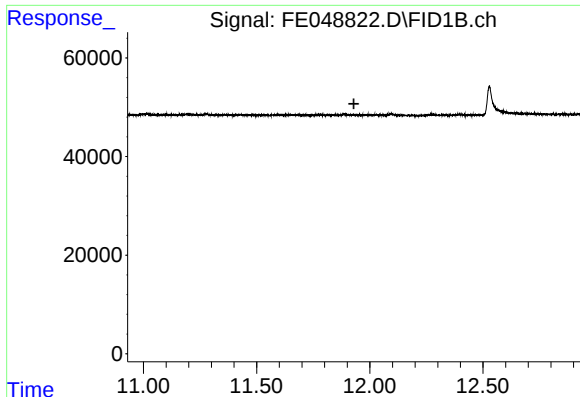

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.930 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

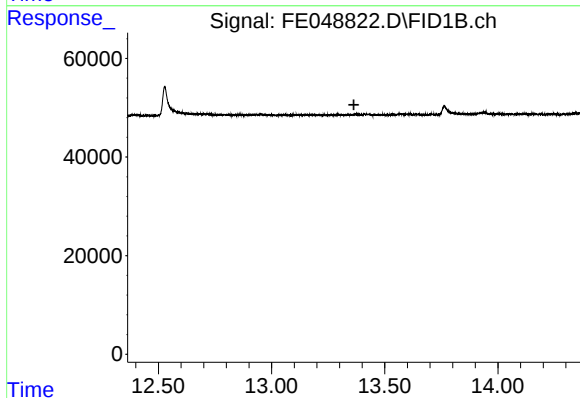


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.364 min
Response: 0
Conc: N.D.

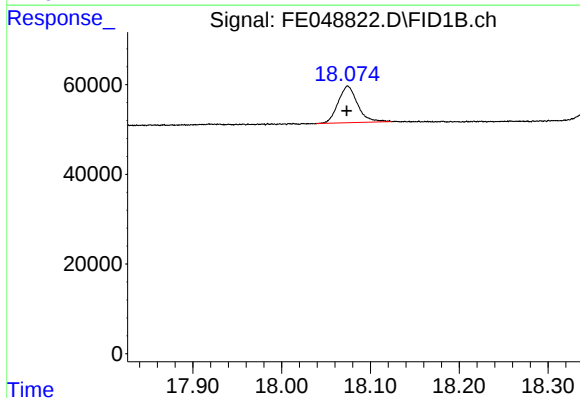


#17 n-Tricontane (C30)

R.T.: 18.074 min
Delta R.T.: 0.001 min
Response: 124229
Conc: 0.85 ug/ml

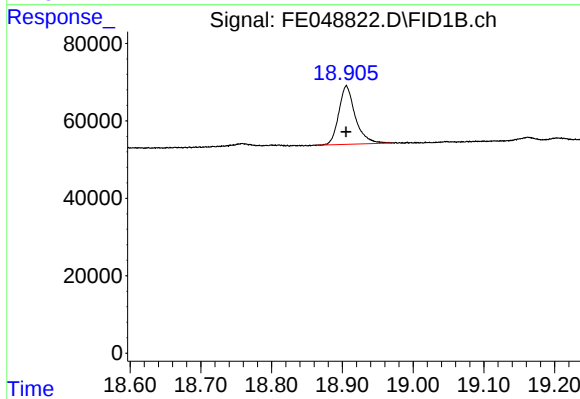

#18 n-Dotriacontane (C32)


R.T.: 18.906 min
Delta R.T.: 0.000 min
Response: 243678
Conc: 1.70 ug/ml

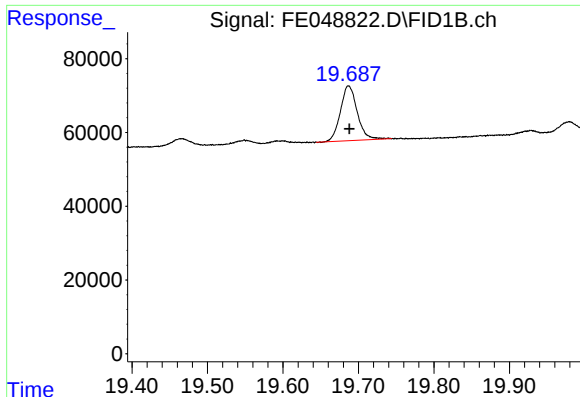

#19 n-Tetratriacontane (C34)


R.T.: 19.687 min
Delta R.T.: -0.001 min
Response: 230448
Conc: 1.67 ug/ml

Instrument :
FID_E
ClientSampleId :

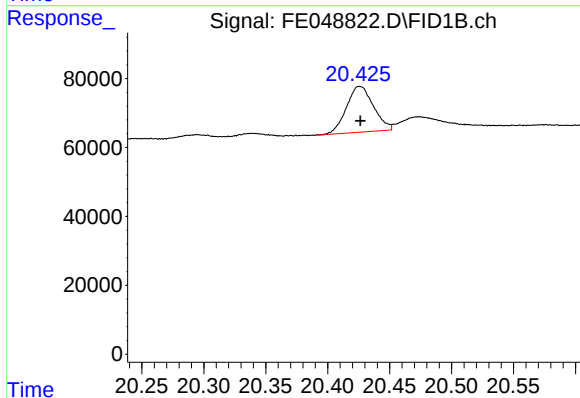


#20 n-Hexatriacontane (C36)

R.T.: 20.426 min
Delta R.T.: 0.000 min
Response: 201419
Conc: 1.55 ug/ml

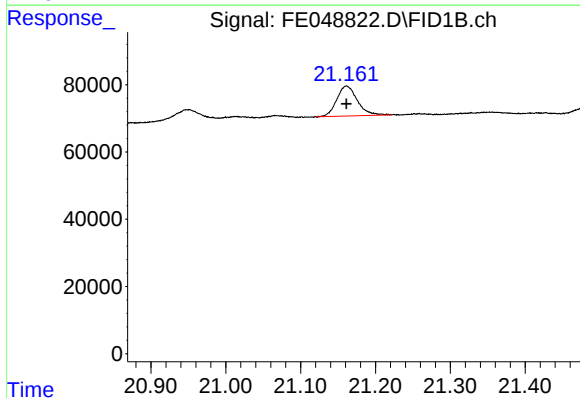

#21 n-Octatriacontane (C38)

R.T.: 21.161 min
Delta R.T.: 0.000 min
Response: 171120
Conc: 1.33 ug/ml

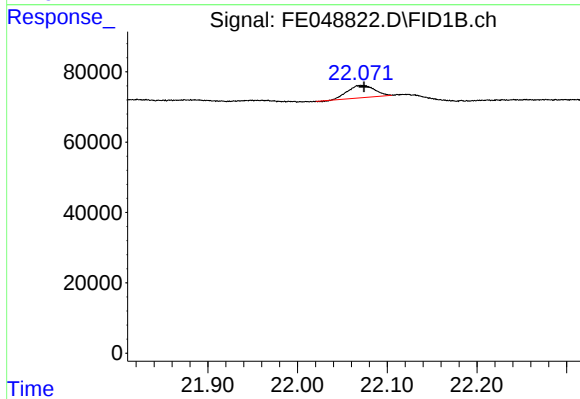

#22 n-Tetracontane (C40)

R.T.: 22.071 min
Delta R.T.: -0.003 min
Response: 72464
Conc: 0.59 ug/ml