

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036155.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 14:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 02:38:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	14.960	2826875	19.547 ug/ml
Target Compounds				
12)	N-DOTRIACONTANE	18.848	83061	0.759 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036155.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 14:33
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 23 02:38:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

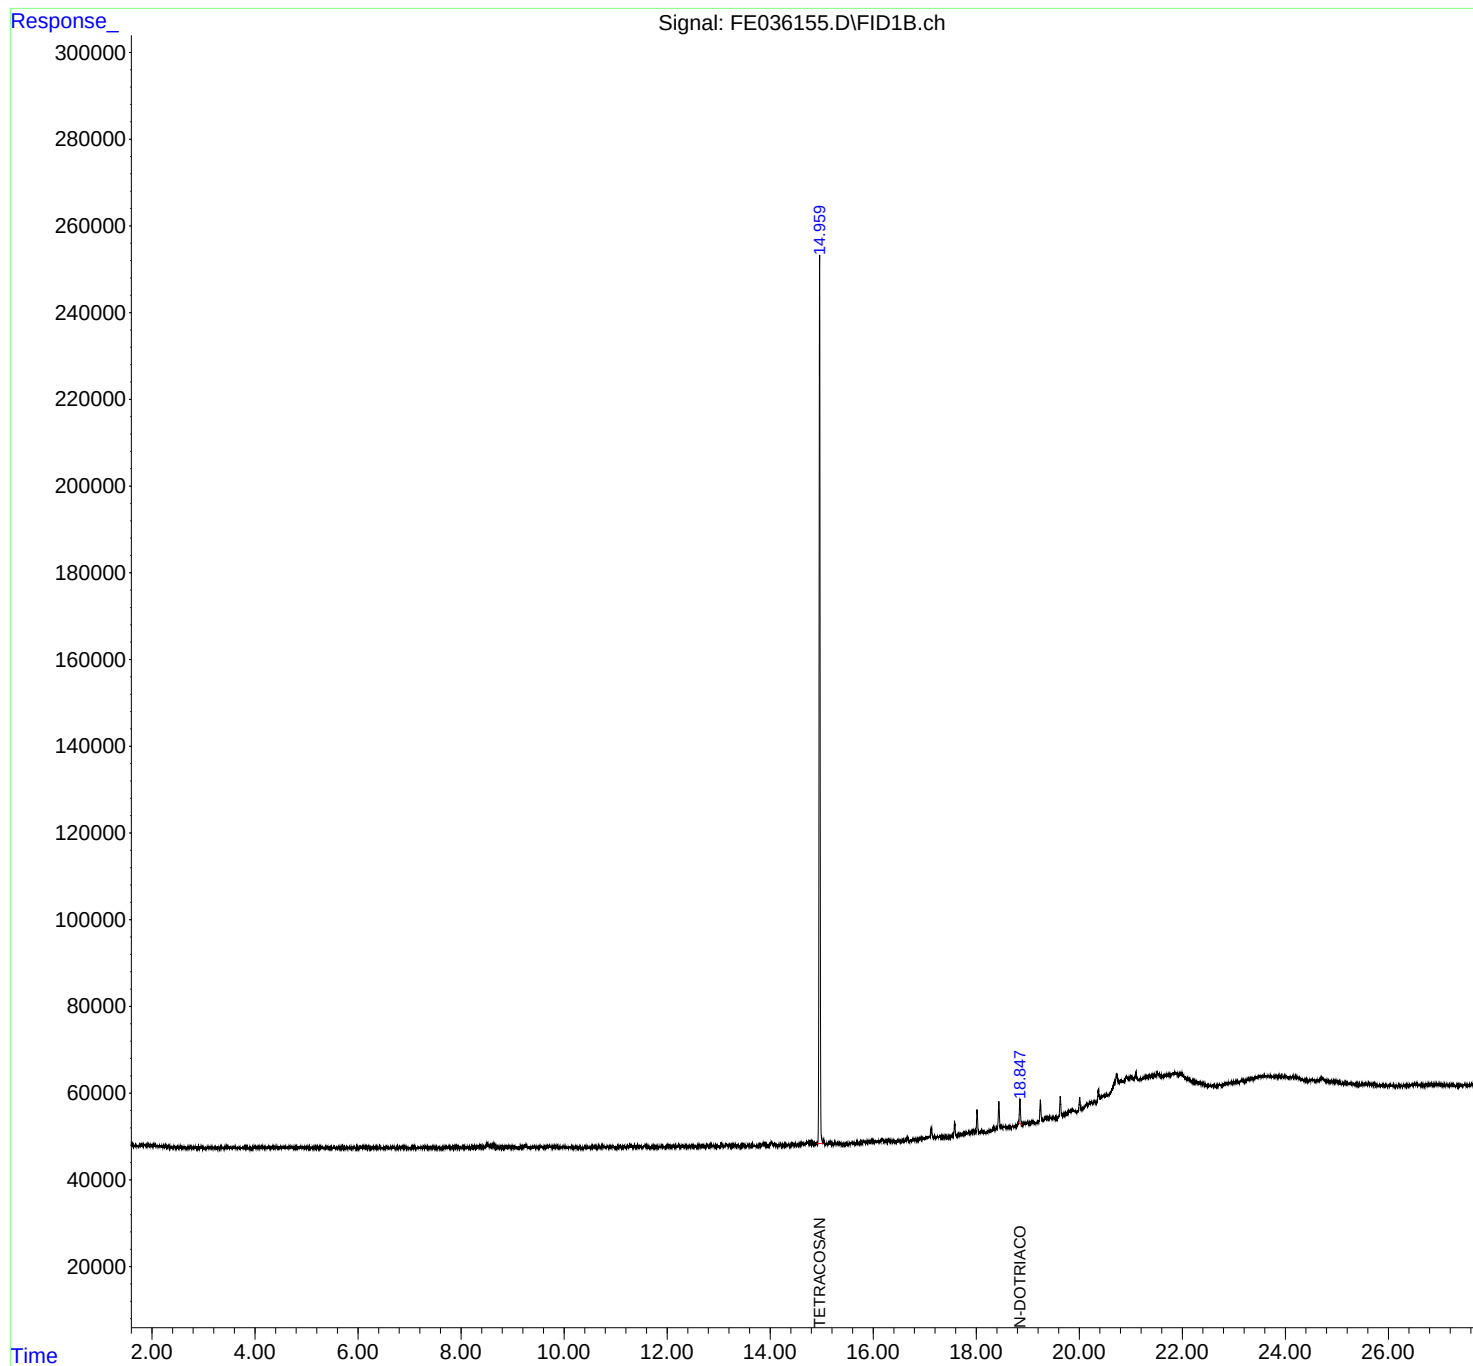


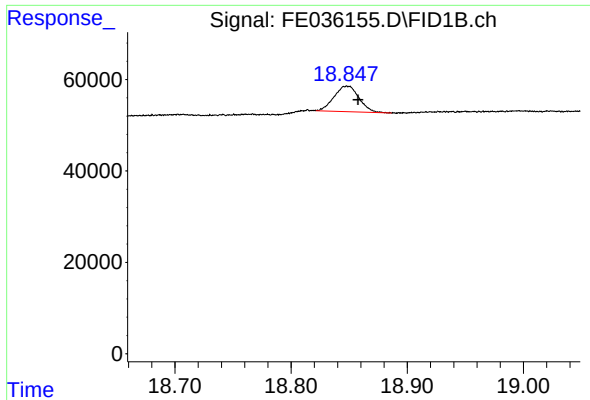

#12 N-DOTRIACONTANE

R.T.: 18.848 min
Delta R.T.: -0.010 min
Response: 83061
Conc: 0.76 ug/ml

Instrument :
FID_E
ClientSampleId :

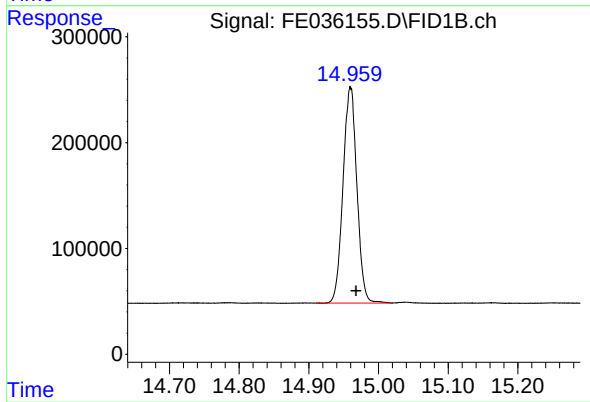

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.960 min
Delta R.T.: -0.008 min
Response: 2826875
Conc: 19.55 ug/ml