

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036147.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 08:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 22 15:17:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036147.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 08:51
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
MECL2

Integration File: autoint1.e
Quant Time: Jun 22 15:17:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

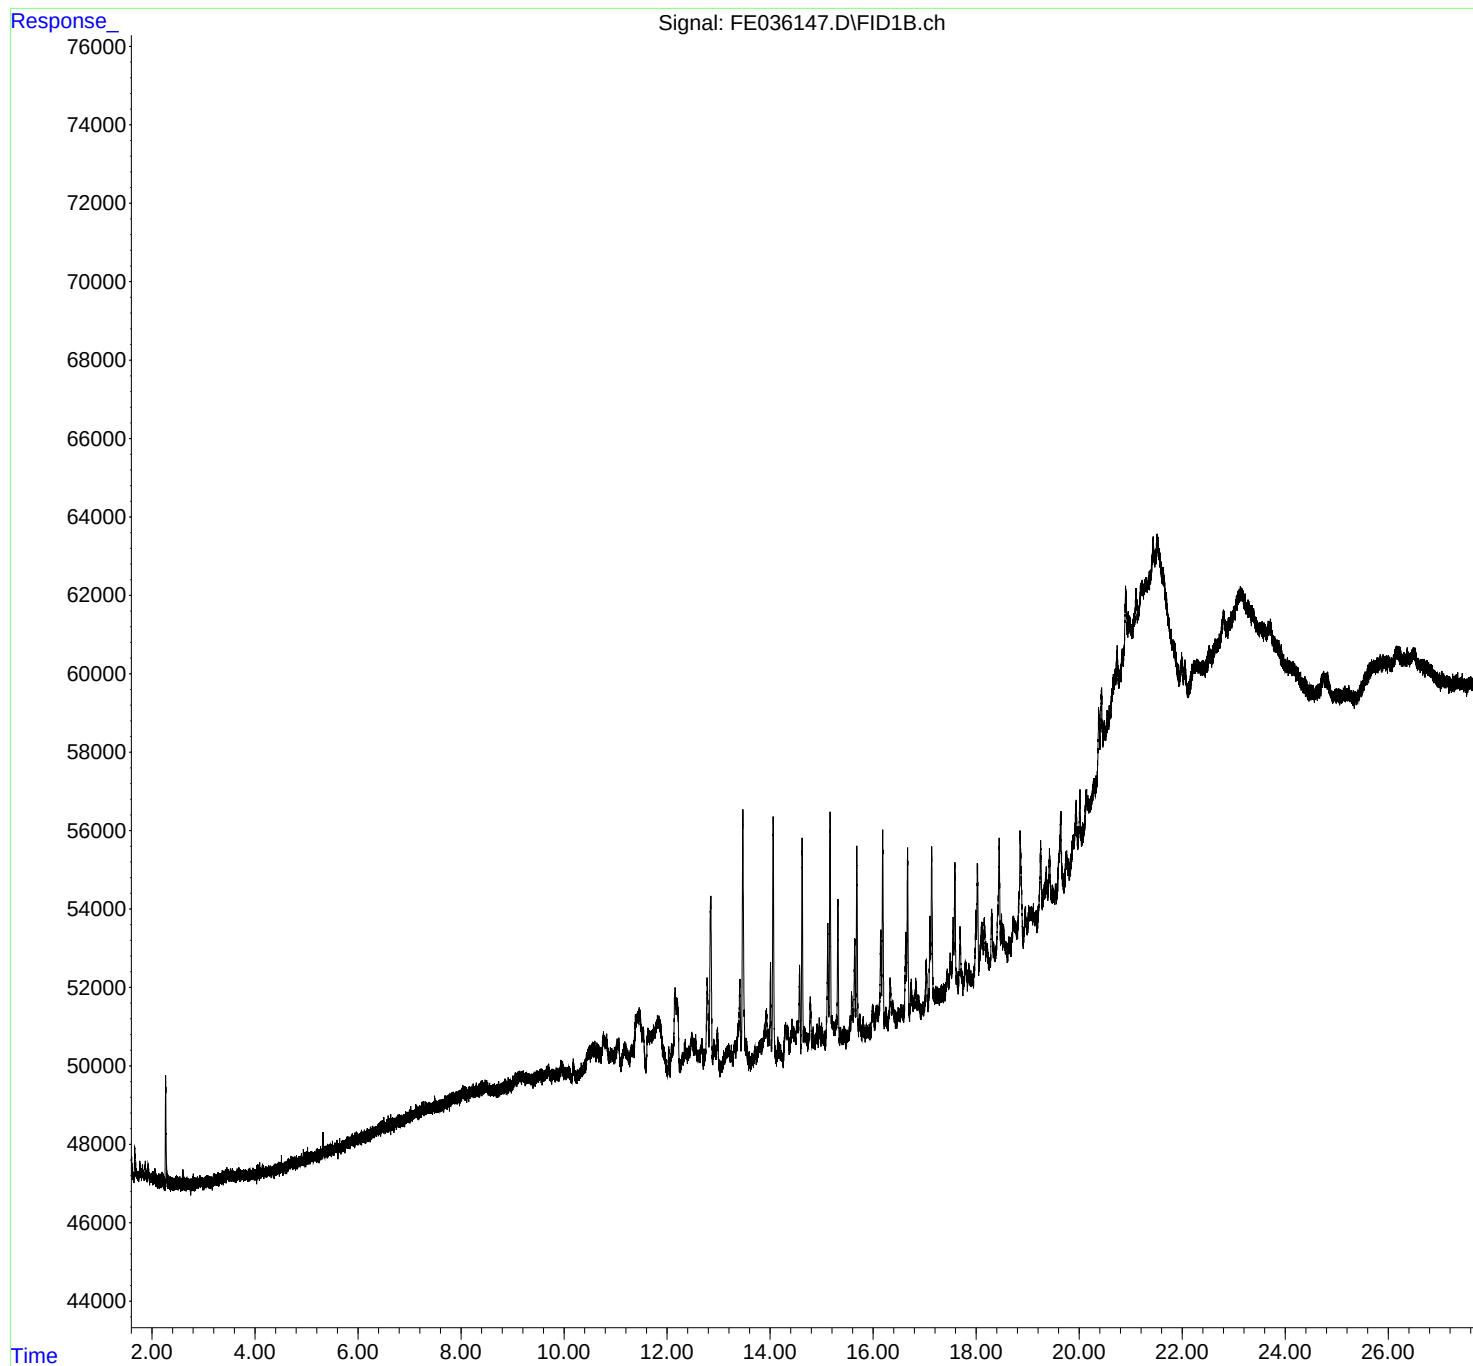

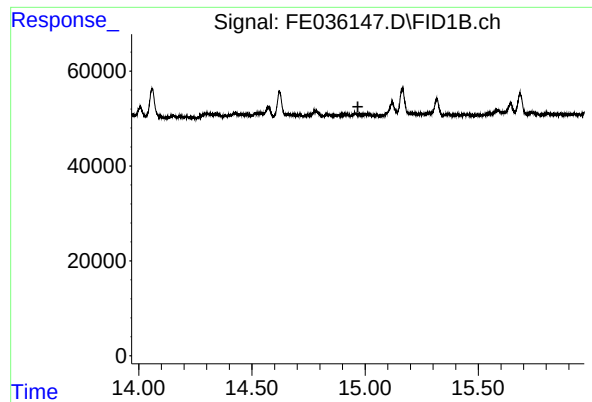

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.968 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
MECL2