

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036150.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 11:26
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 22 15:20:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
5) N-DODECANE	6.682	3800701	30.388 ug/ml
11) N-OCTACOSANE	17.134	3473763	30.717 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036150.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 11:26
Operator : YP\AJ
Sample : RT MARKER
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Jun 22 15:20:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

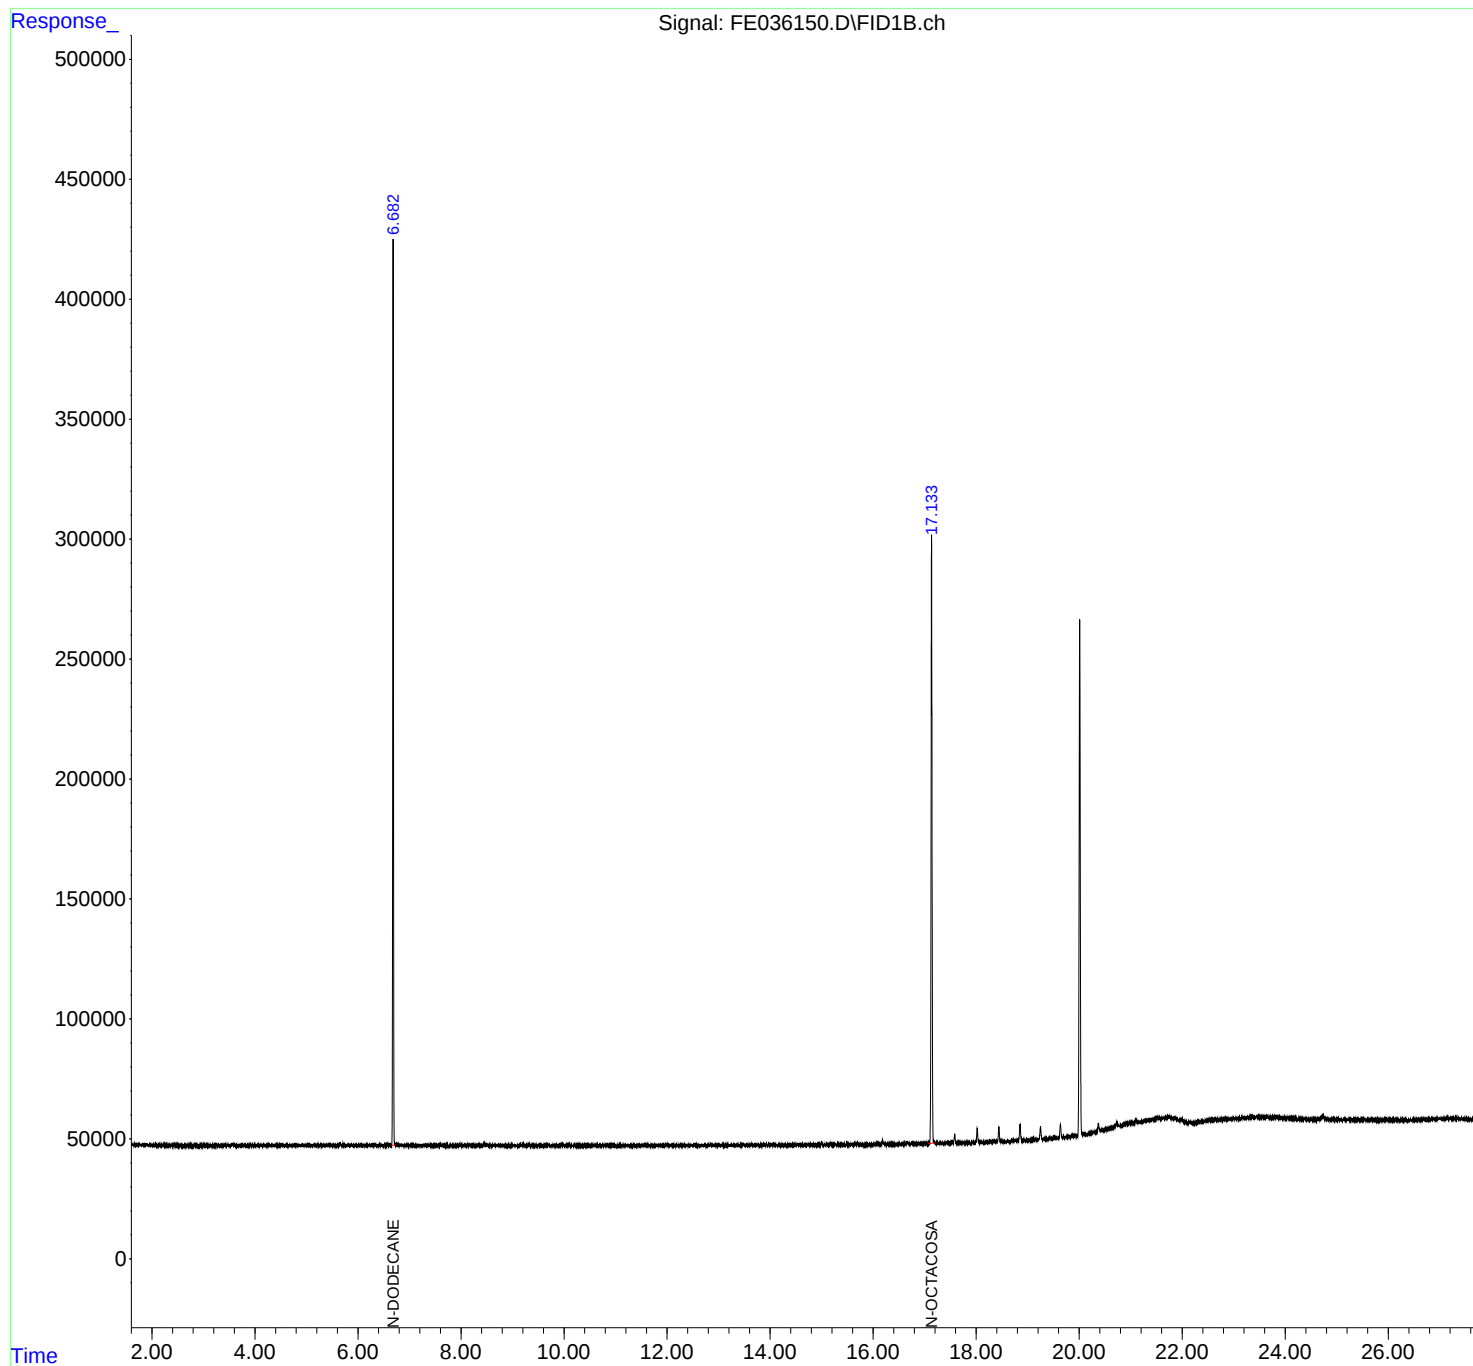


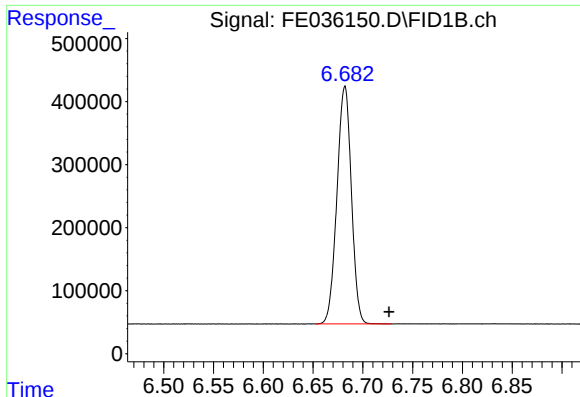

#5 N-DODECANE


R.T.: 6.682 min
Delta R.T.: -0.044 min
Response: 3800701
Conc: 30.39 ug/ml

Instrument :
FID_E
ClientSampleId :
RT MARKER

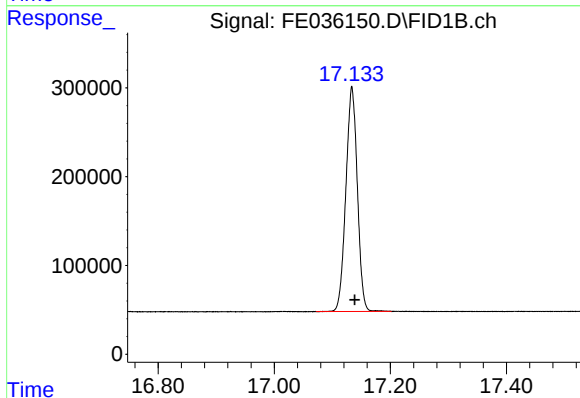

#11 N-OCTACOSANE

R.T.: 17.134 min
Delta R.T.: -0.005 min
Response: 3473763
Conc: 30.72 ug/ml

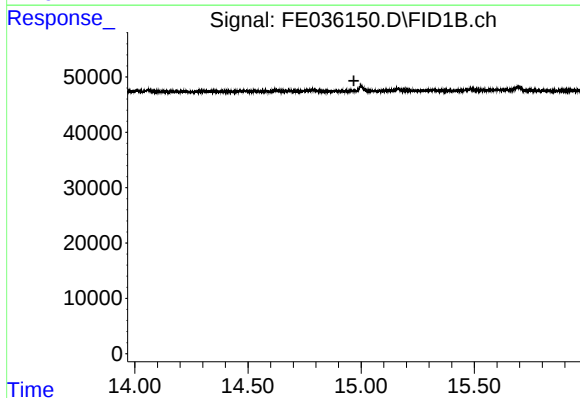

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.968 min
Response: 0
Conc: N.D.