

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
 Data File : FE036154.D
 Signal(s) : FID1B.ch
 Acq On : 22 Jun 2022 13:58
 Operator : YP\AJ
 Sample : N3203-01 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 GATE-6-JET-GROUT-SPOILS

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 06/23/2022
 Supervised By :Ankita Jodhani 06/23/2022

Integration File: autoint1.e
 Quant Time: Jun 23 02:37:52 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
 Quant Title :
 QLast Update : Wed Jun 22 08:57:44 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20m x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
13) S TETRACOSANE-d50 (SURR...	14.960	808766	5.592 ug/mlm
Target Compounds			

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062222\
Data File : FE036154.D
Signal(s) : FID1B.ch
Acq On : 22 Jun 2022 13:58
Operator : YP\AJ
Sample : N3203-01 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
GATE-6-JET-GROUT-SPOILS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022

Integration File: autoint1.e
Quant Time: Jun 23 02:37:52 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062122.M
Quant Title :
QLast Update : Wed Jun 22 08:57:44 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

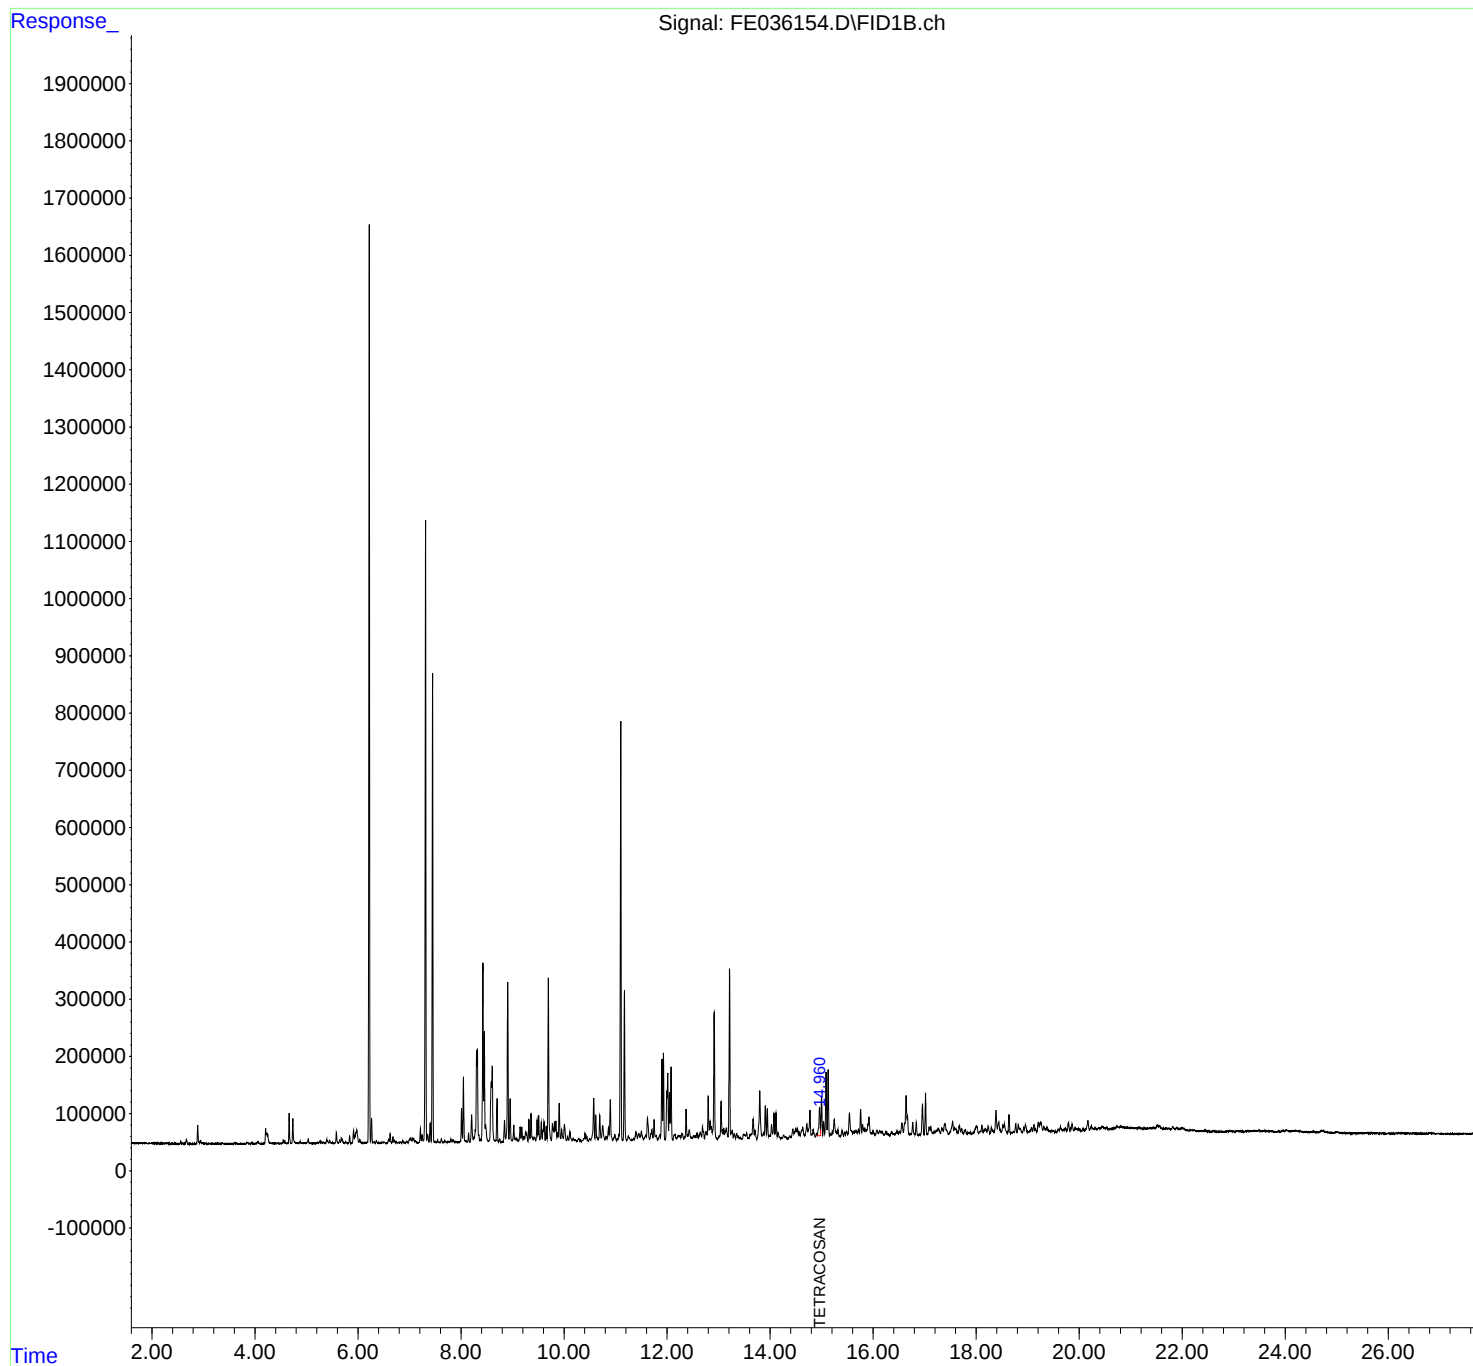

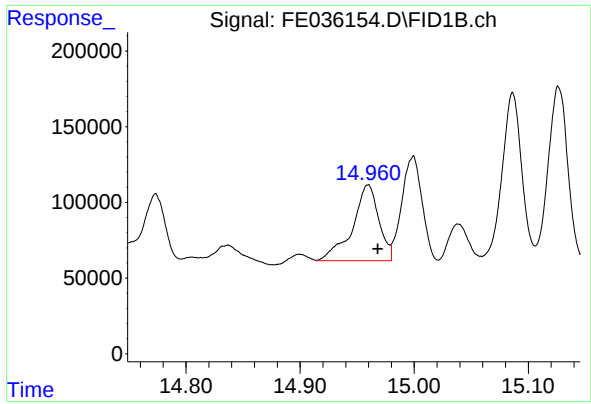

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.960 min
Delta R.T.: -0.008 min
Response: 808766
Conc: 5.59 ug/ml

Instrument :
FID_E
ClientSampleId :
GATE-6-JET-GROUT-SPOILS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 06/23/2022
Supervised By :Ankita Jodhani 06/23/2022