

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062322\
Data File : FE036159.D
Signal(s) : FID1B.ch
Acq On : 23 Jun 2022 10:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 24 01:55:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.959	3020691	21.527 ug/ml
Target Compounds			
13) N-TRIACONTANE	18.018	91419	0.616 ug/ml
14) N-DOTRIACONTANE	18.849	118826	0.842 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062322\
Data File : FE036159.D
Signal(s) : FID1B.ch
Acq On : 23 Jun 2022 10:04
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 24 01:55:28 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

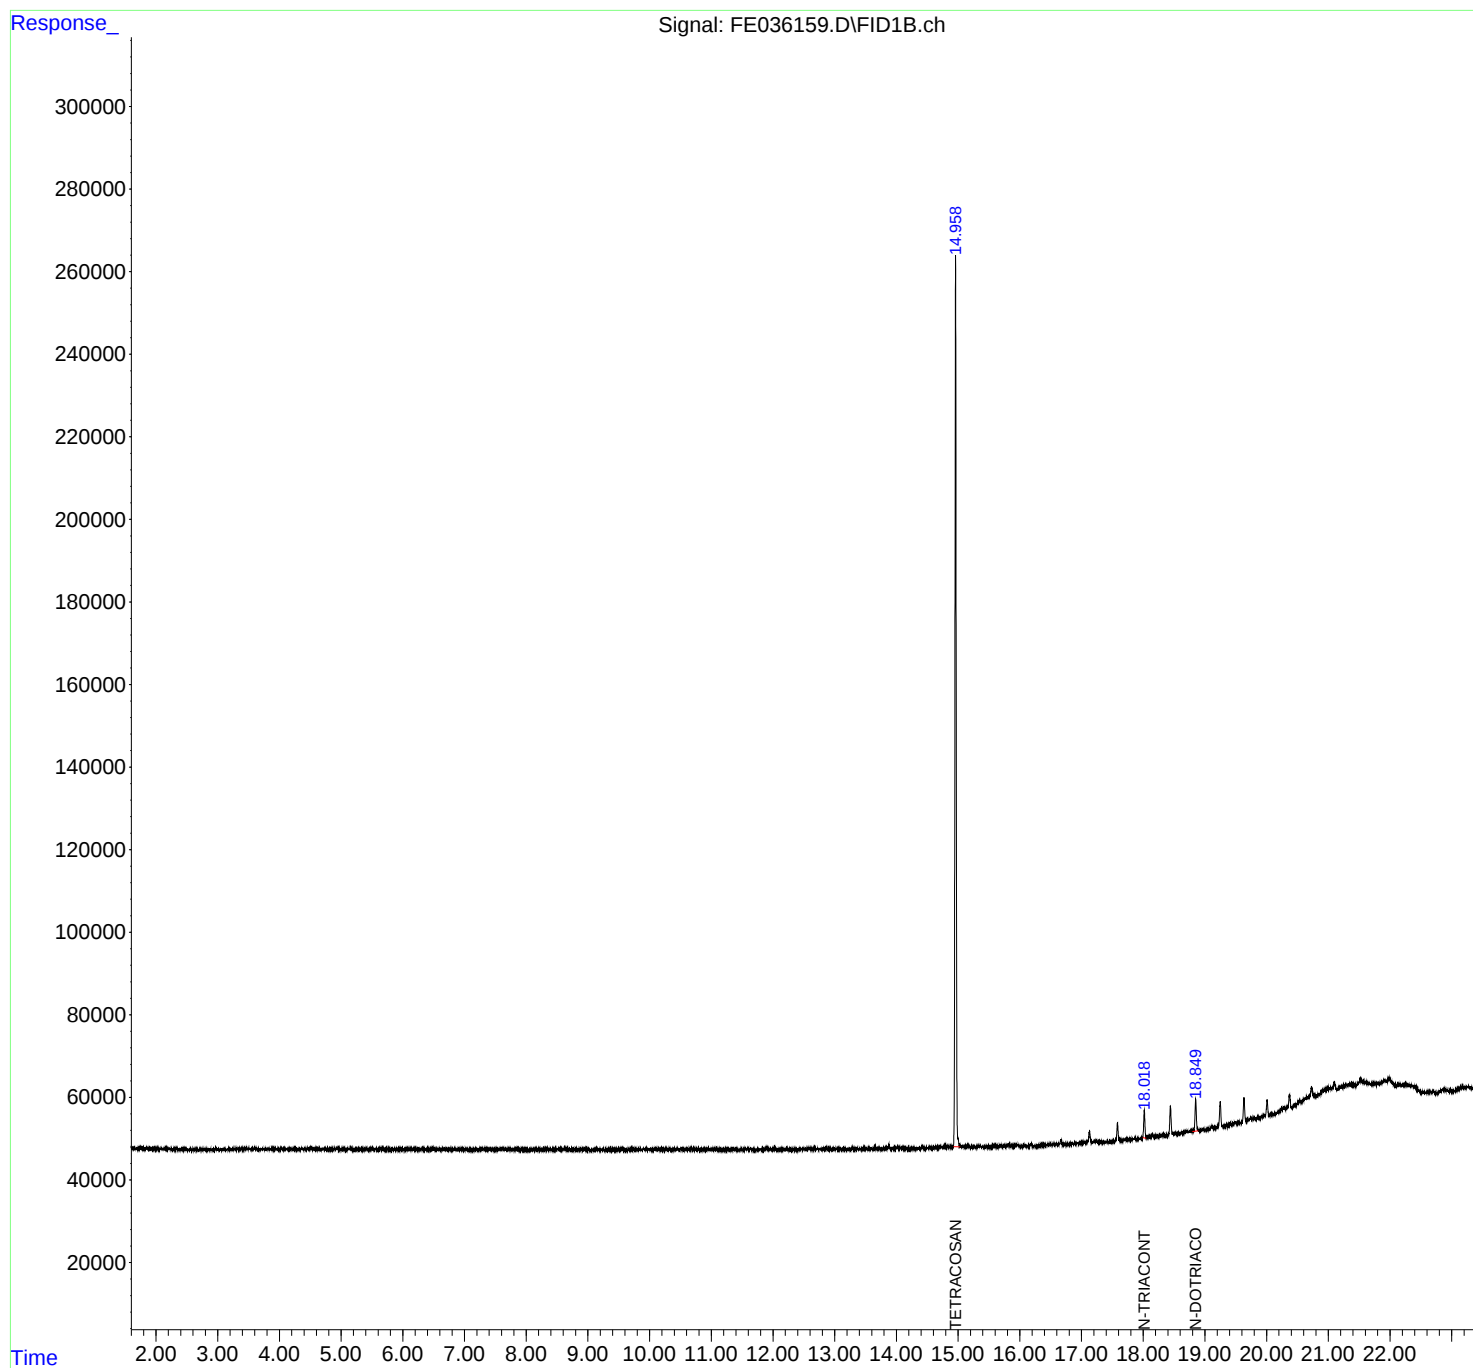

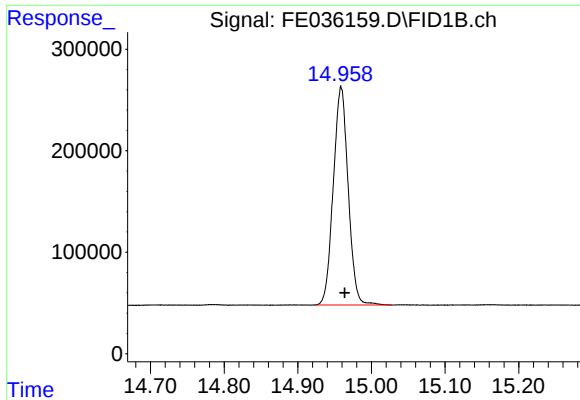


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.959 min
Delta R.T.: -0.005 min
Response: 3020691
Conc: 21.53 ug/ml

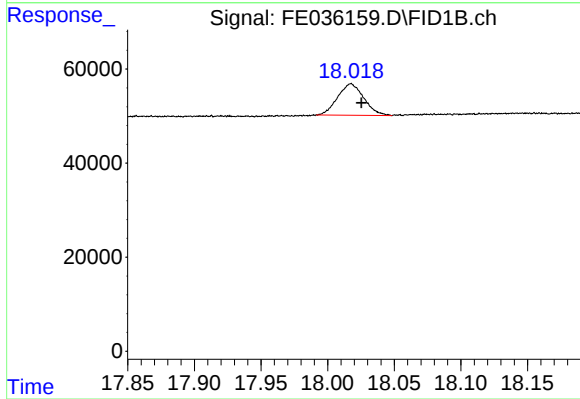

#13 N-TRIACONTANE

R.T.: 18.018 min
Delta R.T.: -0.007 min
Response: 91419
Conc: 0.62 ug/ml

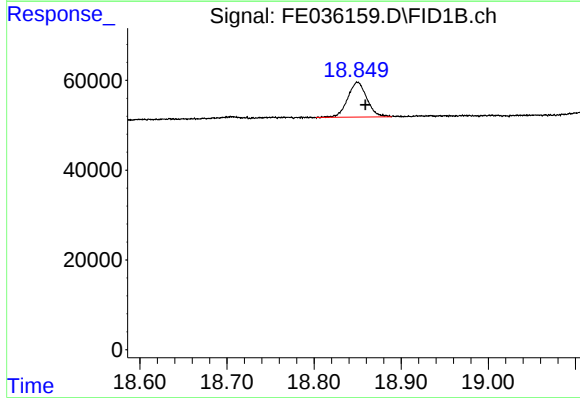

#14 N-DOTRIACONTANE

R.T.: 18.849 min
Delta R.T.: -0.010 min
Response: 118826
Conc: 0.84 ug/ml