

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062323AL\
Data File : FE042854.D
Signal(s) : FID1B.ch
Acq On : 23 Jun 2023 21:50
Operator : YP\AJ
Sample : 03365-16DL 50X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP4-BDL

Integration File: autoint1.e
Quant Time: Jun 24 04:00:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 11:03:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062323AL\
Data File : FE042854.D
Signal(s) : FID1B.ch
Acq On : 23 Jun 2023 21:50
Operator : YP\AJ
Sample : 03365-16DL 50X
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :
TP4-BDL

Integration File: autoint1.e
Quant Time: Jun 24 04:00:18 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 11:03:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

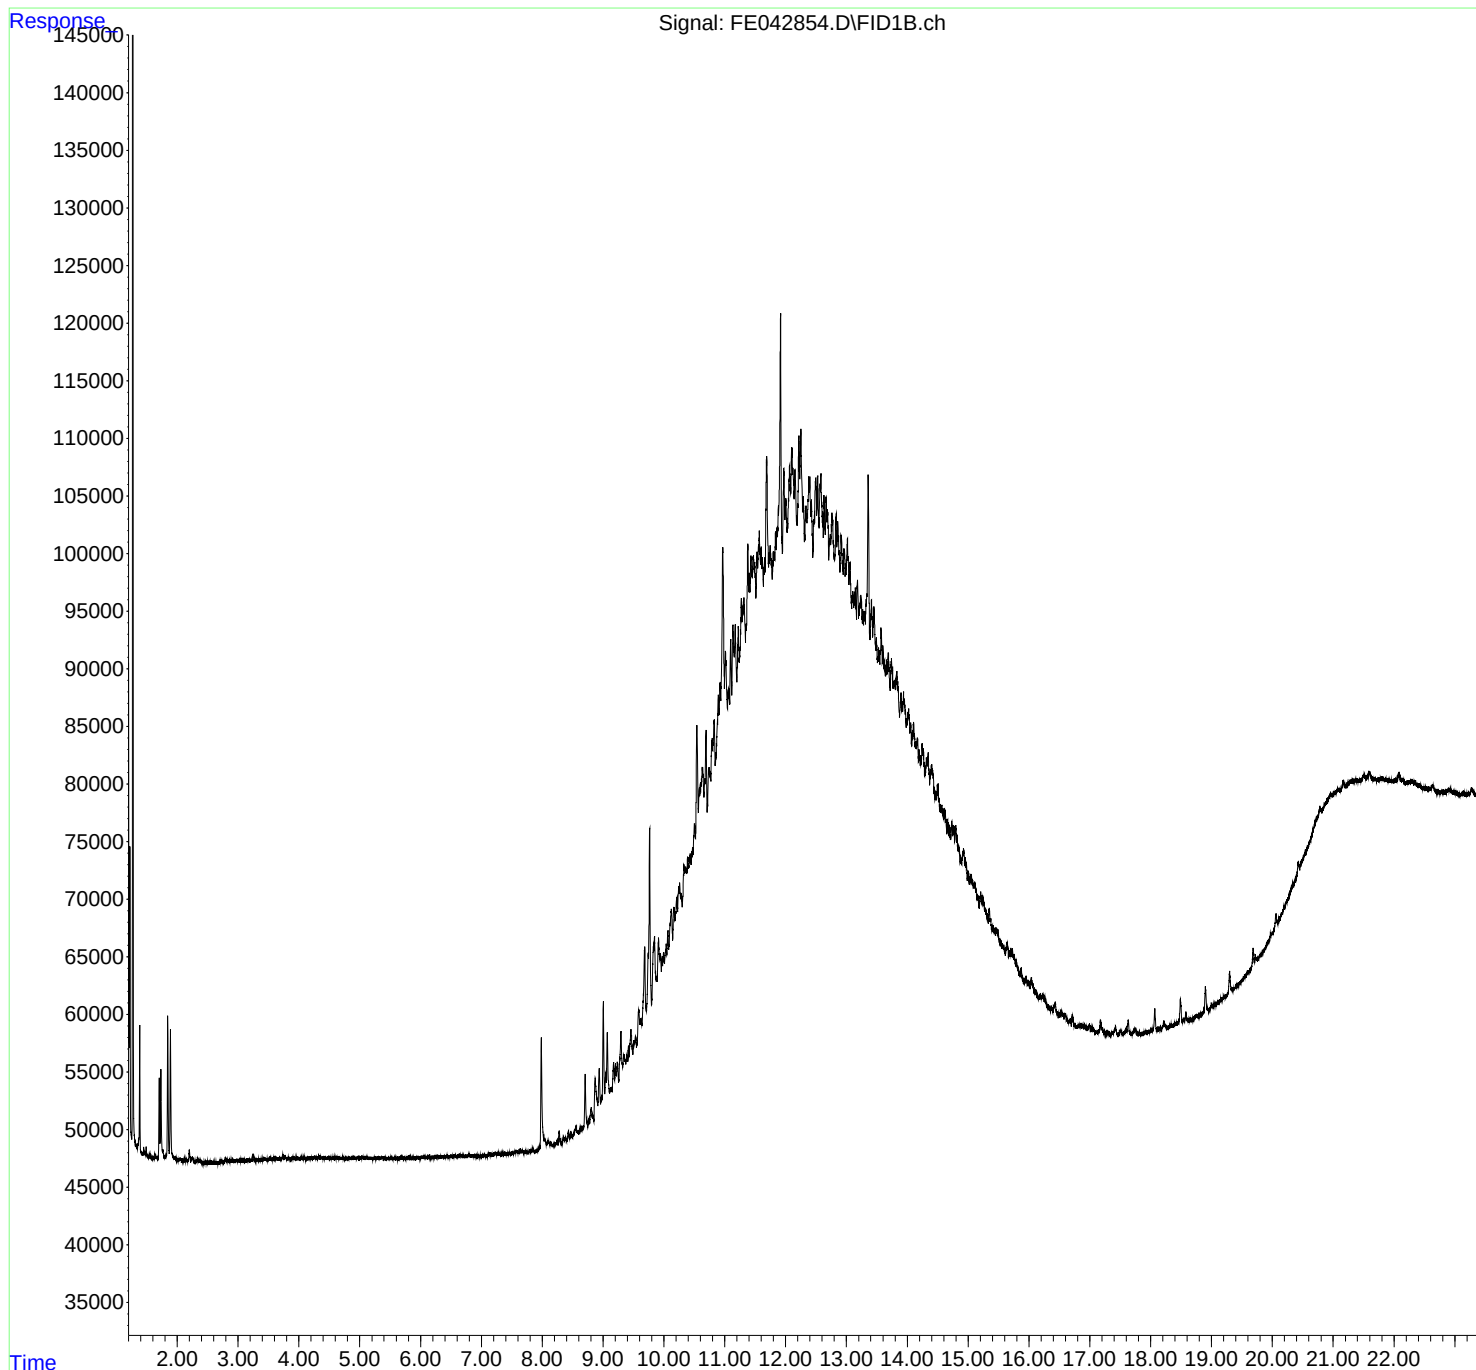


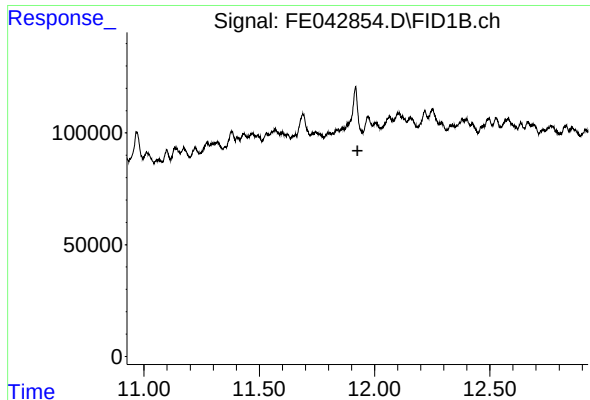

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :
TP4-BDL

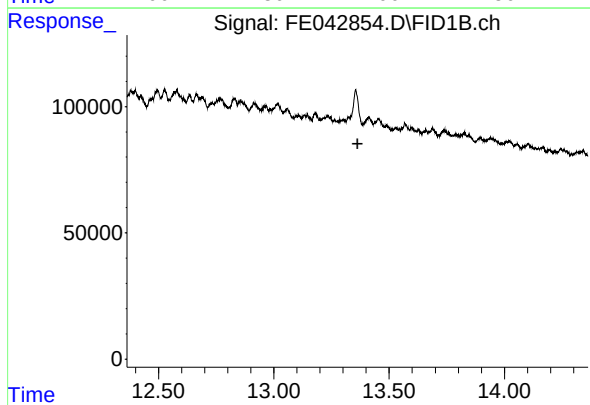

#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.363 min
Response: 0
Conc: N.D.