

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062422\
Data File : FE036177.D
Signal(s) : FID1B.ch
Acq On : 24 Jun 2022 10:26
Operator : YP\AJ
Sample : PB145780BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 24 23:14:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.957	2871943	20.467 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062422\
Data File : FE036177.D
Signal(s) : FID1B.ch
Acq On : 24 Jun 2022 10:26
Operator : YP\AJ
Sample : PB145780BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 24 23:14:43 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE062022.M
Quant Title :
QLast Update : Tue Jun 21 02:15:59 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

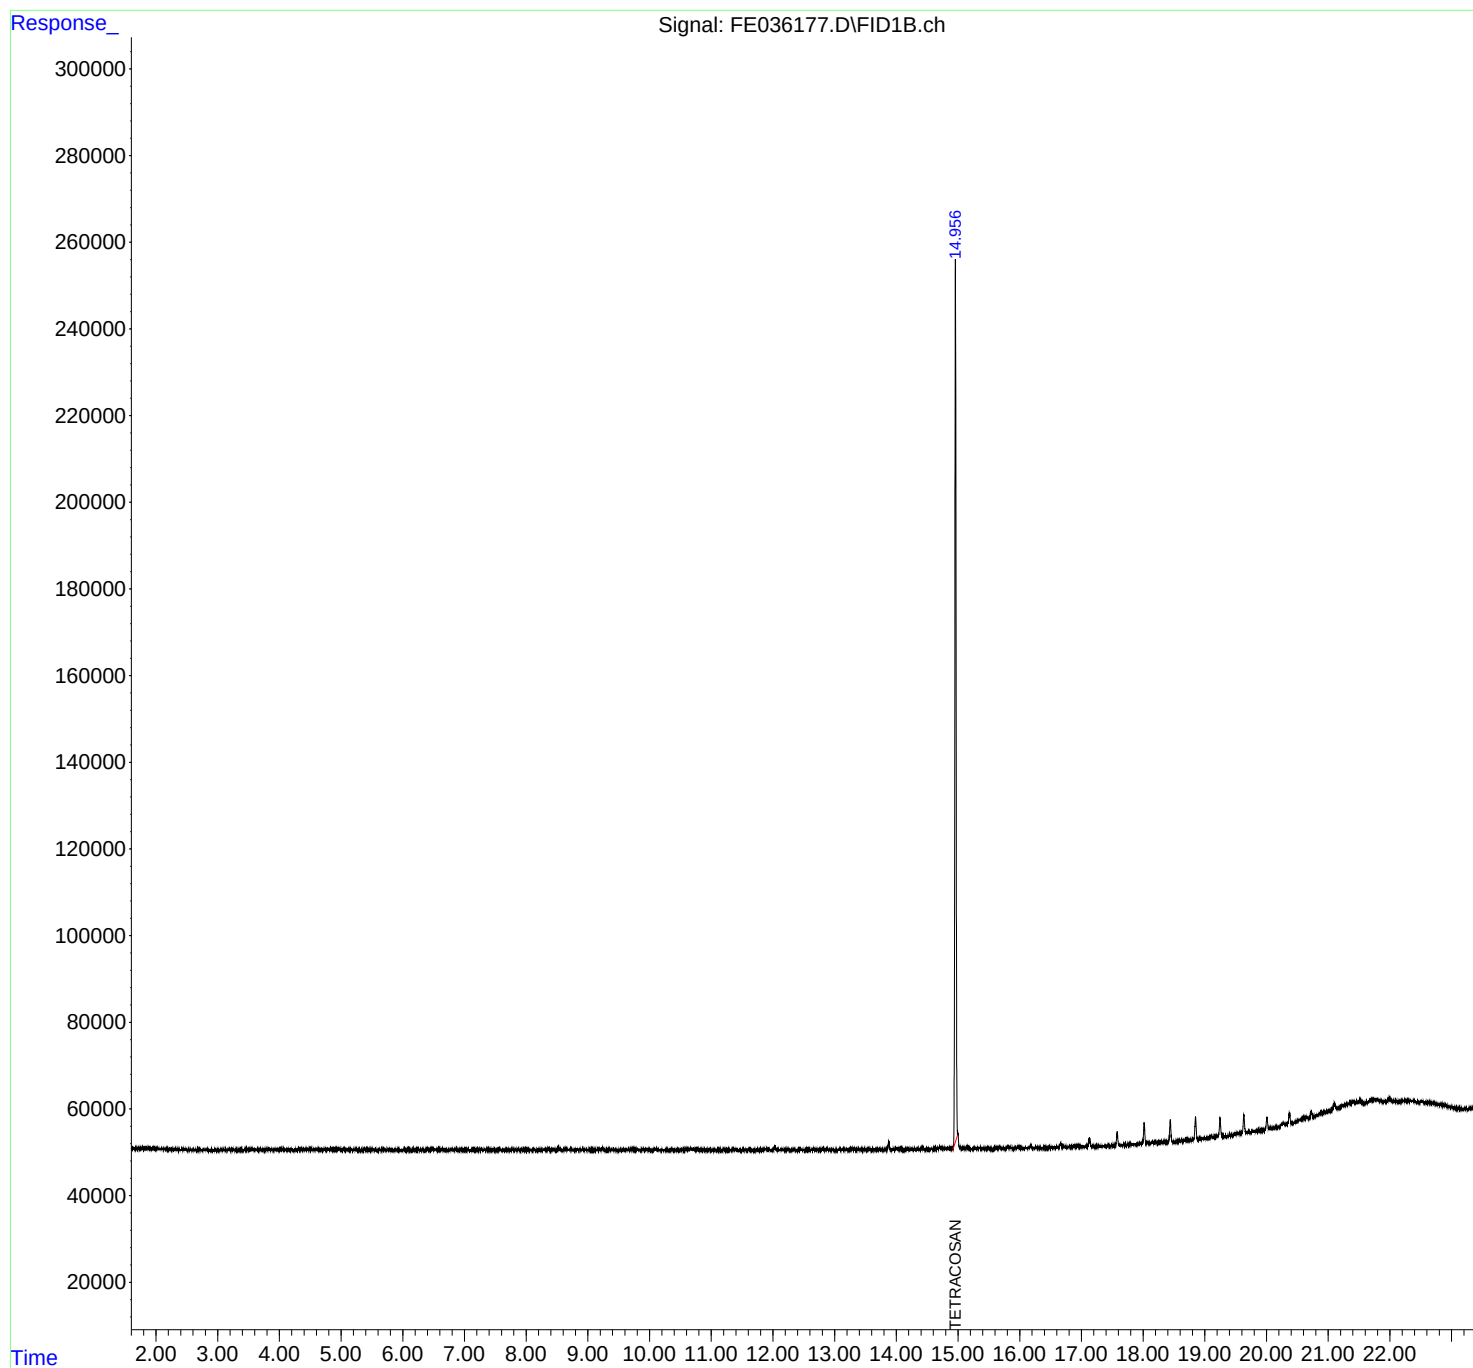

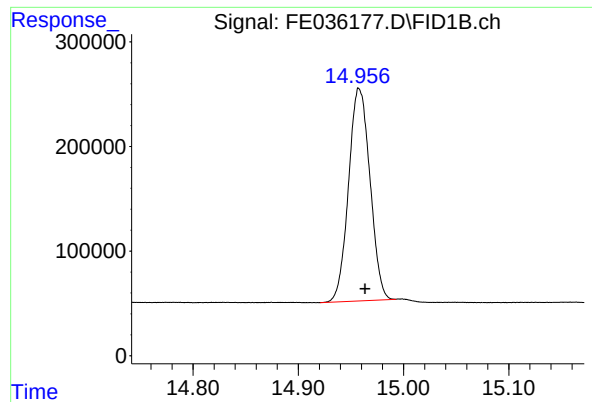

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.957 min
Delta R.T.: -0.006 min
Response: 2871943
Conc: 20.47 ug/ml