

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062422AL\
 Data File : FE036188.D
 Signal(s) : FID1B.ch
 Acq On : 24 Jun 2022 17:46
 Operator : YP\AJ
 Sample : N3431-17DL 50X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 24 23:41:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 21 03:08:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
12) S 1-chlorooctadecane (S...	13.303	79726	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
Target Compounds			
1) T n-Nonane (C9)	3.277	84126	<MDL ug/ml
2) T n-Decane (C10)	4.497	100747	<MDL ug/ml
3) T A~Naphthalene (C11.7)	6.211	66011	<MDL ug/ml
4) T n-Dodecane (C12)	6.699	179205	<MDL ug/ml
5) T A~2-methylnaphthalene...	7.309	145661	<MDL ug/ml
6) T n-Tetradecane (C14)	8.468	41167	<MDL ug/ml
7) T n-Hexadecane (C16)	10.069	57033	<MDL ug/ml
17) T n-Tricontane (C30)	18.015	56559	<MDL ug/ml
18) T n-Dotriacontane (C32)	18.849	74988	<MDL ug/ml
19) T n-Tetratriacontane (C34)	19.630	53025	<MDL ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062422AL\
Data File : FE036188.D
Signal(s) : FID1B.ch
Acq On : 24 Jun 2022 17:46
Operator : YP\AJ
Sample : N3431-17DL 50X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 24 23:41:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

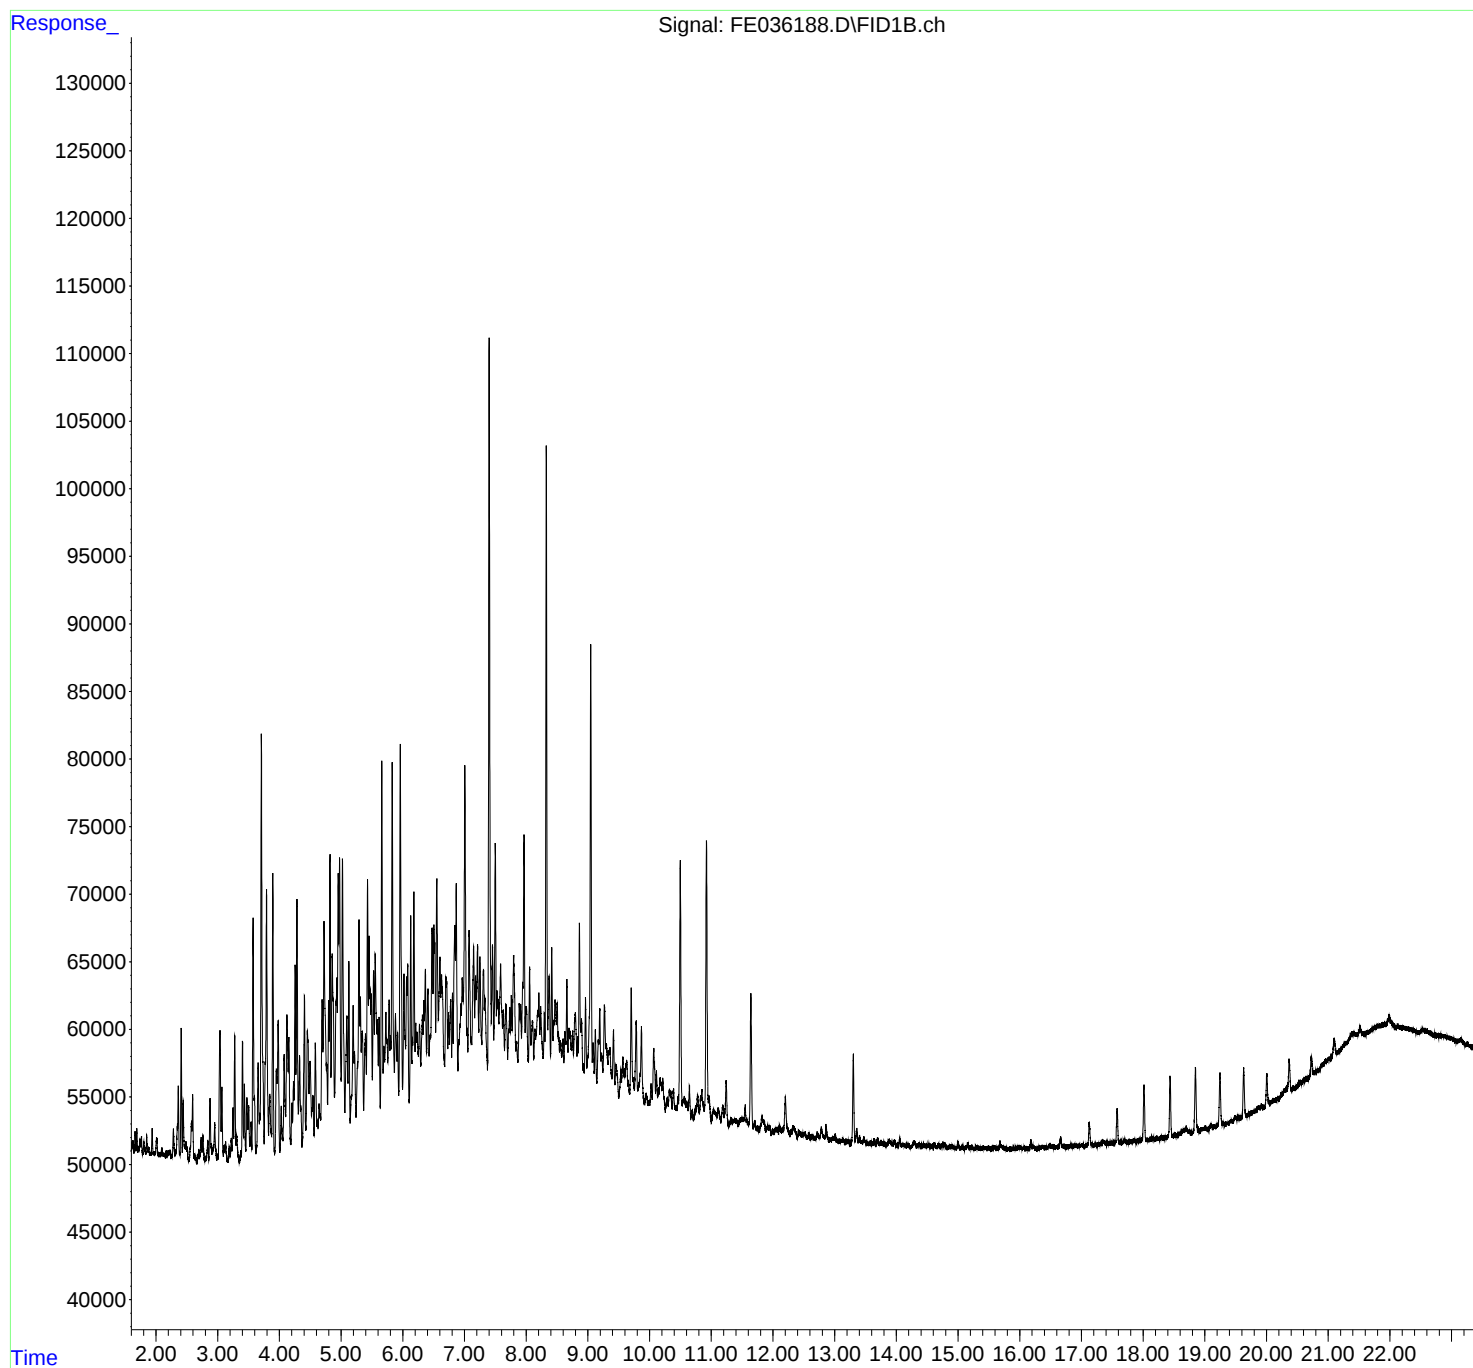


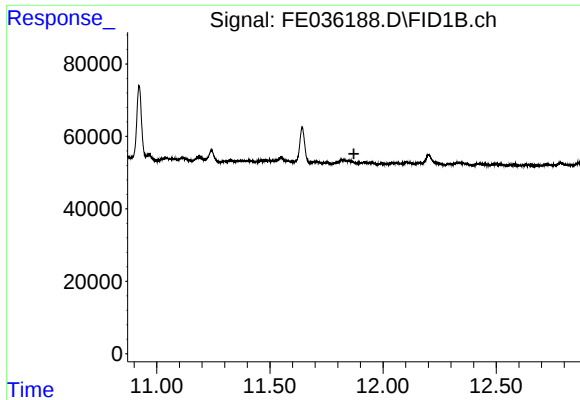

#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min
Exp R.T.: 11.871 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

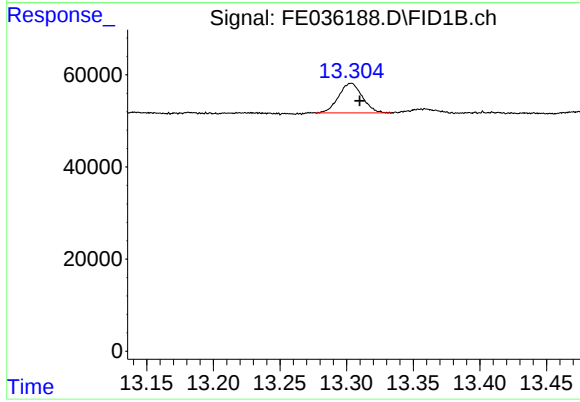

#12 1-chlorooctadecane (SURR)

R.T.: 13.303 min
Delta R.T.: -0.006 min
Response: 79726
Conc: N.D.