

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Jun 2022 23:28
 Operator : AJ\MA
 Sample : PB145787BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:07:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.193	6.777	1302.8E6	556.9E6	543.019	718.733 #
Target Compounds							
1) T	Dalapon	2.964f	2.481f	160.5E6	96465942	31.662	96.135 #
2) T	3,5-DICHL...	6.370f	5.984	3064211	65691802	<MDL	54.804 #
3) T	4-Nitroph...	7.054	6.424	40871120	2171663	41.649	5.074 #
5) T	DICAMBA	7.372	6.941	8147314	9978583	<MDL	2.919 #
6) T	MCP	7.595f	7.047	21775623	579833	2.901	<MDL #
7) T	MCPA	7.742f	7.237	41981857	23830692	3.886	6.202 #
8) T	DICHLORPROP	8.060	7.586	1334541	53769369	<MDL	60.868 #
10) T	Pentachlo...	8.629	8.285	78169412	2827211	2.260	<MDL #
11) T	2,4,5-TP ...	9.222f	8.676	158.0E6	30603724	10.065	6.088 #
12) T	2,4,5-T	9.462	9.027	4719667	25674171	<MDL	5.459 #
13) T	2,4-DB	10.037	9.535	382.7E6	114.9E6	94.597	185.904 #
14) T	DINOSEB	11.118	9.855	2238.4E6	165.7E6	144.718	46.651 #
15) T	Picloram	11.023	10.852	1265.6E6	124.8E6	42.645	19.400 #
16) T	DCPA	0.000	10.778	0	29625378	N.D.	4.800



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Jun 2022 23:28
Operator : AJ\MA
Sample : PB145787BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:07:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

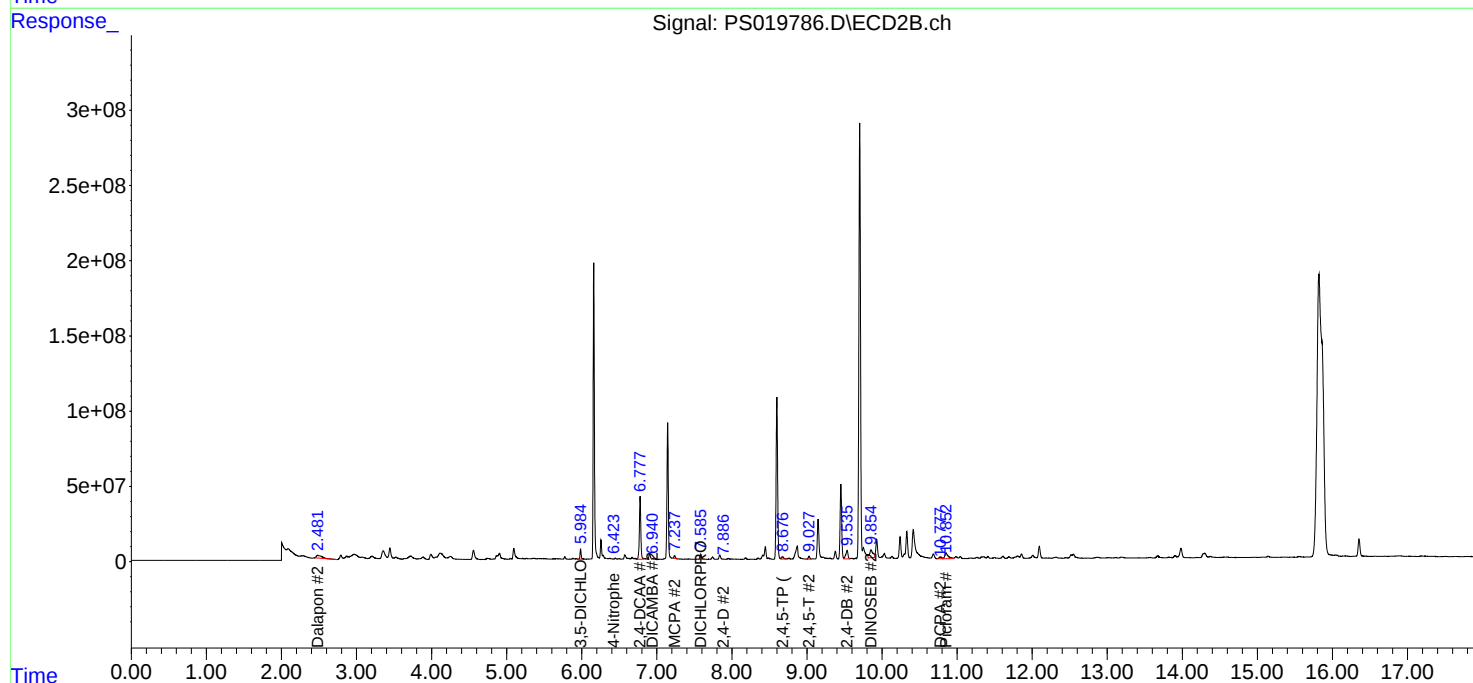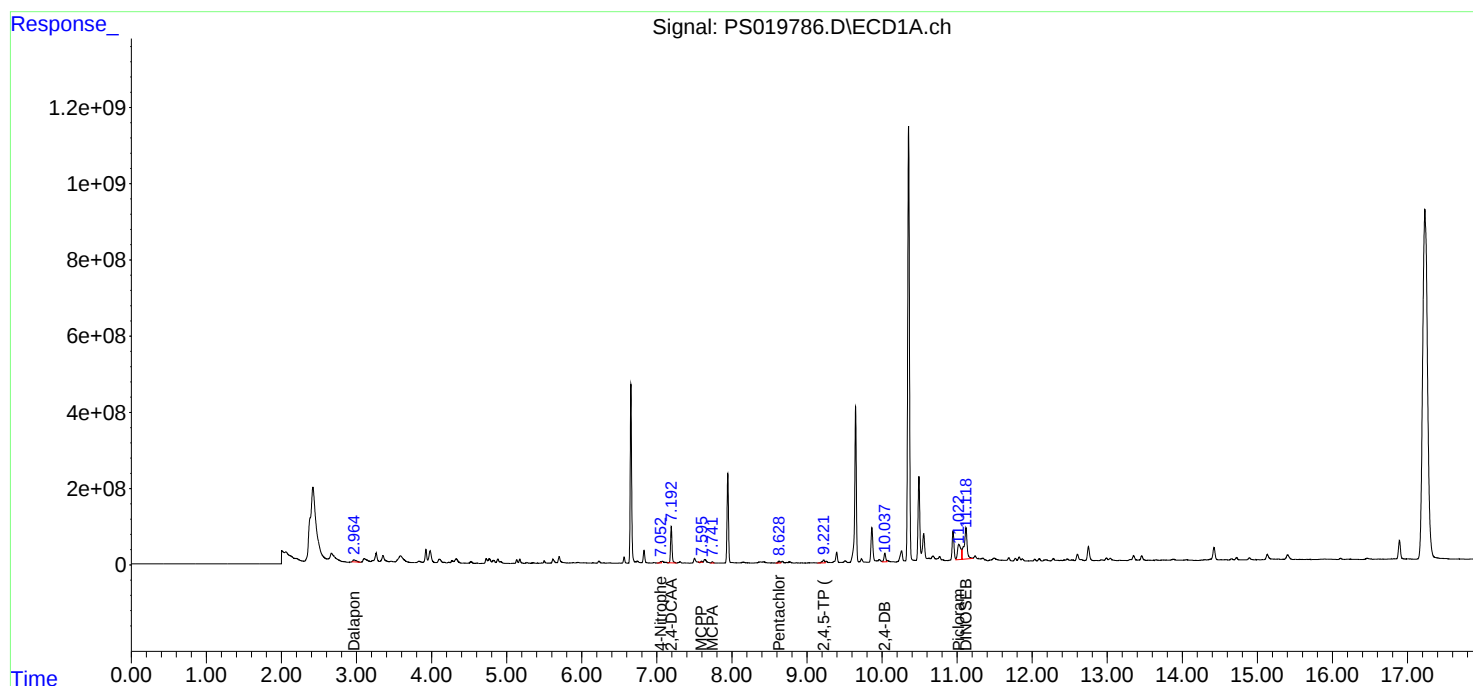


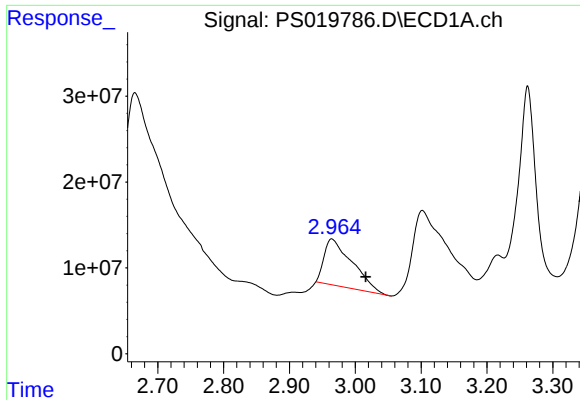

#1 Dalapon


R.T.: 2.964 min
Delta R.T.: -0.052 min
Response: 160488807
Conc: 31.66 ng/ml

Instrument :
FID_E
ClientSampleId :

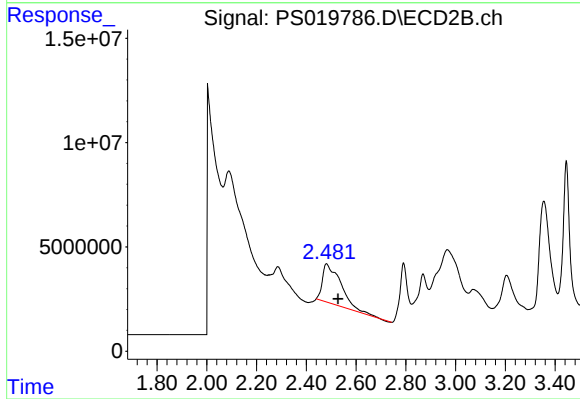


#1 Dalapon

R.T.: 2.481 min
Delta R.T.: -0.047 min
Response: 96465942
Conc: 96.14 ng/ml

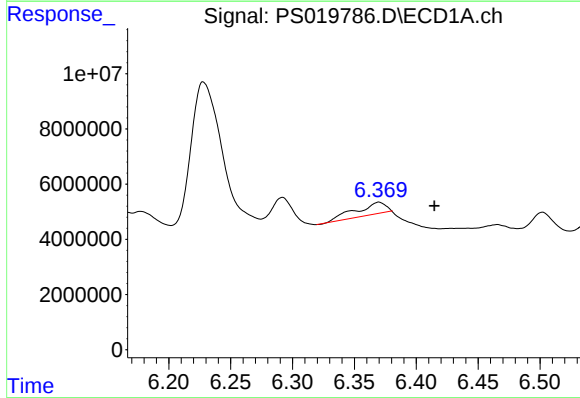


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.370 min
Delta R.T.: -0.045 min
Response: 3064211
Conc: N.D.

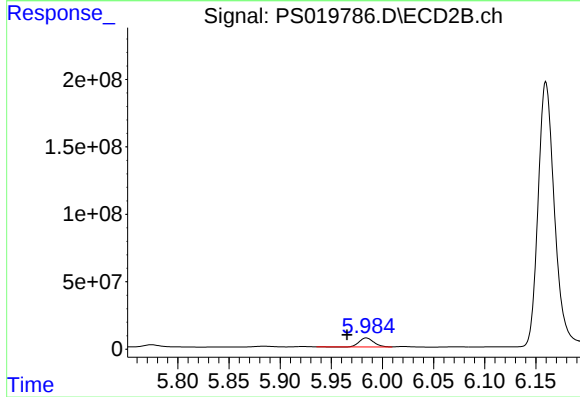

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.984 min
Delta R.T.: 0.019 min
Response: 65691802
Conc: 54.80 ng/ml

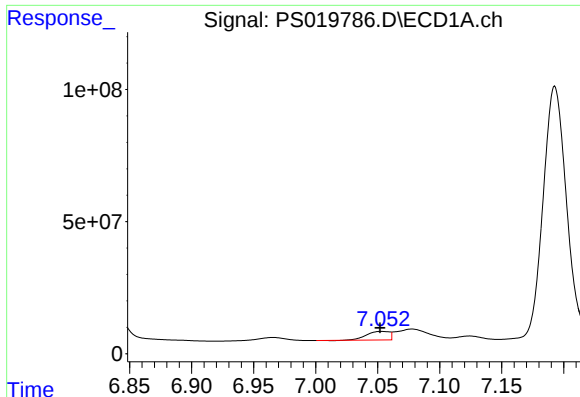

#3 4-Nitrophenol


R.T.: 7.054 min
Delta R.T.: 0.002 min
Response: 40871120
Conc: 41.65 ng/ml

Instrument :
FID_E
ClientSampleId :

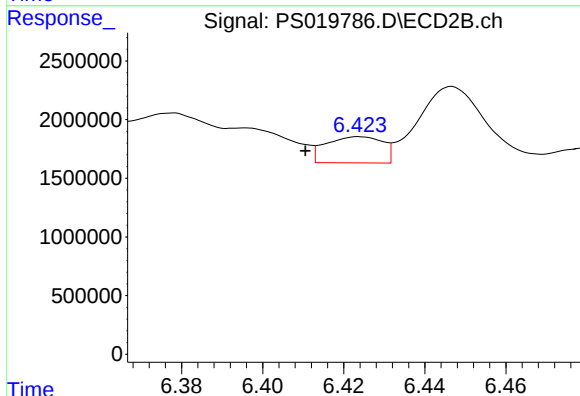


#3 4-Nitrophenol

R.T.: 6.424 min
Delta R.T.: 0.013 min
Response: 2171663
Conc: 5.07 ng/ml

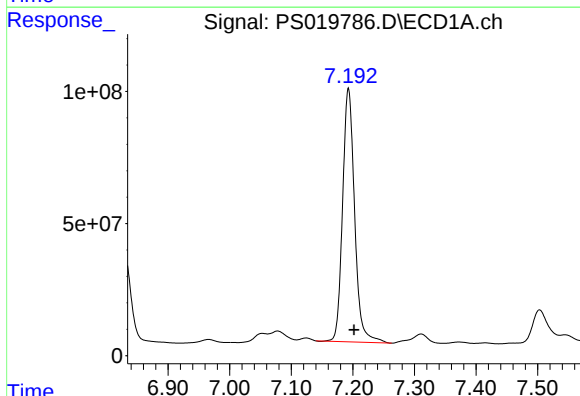


#4 2,4-DCAA

R.T.: 7.193 min
Delta R.T.: -0.009 min
Response: 1302793872
Conc: 543.02 ng/ml

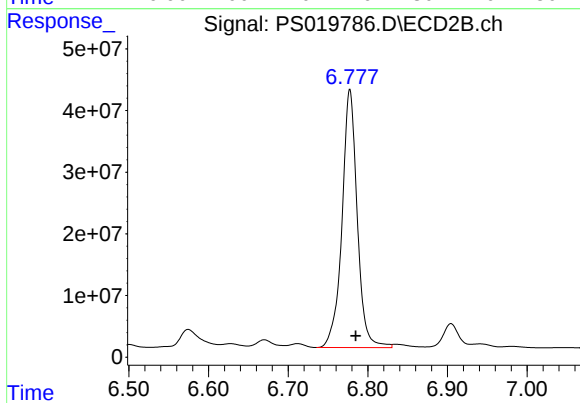

#4 2,4-DCAA


R.T.: 6.777 min
Delta R.T.: -0.007 min
Response: 556924820
Conc: 718.73 ng/ml

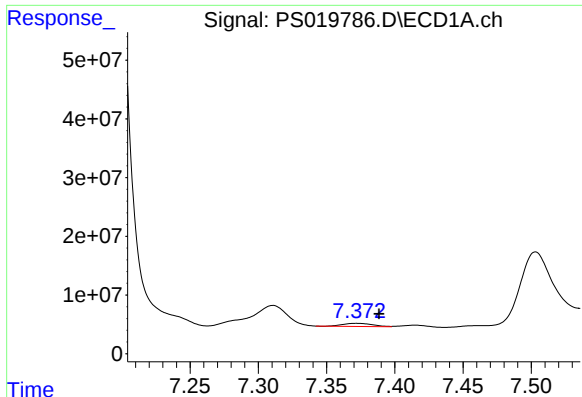

#5 DICAMBA


R.T.: 7.372 min
Delta R.T.: -0.016 min
Response: 8147314
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

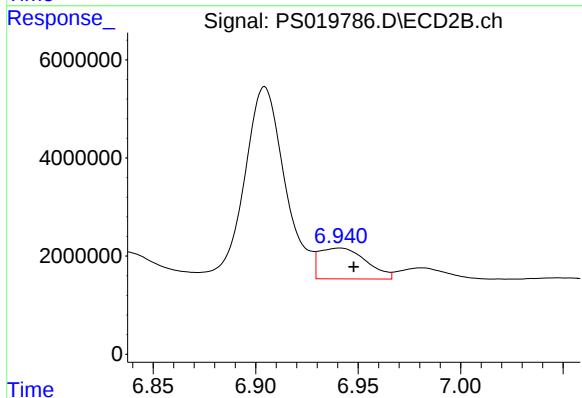


#5 DICAMBA

R.T.: 6.941 min
Delta R.T.: -0.007 min
Response: 9978583
Conc: 2.92 ng/ml

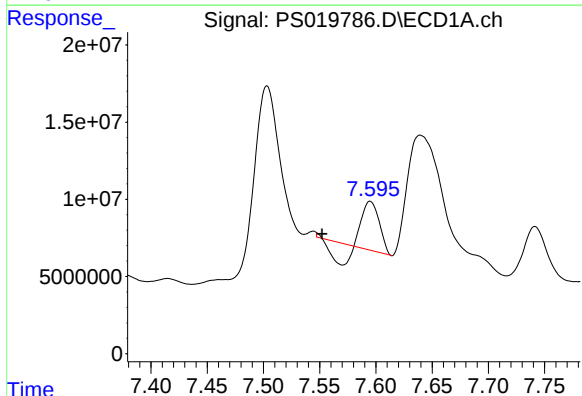


#6 MCP

R.T.: 7.595 min
Delta R.T.: 0.043 min
Response: 21775623
Conc: 2.90 ug/ml

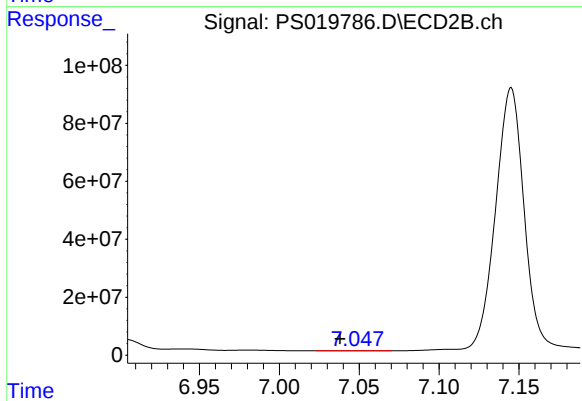

#6 MCP


R.T.: 7.047 min
Delta R.T.: 0.009 min
Response: 579833
Conc: N.D.

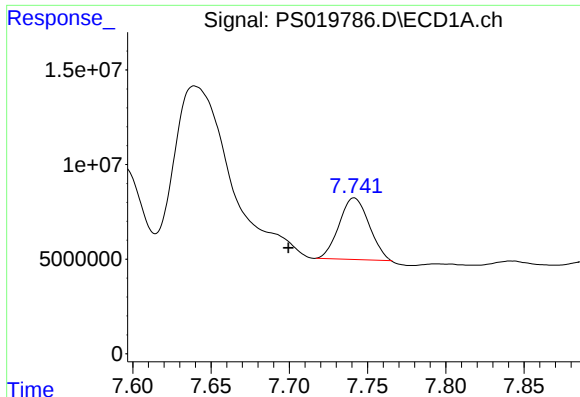

#7 MCPA


R.T.: 7.742 min
Delta R.T.: 0.042 min
Response: 41981857
Conc: 3.89 ug/ml

Instrument :
FID_E
ClientSampleId :

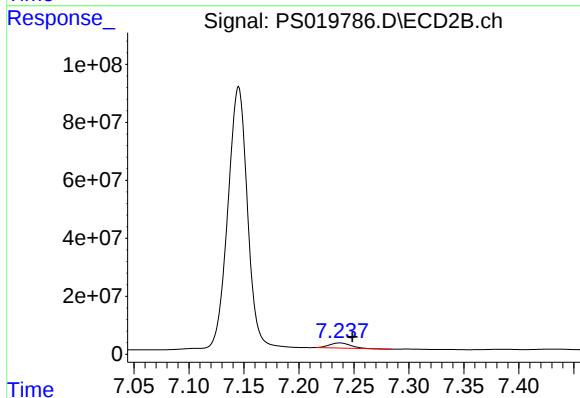


#7 MCPA

R.T.: 7.237 min
Delta R.T.: -0.011 min
Response: 23830692
Conc: 6.20 ug/ml

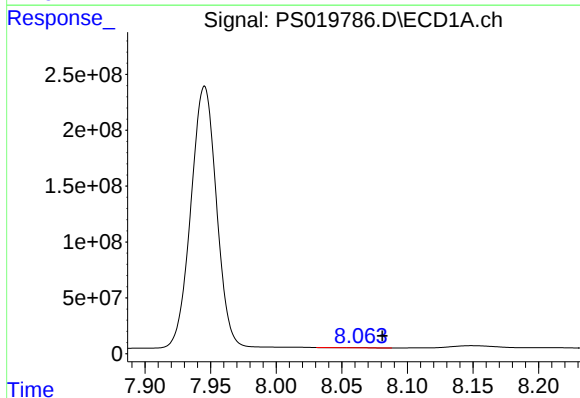


#8 DICHLORPROP

R.T.: 8.060 min
Delta R.T.: -0.021 min
Response: 1334541
Conc: N.D.

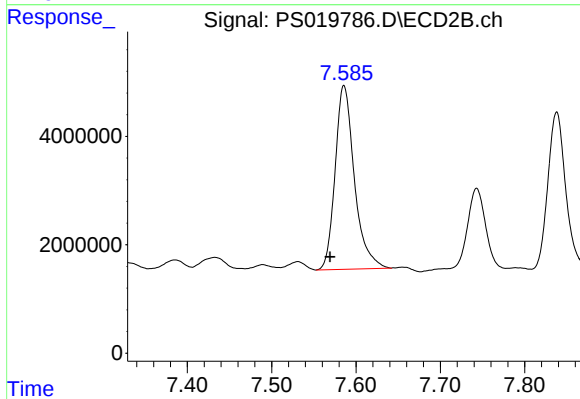

#8 DICHLORPROP


R.T.: 7.586 min
Delta R.T.: 0.017 min
Response: 53769369
Conc: 60.87 ng/ml

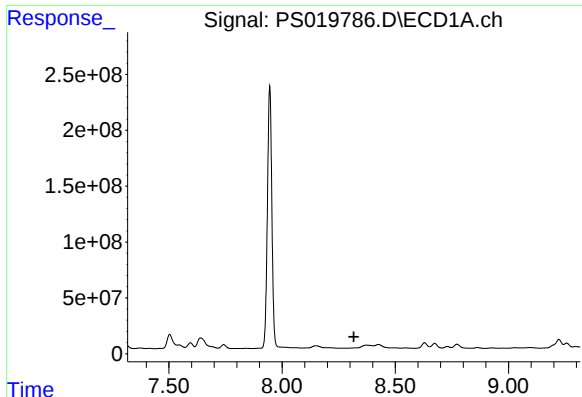

#9 2,4-D


R.T.: 8.372 min
Delta R.T.: 0.055 min
Response: -40519816
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

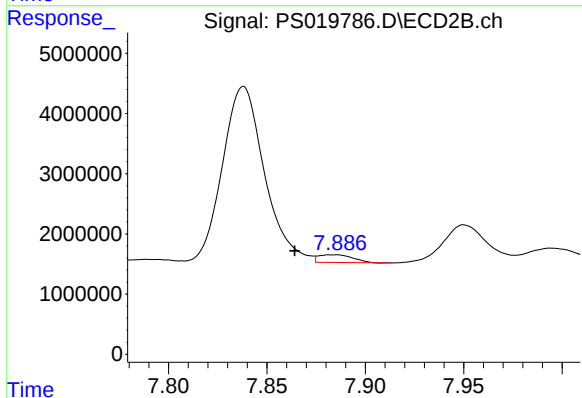


#9 2,4-D

R.T.: 7.885 min
Delta R.T.: 0.021 min
Response: 1528989
Conc: 1.43 ng/ml

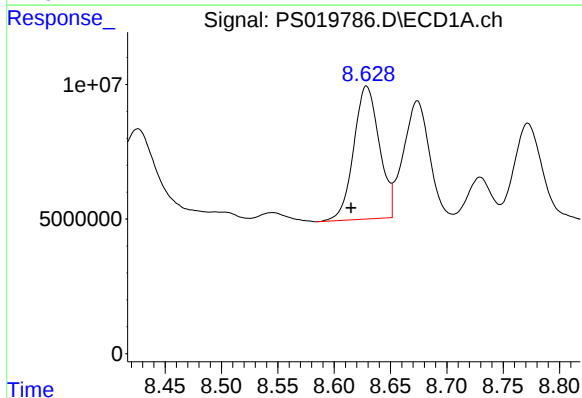


#10 Pentachlorophenol

R.T.: 8.629 min
Delta R.T.: 0.014 min
Response: 78169412
Conc: 2.26 ng/ml

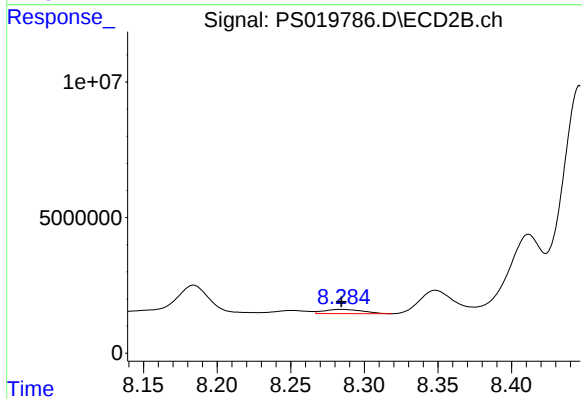

#10 Pentachlorophenol


R.T.: 8.285 min
Delta R.T.: 0.000 min
Response: 2827211
Conc: N.D.

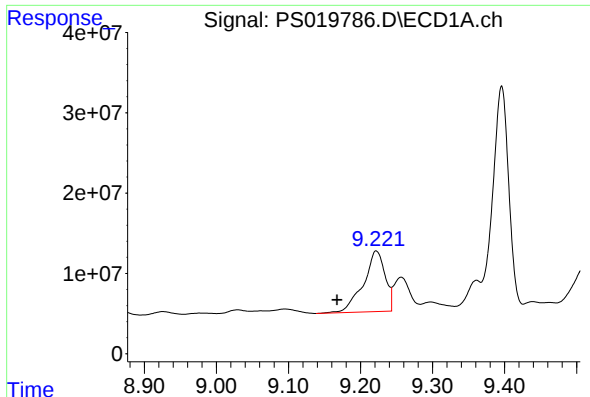

#11 2,4,5-TP (SILVEX)


R.T.: 9.222 min
Delta R.T.: 0.055 min
Response: 158031423
Conc: 10.07 ng/ml

Instrument :
FID_E
ClientSampleId :

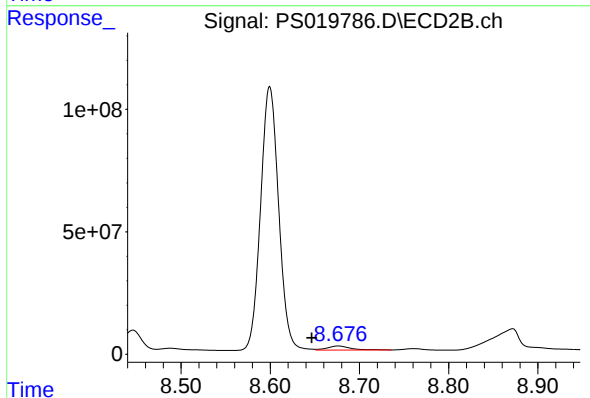


#11 2,4,5-TP (SILVEX)

R.T.: 8.676 min
Delta R.T.: 0.030 min
Response: 30603724
Conc: 6.09 ng/ml

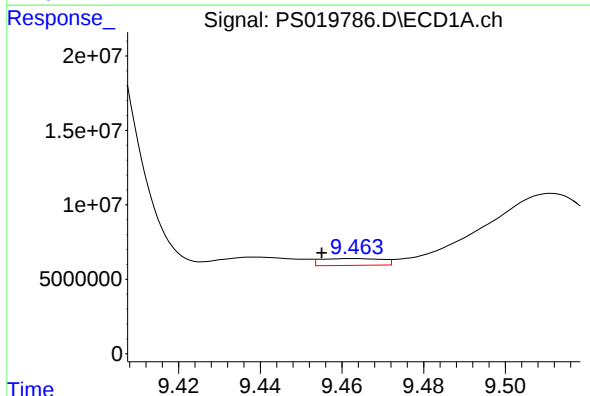


#12 2,4,5-T

R.T.: 9.462 min
Delta R.T.: 0.007 min
Response: 4719667
Conc: N.D.

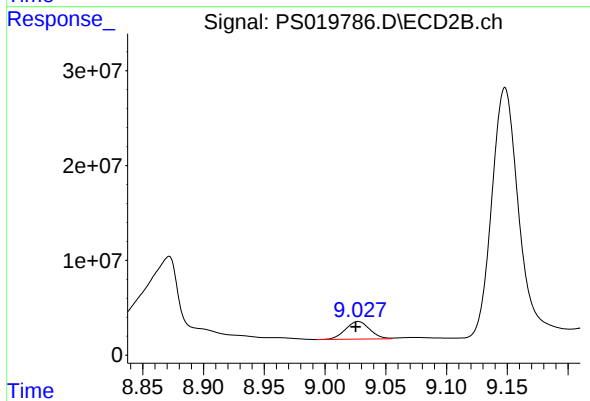

#12 2,4,5-T


R.T.: 9.027 min
Delta R.T.: 0.002 min
Response: 25674171
Conc: 5.46 ng/ml

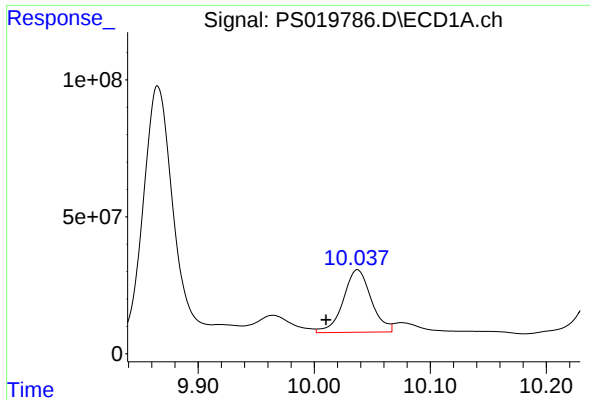

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: 0.027 min
Response: 382743117
Conc: 94.60 ng/ml

Instrument :
FID_E
ClientSampleId :

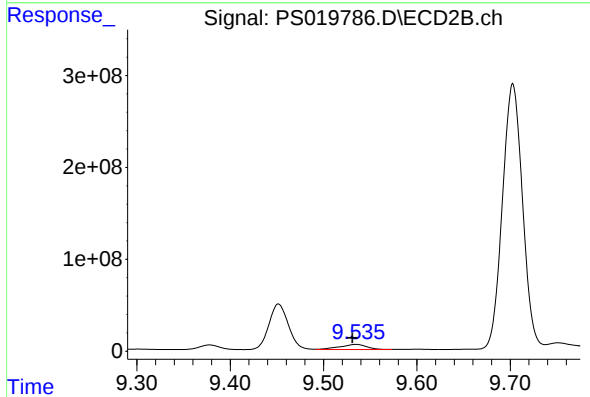


#13 2,4-DB

R.T.: 9.535 min
Delta R.T.: 0.004 min
Response: 114882489
Conc: 185.90 ng/ml

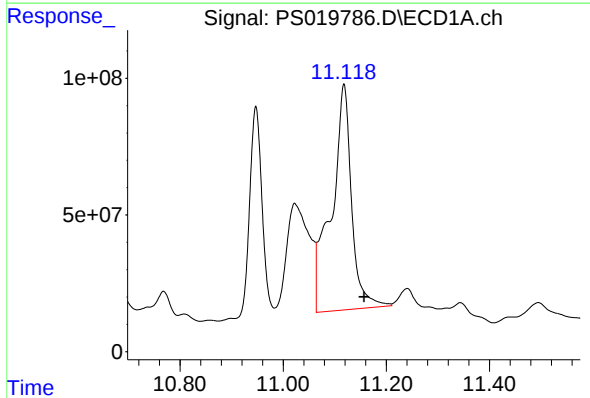


#14 DINOSEB

R.T.: 11.118 min
Delta R.T.: -0.039 min
Response: 2238382703
Conc: 144.72 ng/ml

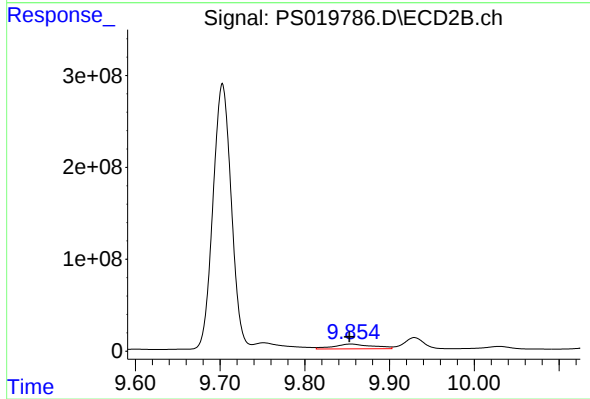

#14 DINOSEB


R.T.: 9.855 min
Delta R.T.: 0.002 min
Response: 165734418
Conc: 46.65 ng/ml

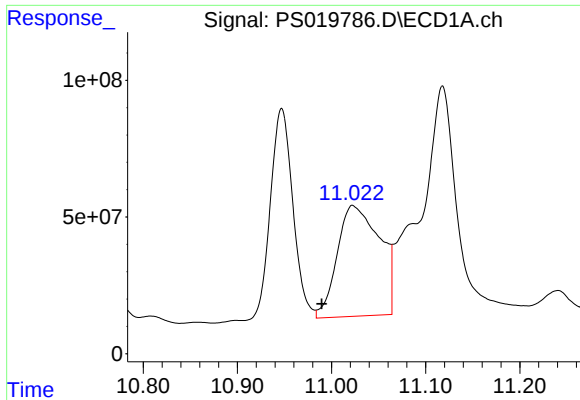

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.033 min
Response: 1265586565
Conc: 42.65 ng/ml

Instrument :
FID_E
ClientSampleId :

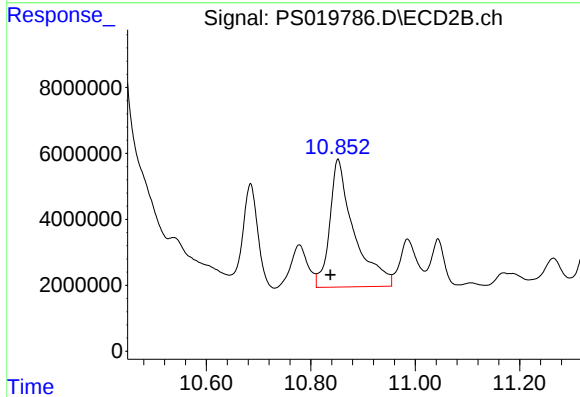


#15 Picloram

R.T.: 10.852 min
Delta R.T.: 0.015 min
Response: 124786267
Conc: 19.40 ng/ml

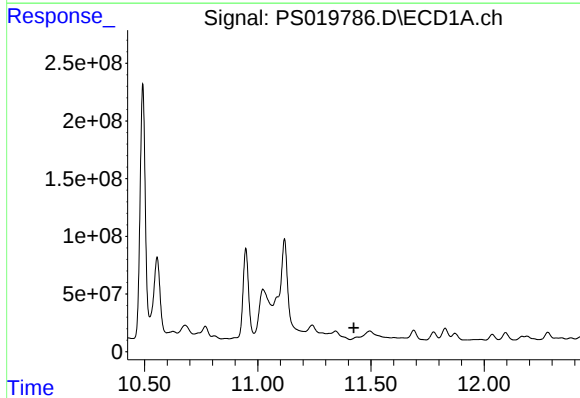

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.424 min
Response: 0
Conc: N.D.

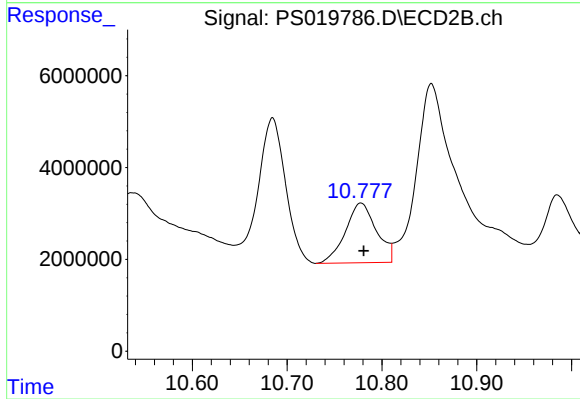

#16 DCPA

R.T.: 10.778 min
Delta R.T.: -0.003 min
Response: 29625378
Conc: 4.80 ng/ml