

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019789.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 00:40
 Operator : AJ\MA
 Sample : PB145801TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 25 01:08:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.192	6.778	1819.3E6	578.9E6	758.299	747.080
Target Compounds							
1) T	Dalapon	2.966f	2.485f	164.3E6	112.0E6	32.411	111.655 #
2) T	3,5-DICHL...	6.437	5.984	-2116893	105.9E6	N.D.	88.322
3) T	4-Nitroph...	7.076	6.444	601.2E6	75010008	612.656	175.242 #
5) T	DICAMBA	7.369	6.980	2919734	2668226	<MDL	<MDL #
6) T	MCP	7.544	7.051	12698660	361098	1.692	<MDL #
7) T	MCPA	7.692	7.231	72309491	5986594	6.693	1.558 #
8) T	DICHLORPROP	8.081	7.585	865894	29884015	<MDL	33.829 #
9) T	2,4-D	0.000	7.885	0	3514136	N.D.	3.295
10) T	Pentachlo...	8.628	8.291	29243667	1047563	<MDL	<MDL #
11) T	2,4,5-TP ...	9.221f	8.675	128.2E6	18413465	8.166	3.663 #
12) T	2,4,5-T	9.510f	9.026	72683814	18150574	3.862	3.859
13) T	2,4-DB	10.037	9.535	442.4E6	78324100	109.342	126.745
14) T	DINOSEB	11.117	9.886	2500.6E6	1559.7E6	161.672	439.032 #
15) T	Picloram	10.946f	10.847	1546.0E6	70011241	52.095	10.884 #
16) T	DCPA	11.429	10.778	1973040	23870716	<MDL	3.867 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019789.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 00:40
Operator : AJ\MA
Sample : PB145801TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 25 01:08:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

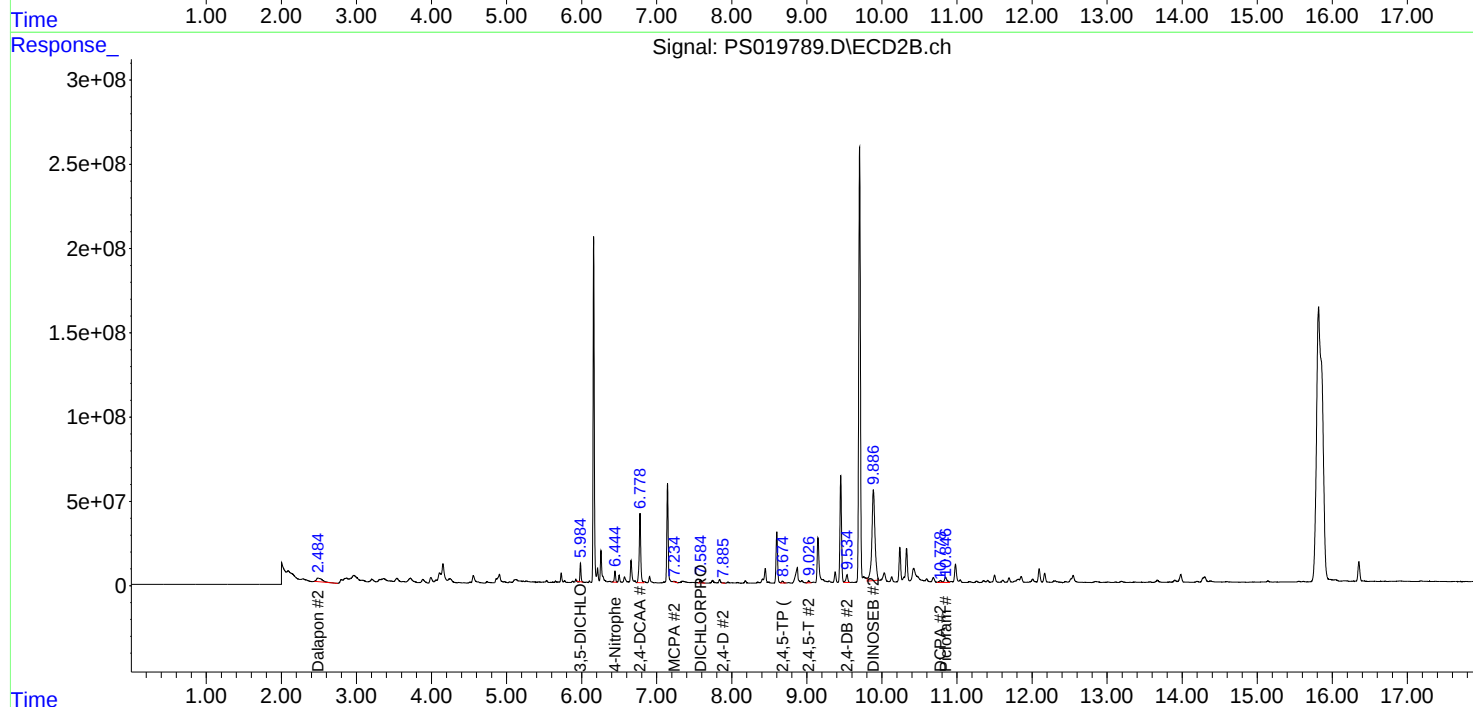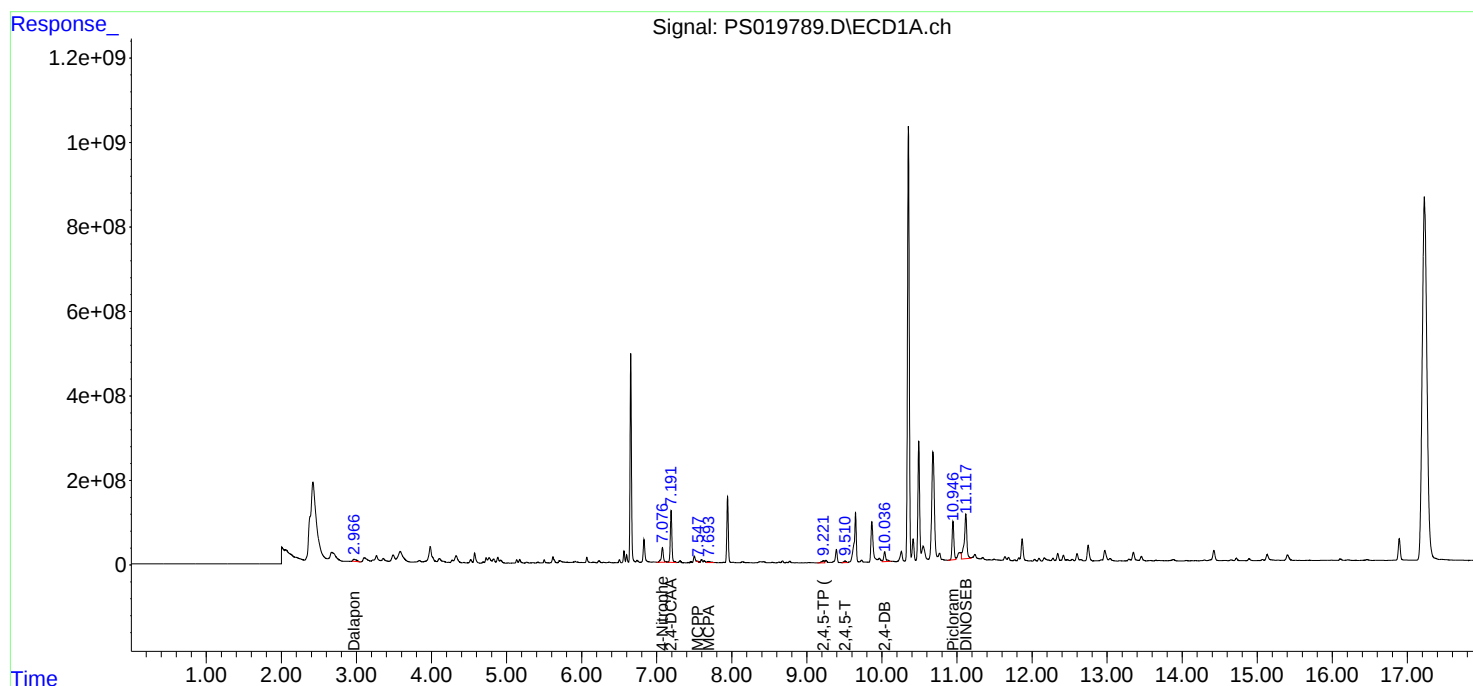


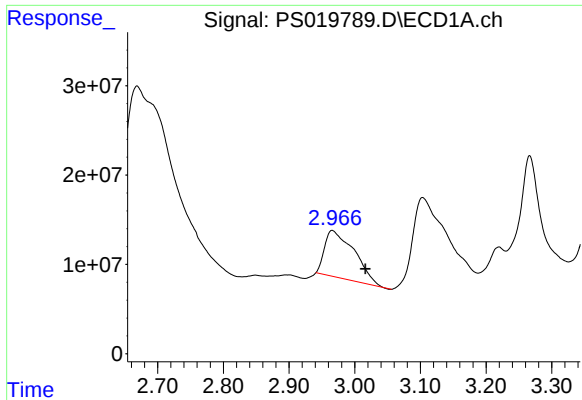

#1 Dalapon


R.T.: 2.966 min
Delta R.T.: -0.050 min
Response: 164281257
Conc: 32.41 ng/ml

Instrument :
FID_E
ClientSampleId :

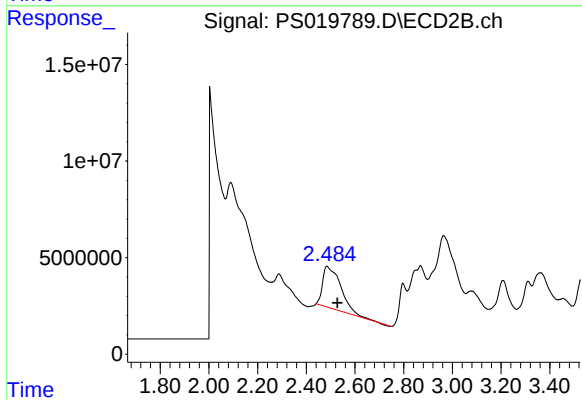


#1 Dalapon

R.T.: 2.485 min
Delta R.T.: -0.043 min
Response: 112039308
Conc: 111.66 ng/ml

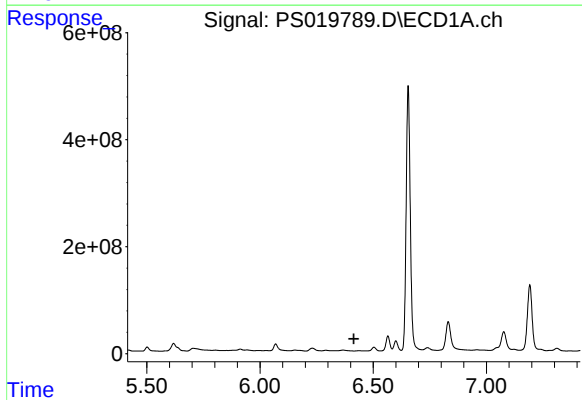


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.437 min
Delta R.T.: 0.023 min
Response: -2116893
Conc: N.D.

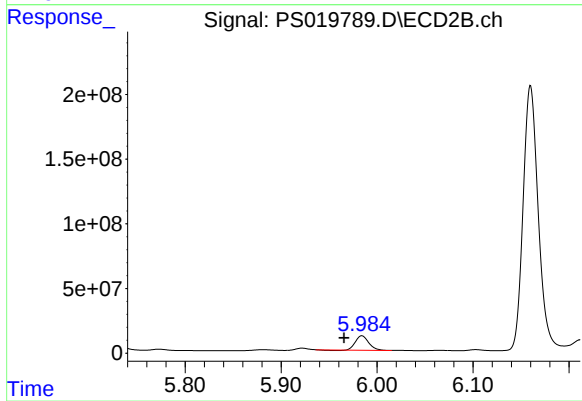

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.984 min
Delta R.T.: 0.019 min
Response: 105869747
Conc: 88.32 ng/ml

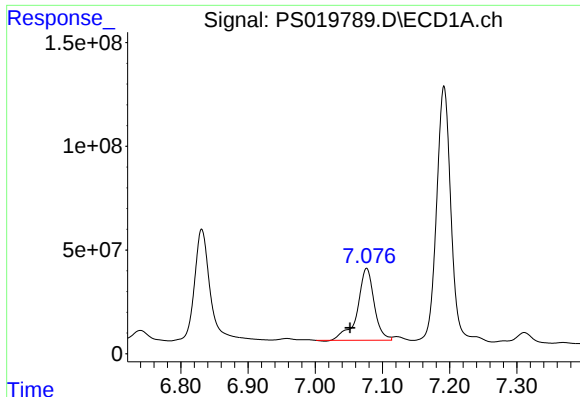

#3 4-Nitrophenol


R.T.: 7.076 min
Delta R.T.: 0.024 min
Response: 601209917
Conc: 612.66 ng/ml

Instrument :
FID_E
ClientSampleId :

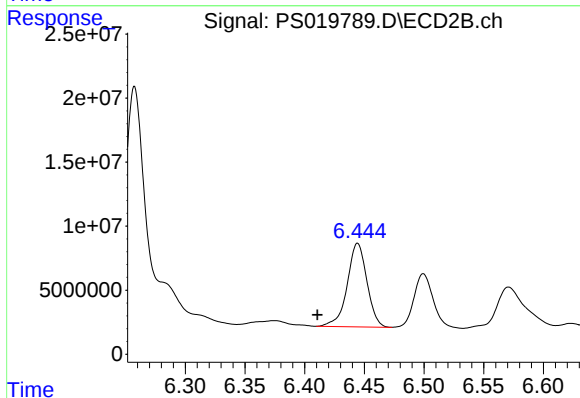


#3 4-Nitrophenol

R.T.: 6.444 min
Delta R.T.: 0.034 min
Response: 75010008
Conc: 175.24 ng/ml

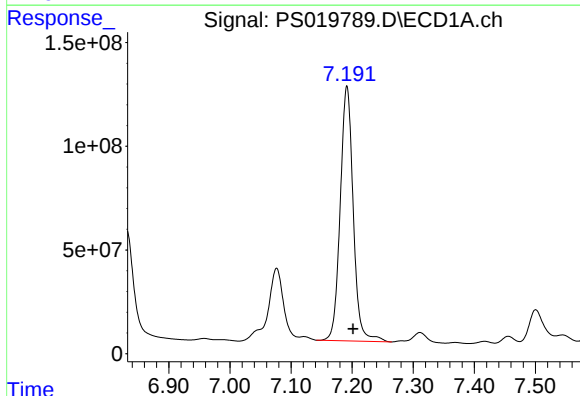


#4 2,4-DCAA

R.T.: 7.192 min
Delta R.T.: -0.010 min
Response: 1819285195
Conc: 758.30 ng/ml

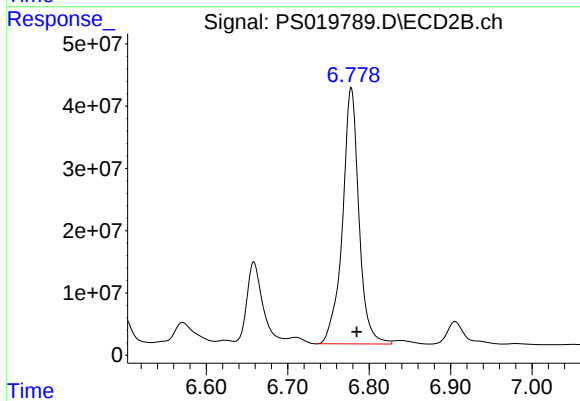

#4 2,4-DCAA


R.T.: 6.778 min
Delta R.T.: -0.007 min
Response: 578890479
Conc: 747.08 ng/ml

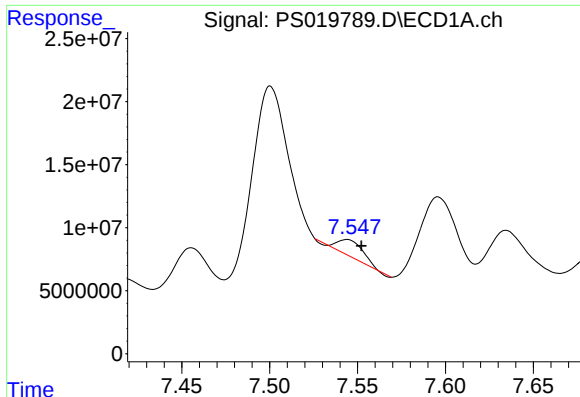

#6 MCPP


R.T.: 7.544 min
Delta R.T.: -0.008 min
Response: 12698660
Conc: 1.69 ug/ml

Instrument :
FID_E
ClientSampleId :

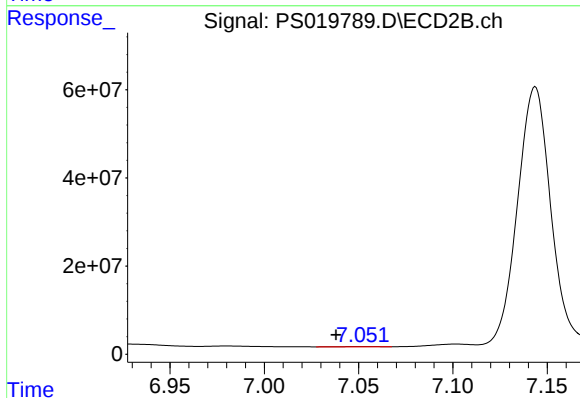


#6 MCPP

R.T.: 7.051 min
Delta R.T.: 0.013 min
Response: 361098
Conc: N.D.

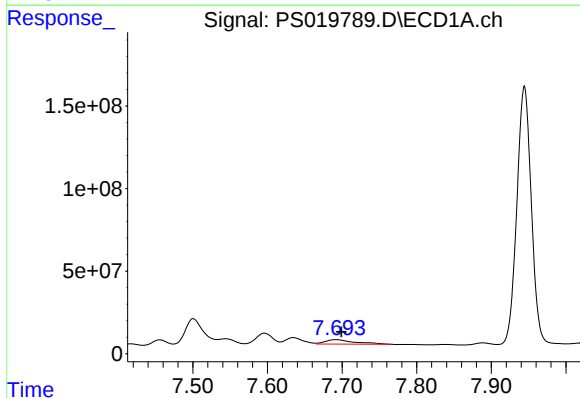


#7 MCPA

R.T.: 7.692 min
Delta R.T.: -0.007 min
Response: 72309491
Conc: 6.69 ug/ml

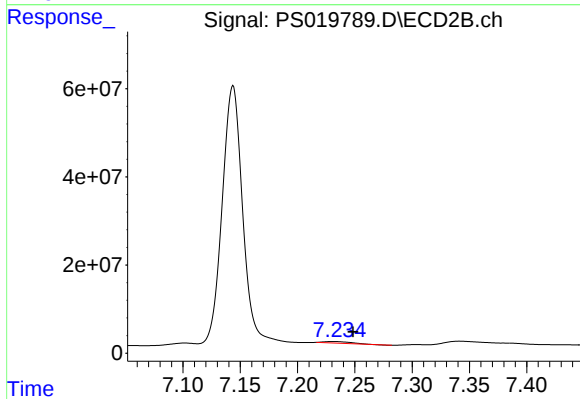

#7 MCPA


R.T.: 7.231 min
Delta R.T.: -0.017 min
Response: 5986594
Conc: 1.56 ug/ml

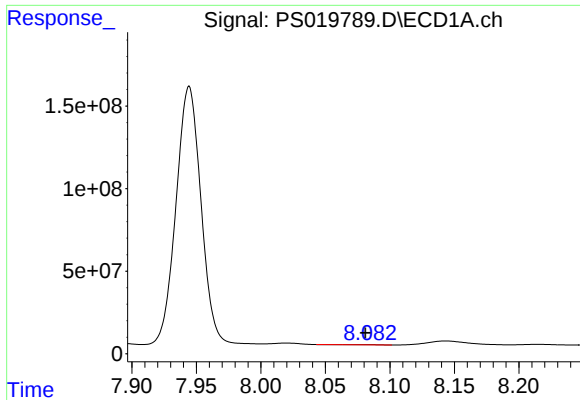

#8 DICHLORPROP


R.T.: 8.081 min
Delta R.T.: 0.000 min
Response: 865894
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

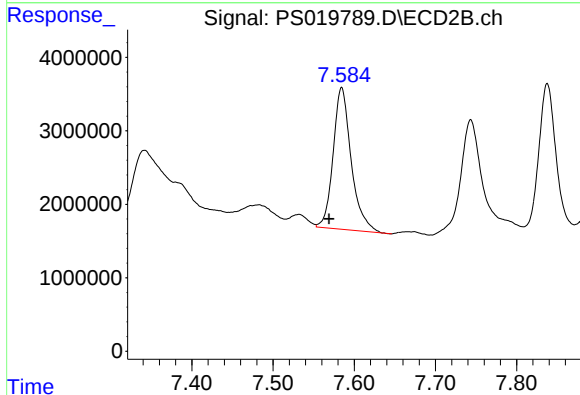


#8 DICHLORPROP

R.T.: 7.585 min
Delta R.T.: 0.015 min
Response: 29884015
Conc: 33.83 ng/ml

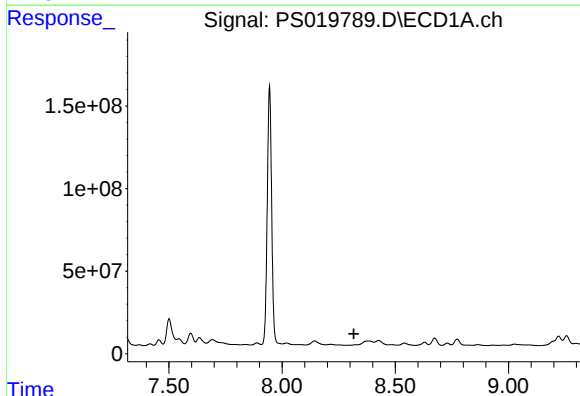


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.317 min
Response: 0
Conc: N.D.

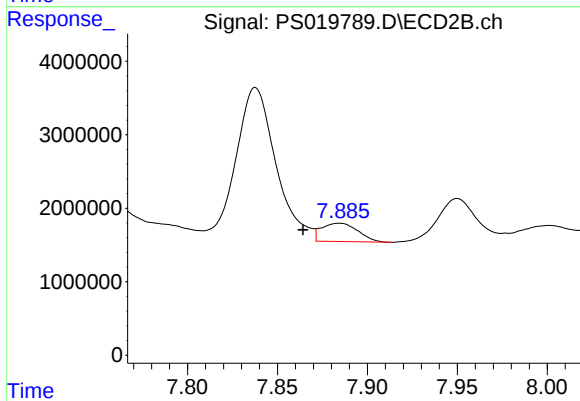

#9 2,4-D


R.T.: 7.885 min
Delta R.T.: 0.020 min
Response: 3514136
Conc: 3.29 ng/ml

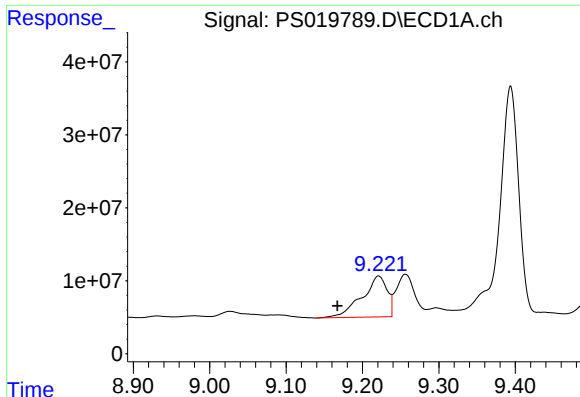

#11 2,4,5-TP (SILVEX)


R.T.: 9.221 min
Delta R.T.: 0.054 min
Response: 128212338
Conc: 8.17 ng/ml

Instrument :
FID_E
ClientSampleId :

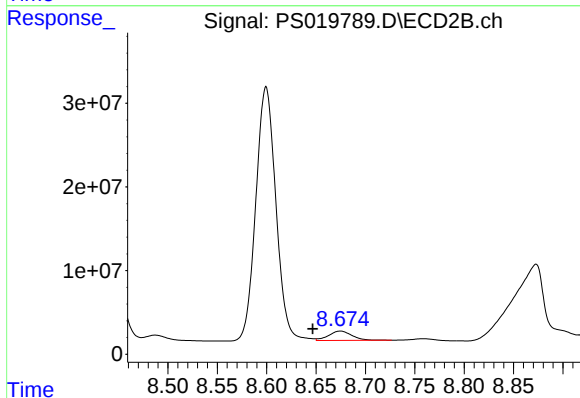


#11 2,4,5-TP (SILVEX)

R.T.: 8.675 min
Delta R.T.: 0.028 min
Response: 18413465
Conc: 3.66 ng/ml

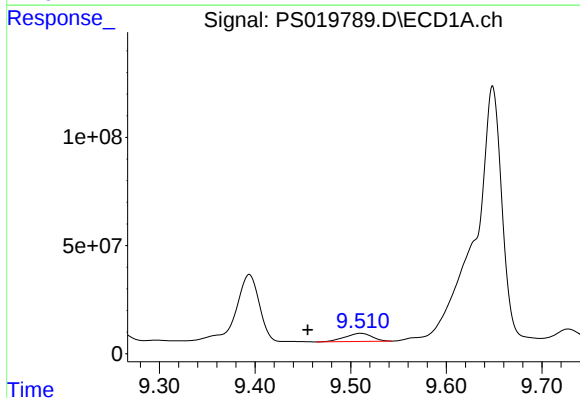


#12 2,4,5-T

R.T.: 9.510 min
Delta R.T.: 0.055 min
Response: 72683814
Conc: 3.86 ng/ml

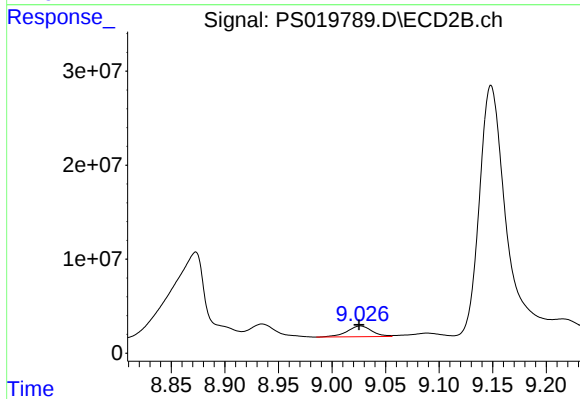

#12 2,4,5-T


R.T.: 9.026 min
Delta R.T.: 0.001 min
Response: 18150574
Conc: 3.86 ng/ml

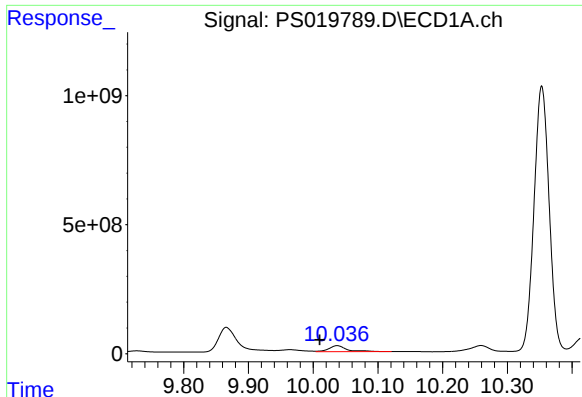

#13 2,4-DB


R.T.: 10.037 min
Delta R.T.: 0.027 min
Response: 442398088
Conc: 109.34 ng/ml

Instrument :
FID_E
ClientSampleId :

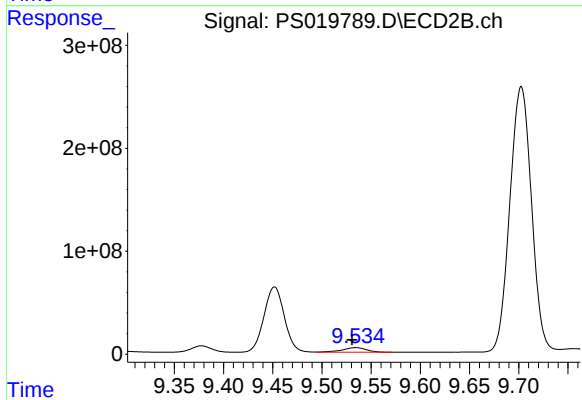


#13 2,4-DB

R.T.: 9.535 min
Delta R.T.: 0.004 min
Response: 78324100
Conc: 126.75 ng/ml

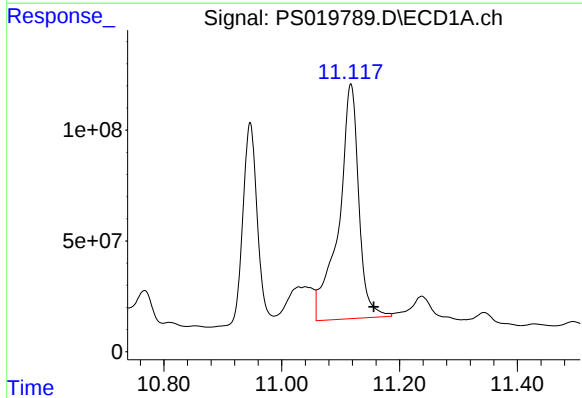


#14 DINOSEB

R.T.: 11.117 min
Delta R.T.: -0.039 min
Response: 2500603748
Conc: 161.67 ng/ml

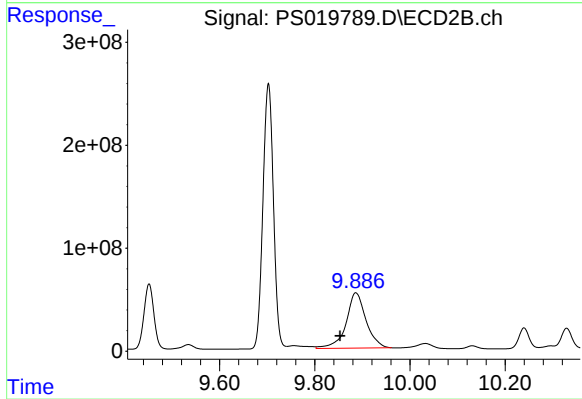

#14 DINOSEB


R.T.: 9.886 min
Delta R.T.: 0.033 min
Response: 1559714722
Conc: 439.03 ng/ml

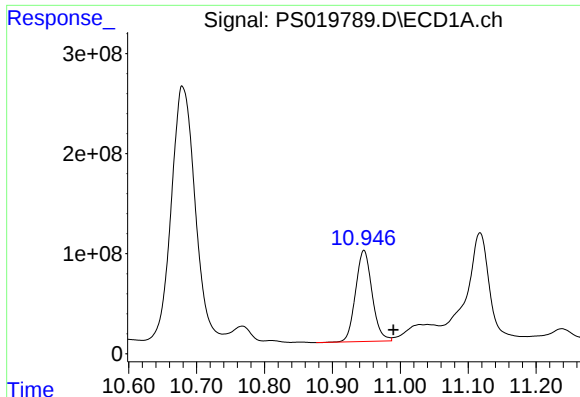

#15 Picloram


R.T.: 10.946 min
Delta R.T.: -0.043 min
Response: 1546030421
Conc: 52.09 ng/ml

Instrument :
FID_E
ClientSampleId :

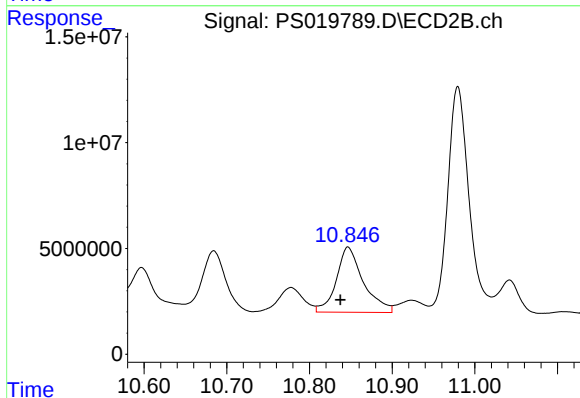


#15 Picloram

R.T.: 10.847 min
Delta R.T.: 0.009 min
Response: 70011241
Conc: 10.88 ng/ml

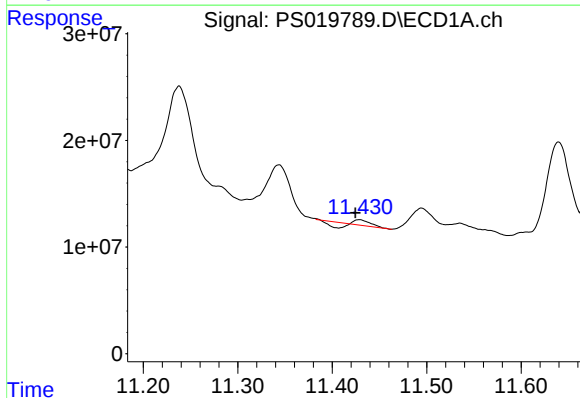

#16 DCPA

R.T.: 11.429 min
Delta R.T.: 0.004 min
Response: 1973040
Conc: N.D.

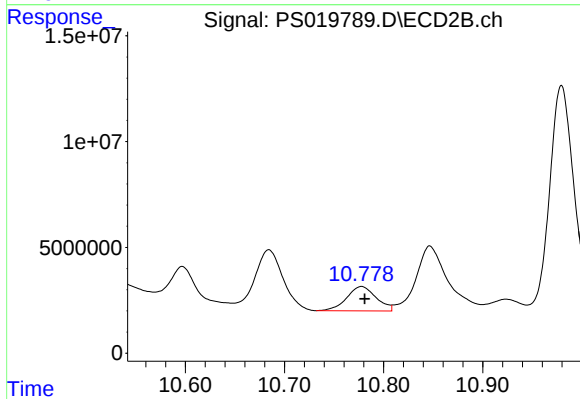

#16 DCPA

R.T.: 10.778 min
Delta R.T.: -0.003 min
Response: 23870716
Conc: 3.87 ng/ml