

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019797.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 05:50
 Operator : AJ\MA
 Sample : N3431-20
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 03:07:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.198	6.782	170.8E6	64650727	71.183	83.434
Target Compounds							
1) T	Dalapon	2.971f	2.490	7585179	2131353	1.496	2.124 #
2) T	3,5-DICHL...	0.000	5.986	0	10978853	N.D.	9.159
3) T	4-Nitroph...	7.029	6.425	232107	999260	<MDL	2.335 #
5) T	DICAMBA	7.368	6.953	1212799	1479434	<MDL	<MDL #
6) T	MCPD	7.542	0.000	2790161	0	<MDL	N.D. #
7) T	MCPA	7.693	0.000	365.5E6	0	33.830	N.D. #
8) T	DICHLORPROP	0.000	7.592	0	10675142	N.D.	12.085
10) T	Pentachlo...	8.611	0.000	537913	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.222f	8.681	18934715	14203393	1.206	2.825 #
12) T	2,4,5-T	9.440	9.025	1301772	1031922	<MDL	<MDL #
13) T	2,4-DB	10.038	9.535	37832722	6491786	9.351	10.505
14) T	DINOSEB	11.120	9.887	350.3E6	155.1E6	22.650	43.653 #
15) T	Picloram	11.024	10.863	112.7E6	17774719	3.798	2.763 #
16) T	DCPA	11.427	10.781	50852	2852351	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019797.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 05:50
Operator : AJ\MA
Sample : N3431-20
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 03:07:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

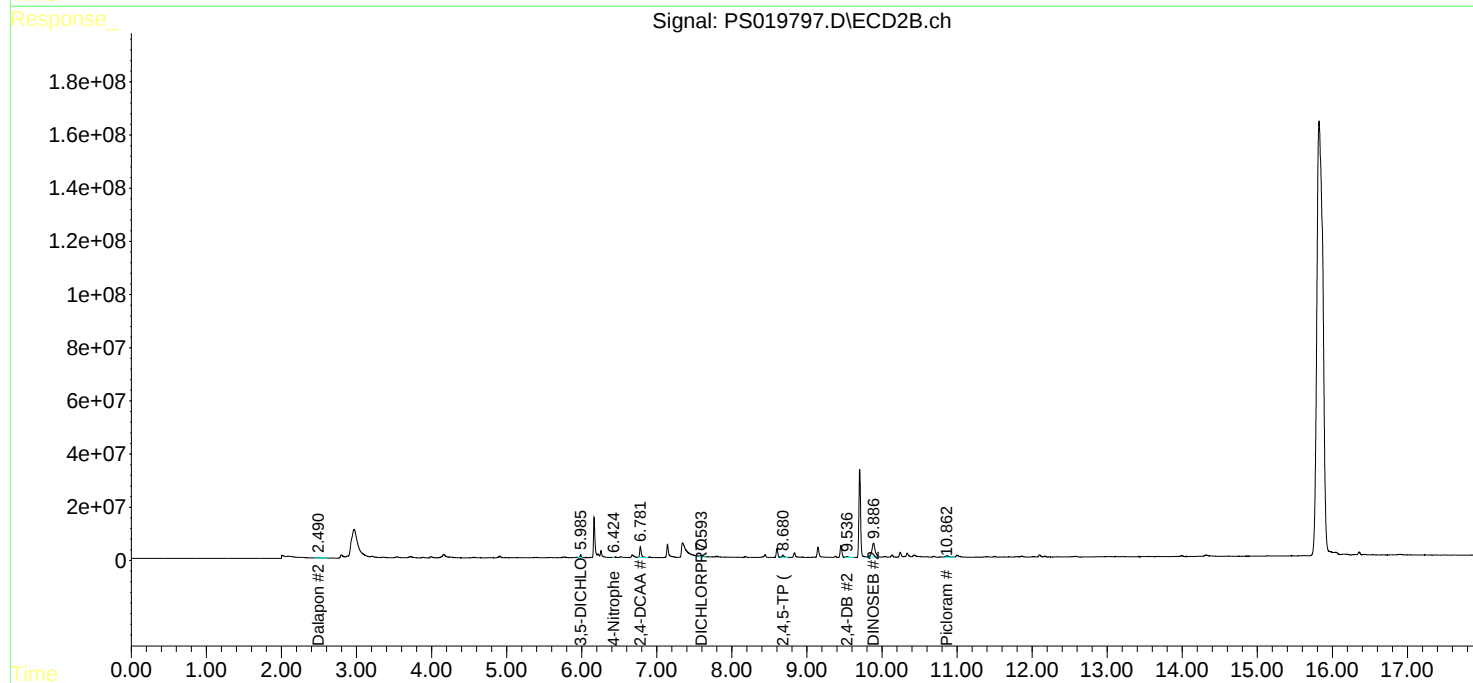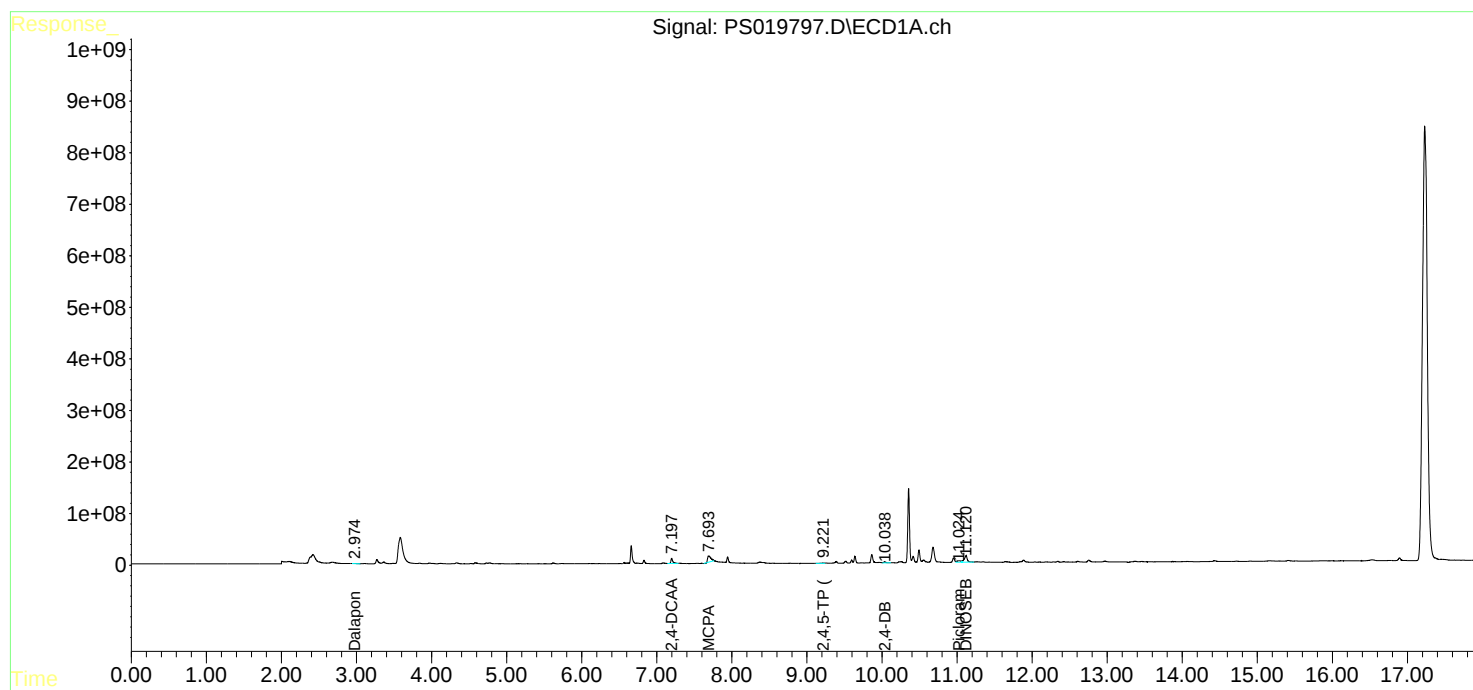


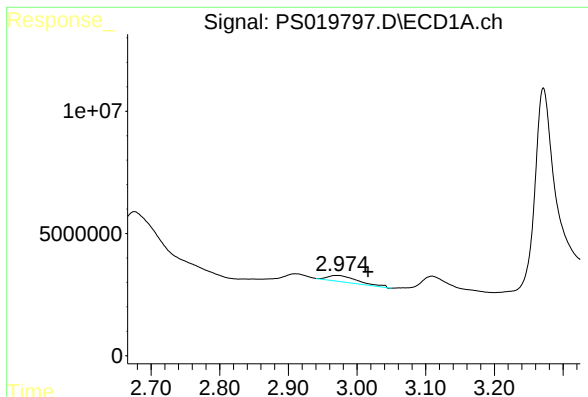

#1 Dalapon


R.T.: 2.971 min
Delta R.T.: -0.045 min
Response: 7585179
Conc: 1.50 ng/ml

Instrument :
FID_E
ClientSampleId :

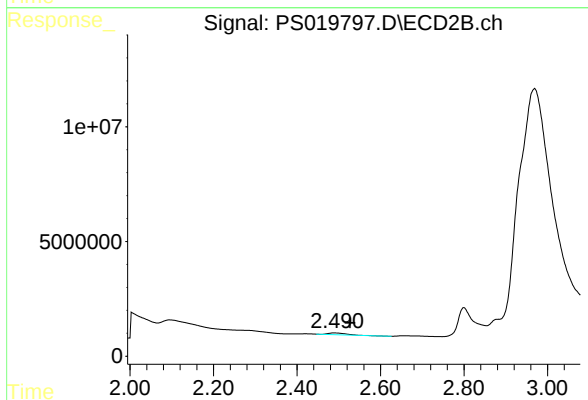


#1 Dalapon

R.T.: 2.490 min
Delta R.T.: -0.038 min
Response: 2131353
Conc: 2.12 ng/ml

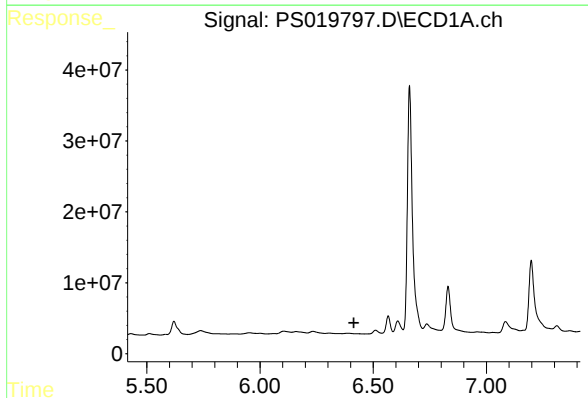


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.415 min
Response: 0
Conc: N.D.

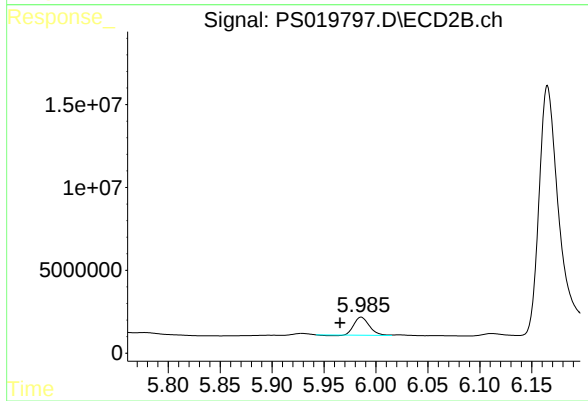

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.986 min
Delta R.T.: 0.020 min
Response: 10978853
Conc: 9.16 ng/ml

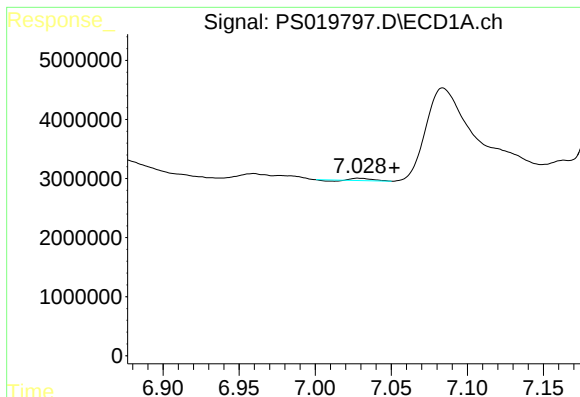

#3 4-Nitrophenol


R.T.: 7.029 min
Delta R.T.: -0.023 min
Response: 232107
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

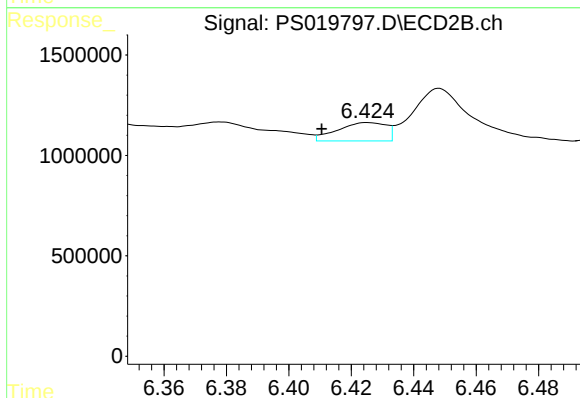


#3 4-Nitrophenol

R.T.: 6.425 min
Delta R.T.: 0.015 min
Response: 999260
Conc: 2.33 ng/ml

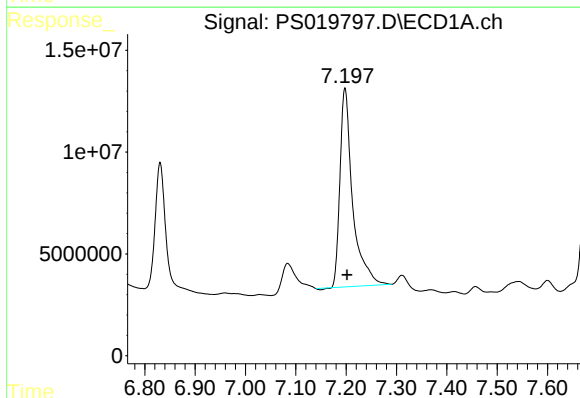


#4 2,4-DCAA

R.T.: 7.198 min
Delta R.T.: -0.004 min
Response: 170780297
Conc: 71.18 ng/ml

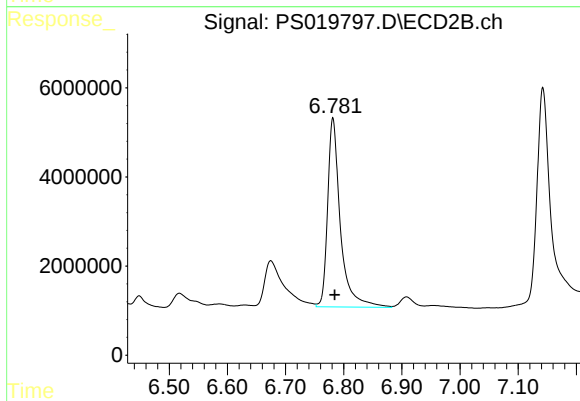

#4 2,4-DCAA


R.T.: 6.782 min
Delta R.T.: -0.003 min
Response: 64650727
Conc: 83.43 ng/ml

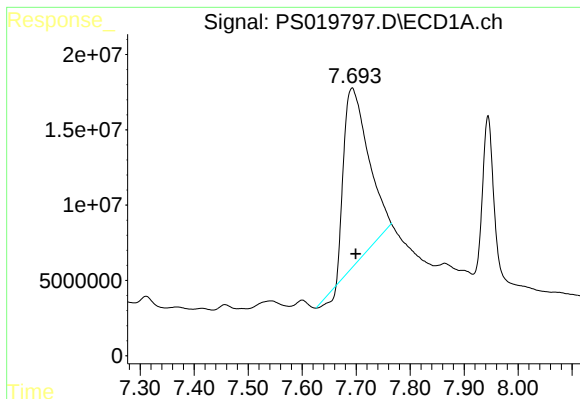

#7 MCPA


R.T.: 7.693 min
Delta R.T.: -0.007 min
Response: 365499955
Conc: 33.83 ug/ml

Instrument :
FID_E
ClientSampleId :

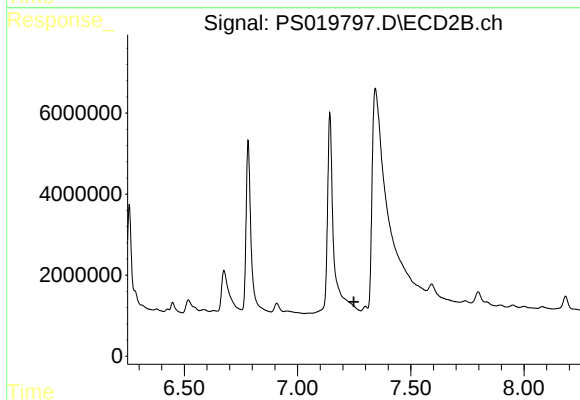


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.249 min
Response: 0
Conc: N.D.

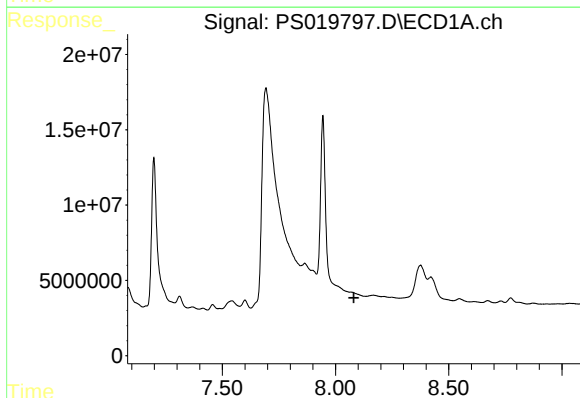


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.081 min
Response: 0
Conc: N.D.

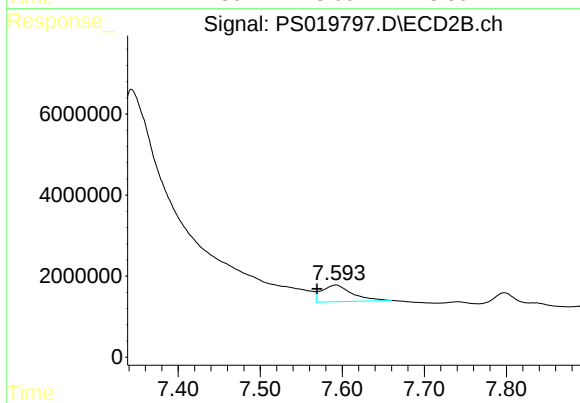

#8 DICHLORPROP


R.T.: 7.592 min
Delta R.T.: 0.023 min
Response: 10675142
Conc: 12.08 ng/ml

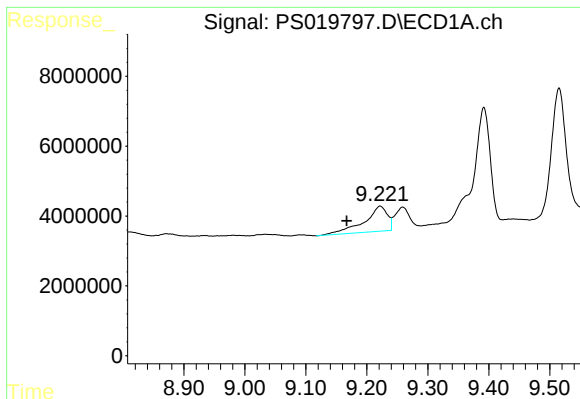

#11 2,4,5-TP (SILVEX)


R.T.: 9.222 min
Delta R.T.: 0.055 min
Response: 18934715
Conc: 1.21 ng/ml

Instrument :
FID_E
ClientSampleId :

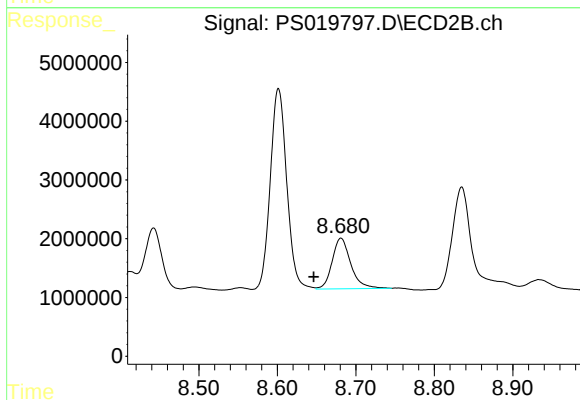


#11 2,4,5-TP (SILVEX)

R.T.: 8.681 min
Delta R.T.: 0.035 min
Response: 14203393
Conc: 2.83 ng/ml

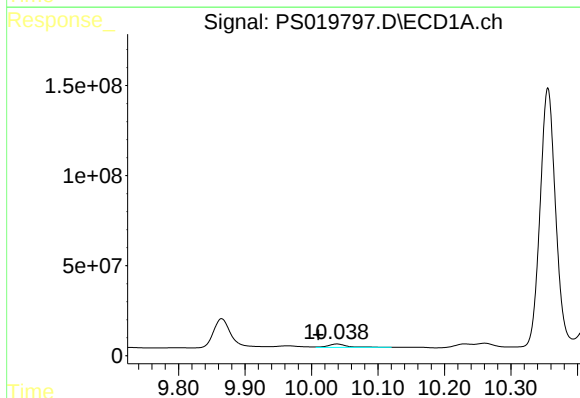


#13 2,4-DB

R.T.: 10.038 min
Delta R.T.: 0.028 min
Response: 37832722
Conc: 9.35 ng/ml

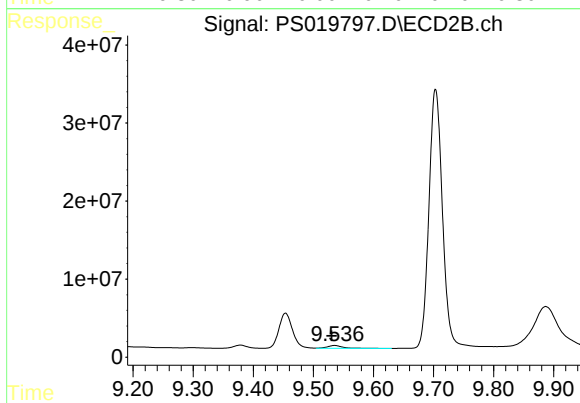

#13 2,4-DB


R.T.: 9.535 min
Delta R.T.: 0.005 min
Response: 6491786
Conc: 10.51 ng/ml

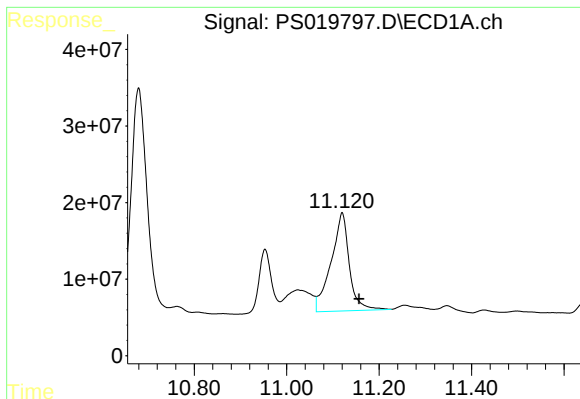

#14 DINOSEB


R.T.: 11.120 min
Delta R.T.: -0.037 min
Response: 350333945
Conc: 22.65 ng/ml

Instrument :
FID_E
ClientSampleId :

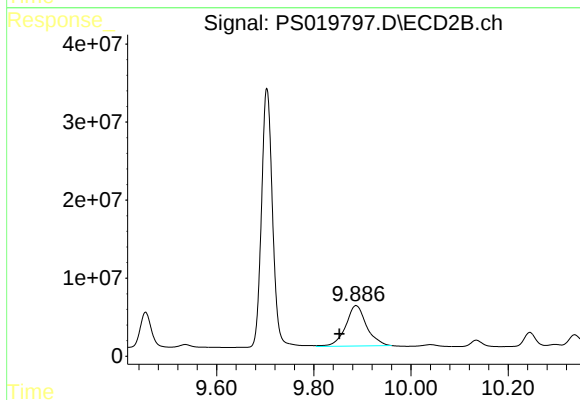


#14 DINOSEB

R.T.: 9.887 min
Delta R.T.: 0.034 min
Response: 155082550
Conc: 43.65 ng/ml

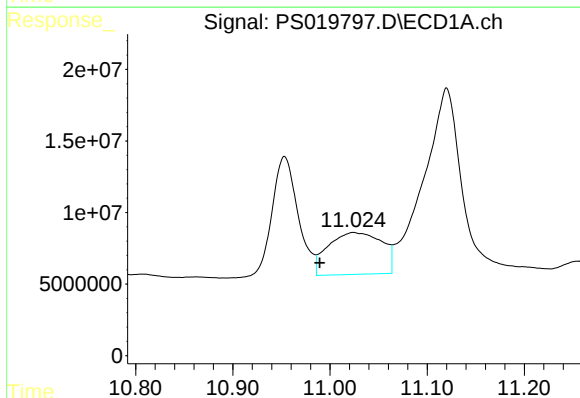

#15 Picloram

R.T.: 11.024 min
Delta R.T.: 0.035 min
Response: 112707276
Conc: 3.80 ng/ml

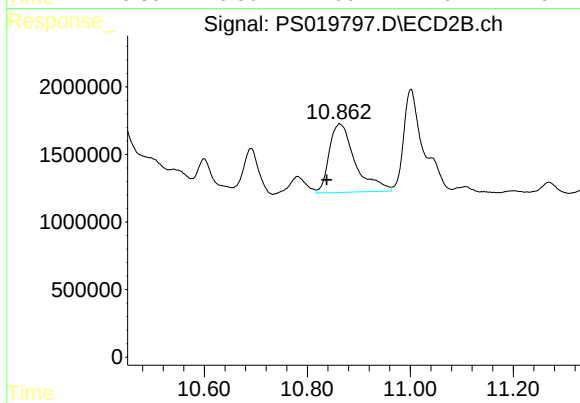

#15 Picloram

R.T.: 10.863 min
Delta R.T.: 0.025 min
Response: 17774719
Conc: 2.76 ng/ml