

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
 Data File : PS019801.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Jun 2022 07:26
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jun 27 03:09:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
 Quant Title : 8080.M
 QLast Update : Wed May 25 02:05:34 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.195	6.779	1178.4E6	458.9E6	491.154	592.236
Target Compounds							
1) T	Dalapon	3.019	0.000	1546911	0	<MDL	N.D. #
2) T	3,5-DICHL...	6.450	0.000	754404	0	<MDL	N.D. #
3) T	4-Nitroph...	6.985f	0.000	2641234	0	2.692	N.D. #
5) T	DICAMBA	0.000	7.004f	0	1160939	N.D.	<MDL
6) T	MCP	0.000	7.004	0	1160939	N.D.	<MDL
7) T	MCPA	7.675	0.000	7493515	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.613f	0	2614051	N.D.	2.959
10) T	Pentachlo...	8.613	8.281	2163011	1557832	<MDL	<MDL #
11) T	2,4,5-TP ...	9.173	8.645	2997447	415640	<MDL	<MDL #
12) T	2,4,5-T	9.467	9.041	8888144	674072	<MDL	<MDL #
13) T	2,4-DB	10.030	9.549	4794742	430083	1.185	<MDL #
14) T	DINOSEB	11.108f	9.855	14351386	404712	<MDL	<MDL #
15) T	Picloram	11.023	10.871	39145919	17436620	1.319	2.711 #
16) T	DCPA	11.420	10.776	2789062	10949928	<MDL	1.774 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS062422\
Data File : PS019801.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Jun 2022 07:26
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jun 27 03:09:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS052422.M
Quant Title : 8080.M
QLast Update : Wed May 25 02:05:34 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

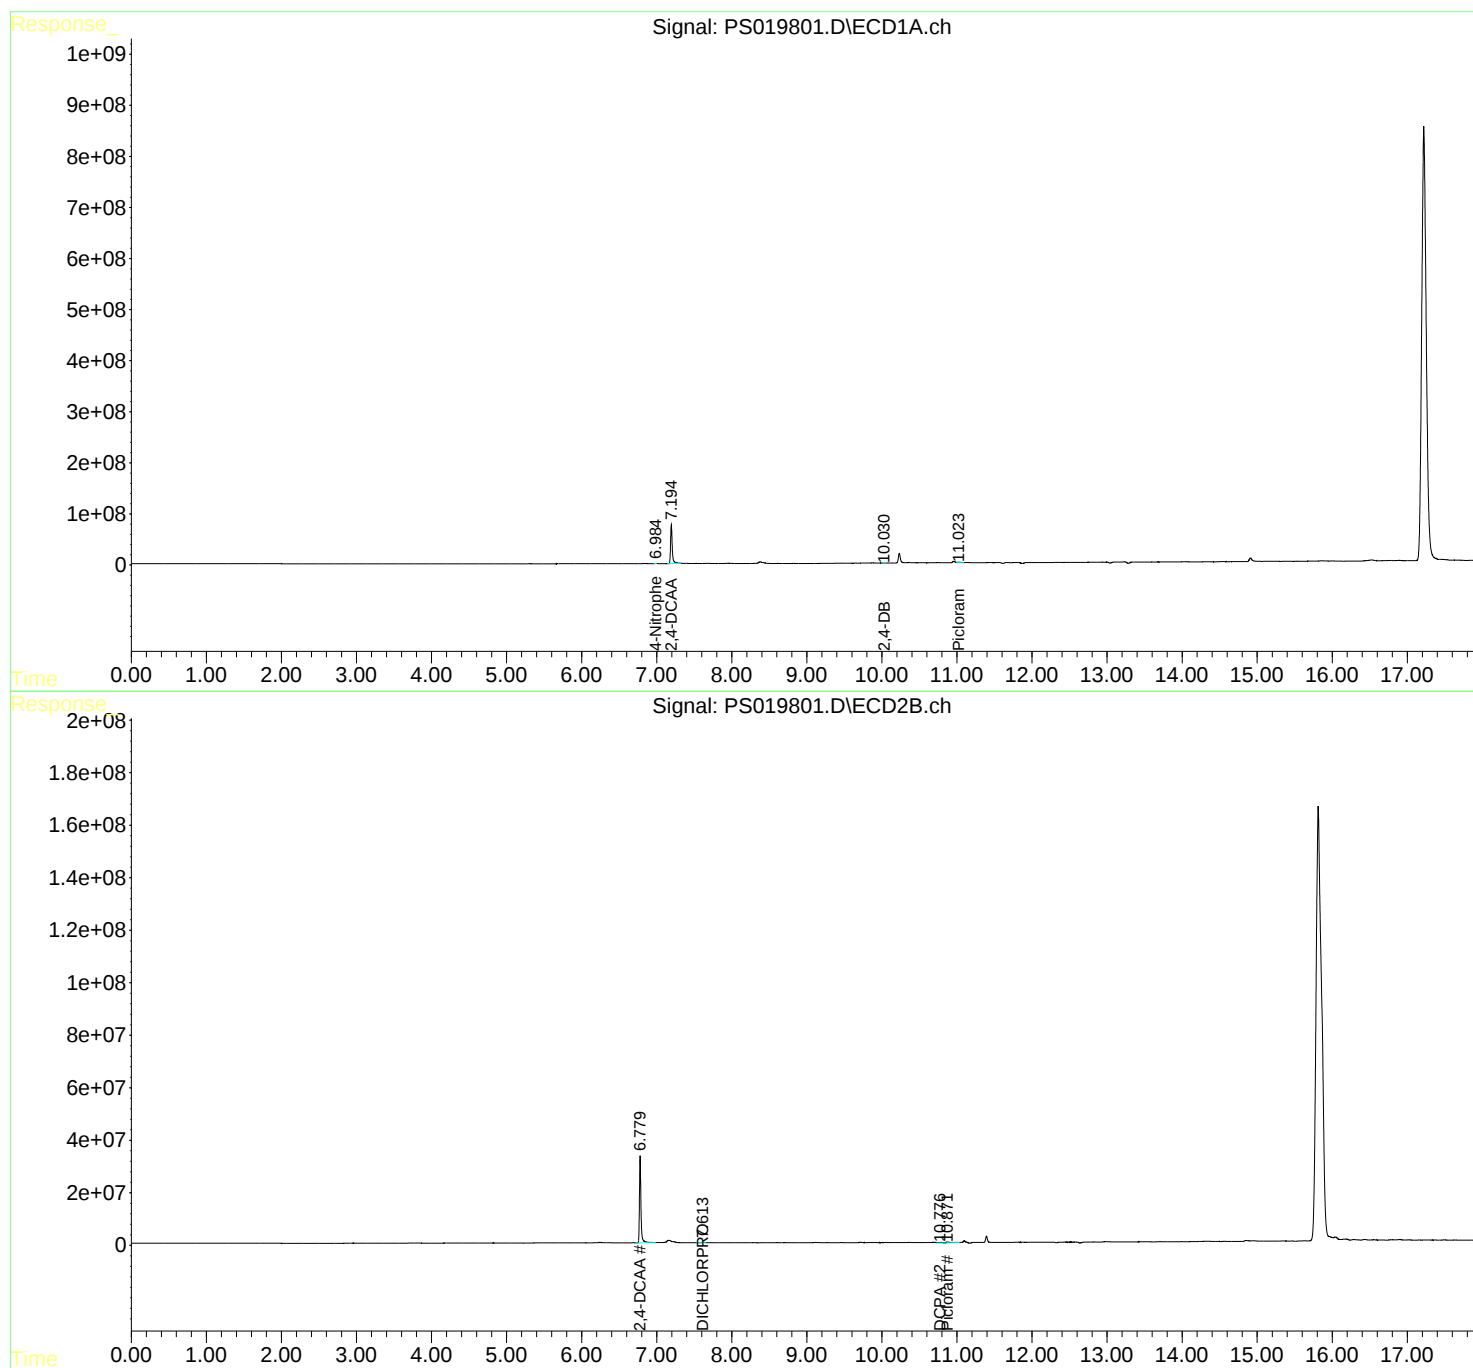


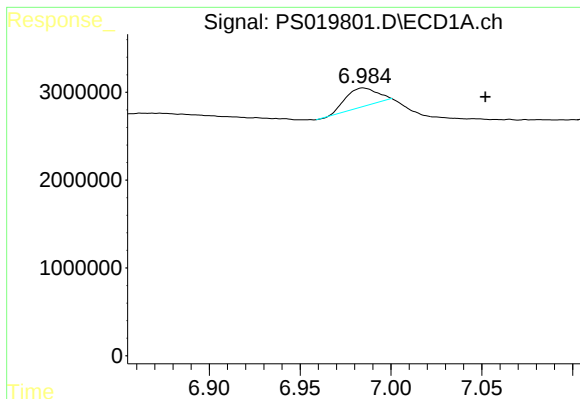

#3 4-Nitrophenol


R.T.: 6.985 min
Delta R.T.: -0.067 min
Response: 2641234
Conc: 2.69 ng/ml

Instrument :
FID_E
ClientSampleId :

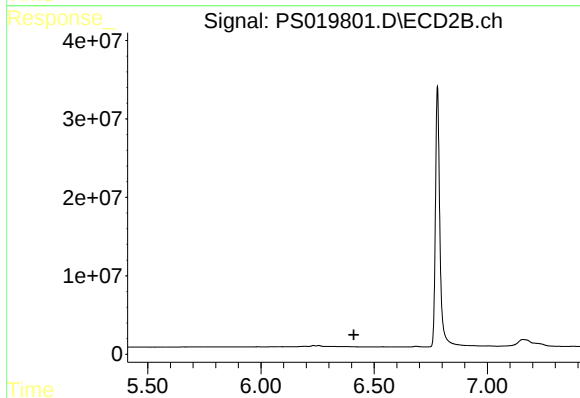


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.411 min
Response: 0
Conc: N.D.

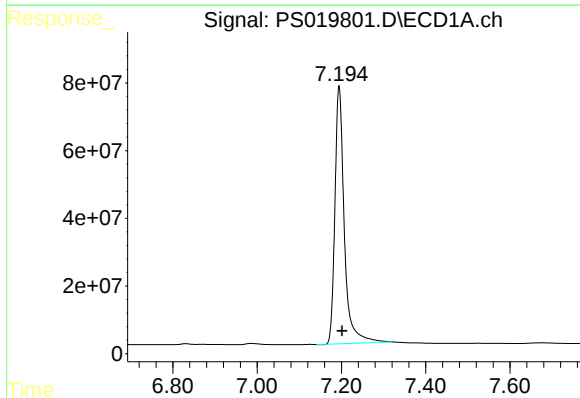


#4 2,4-DCAA

R.T.: 7.195 min
Delta R.T.: -0.007 min
Response: 1178360445
Conc: 491.15 ng/ml

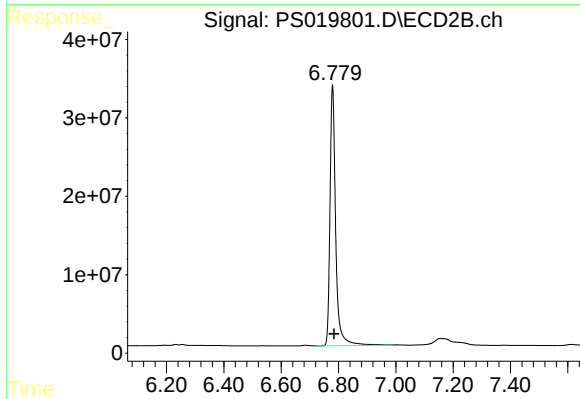

#4 2,4-DCAA


R.T.: 6.779 min
Delta R.T.: -0.005 min
Response: 458905828
Conc: 592.24 ng/ml

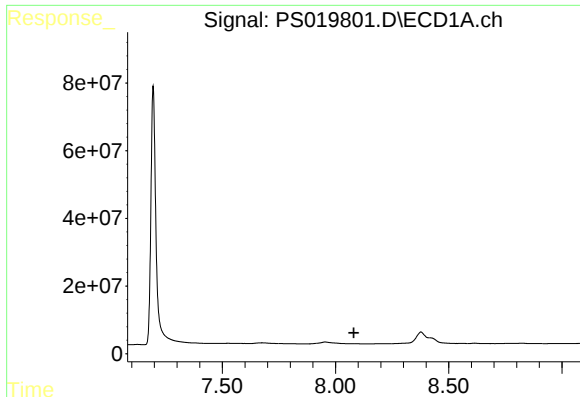

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.081 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

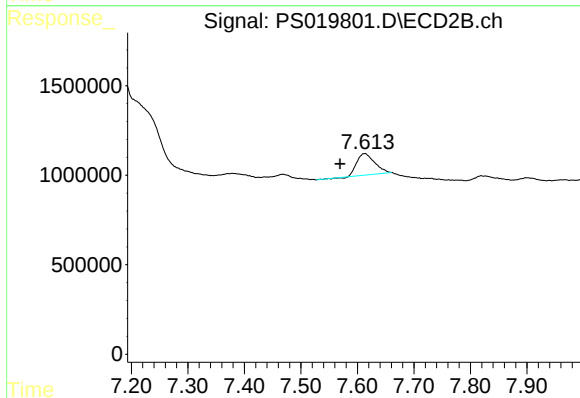


#8 DICHLORPROP

R.T.: 7.613 min
Delta R.T.: 0.044 min
Response: 2614051
Conc: 2.96 ng/ml

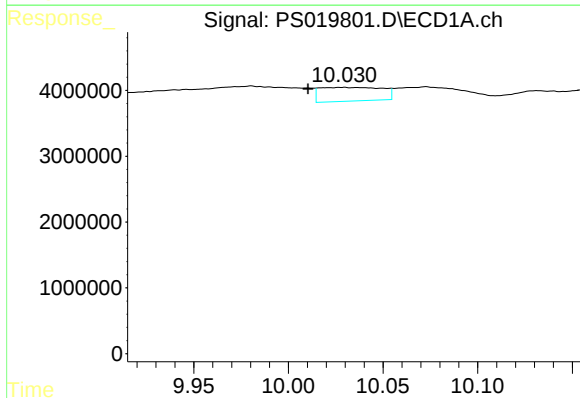


#13 2,4-DB

R.T.: 10.030 min
Delta R.T.: 0.019 min
Response: 4794742
Conc: 1.19 ng/ml

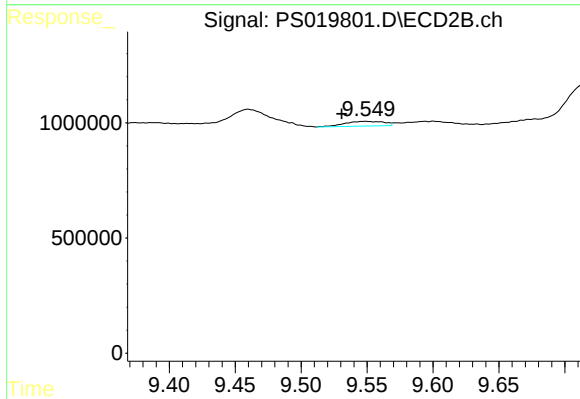

#13 2,4-DB


R.T.: 9.549 min
Delta R.T.: 0.018 min
Response: 430083
Conc: N.D.

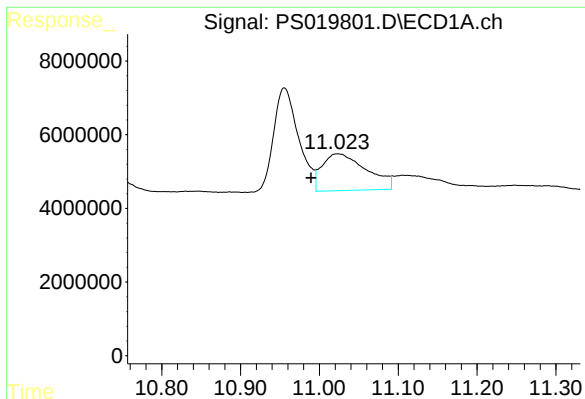

#15 Picloram


R.T.: 11.023 min
Delta R.T.: 0.034 min
Response: 39145919
Conc: 1.32 ng/ml

Instrument :
FID_E
ClientSampleId :

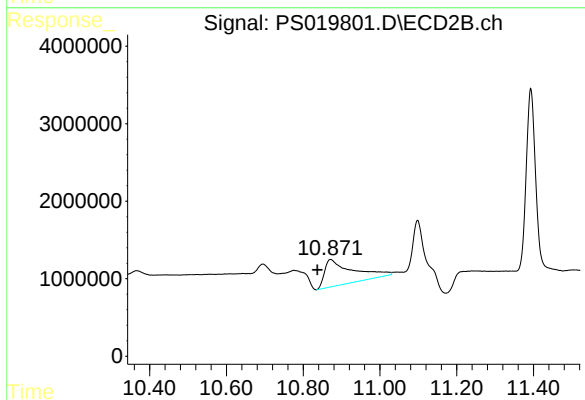


#15 Picloram

R.T.: 10.871 min
Delta R.T.: 0.034 min
Response: 17436620
Conc: 2.71 ng/ml

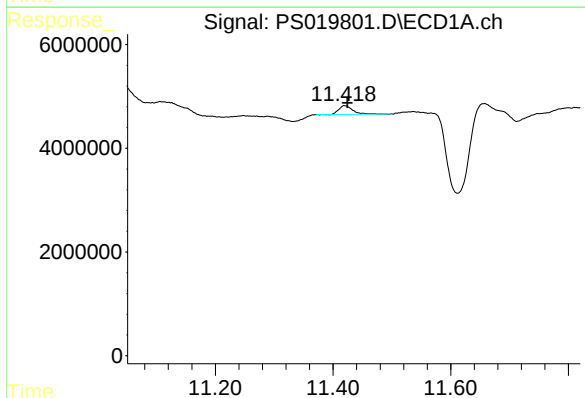

#16 DCPA

R.T.: 11.420 min
Delta R.T.: -0.004 min
Response: 2789062
Conc: N.D.

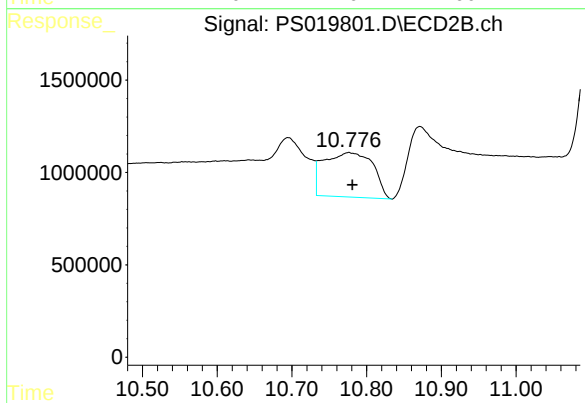

#16 DCPA

R.T.: 10.776 min
Delta R.T.: -0.005 min
Response: 10949928
Conc: 1.77 ng/ml