

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE062422AL\  
 Data File : FE036189.D  
 Signal(s) : FID1B.ch  
 Acq On : 24 Jun 2022 18:17  
 Operator : YP\AJ  
 Sample : N3422-05D  
 Misc :  
 ALS Vial : 9 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 WC-14A-1A-12-GR

Manual Integrations  
 APPROVED

Reviewed By :Yogesh Patel 06/27/2022  
 Supervised By :Ankita Jodhani 06/27/2022

Integration File: autoint1.e  
 Quant Time: Jun 24 23:41:37 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062022.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jun 21 03:08:45 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units    |
|--------------------------------|--------|------------|---------------|
| -----                          |        |            |               |
| System Monitoring Compounds    |        |            |               |
| 12) S 1-chlorooctadecane (S... | 13.313 | 6871705    | 44.386 ug/mlm |
| Spiked Amount 50.000           |        | Recovery = | 88.77%        |

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE062422AL\  
Data File : FE036189.D  
Signal(s) : FID1B.ch  
Acq On : 24 Jun 2022 18:17  
Operator : YP\AJ  
Sample : N3422-05D  
Misc :  
ALS Vial : 9 Sample Multiplier: 1


Instrument :  
FID\_E  
ClientSampleId :  
WC-14A-1A-12-GR


Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/27/2022  
Supervised By :Ankita Jodhani 06/27/2022

Integration File: autoint1.e  
Quant Time: Jun 24 23:41:37 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062022.M  
Quant Title : GC Extractables  
QLast Update : Tue Jun 21 03:08:45 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

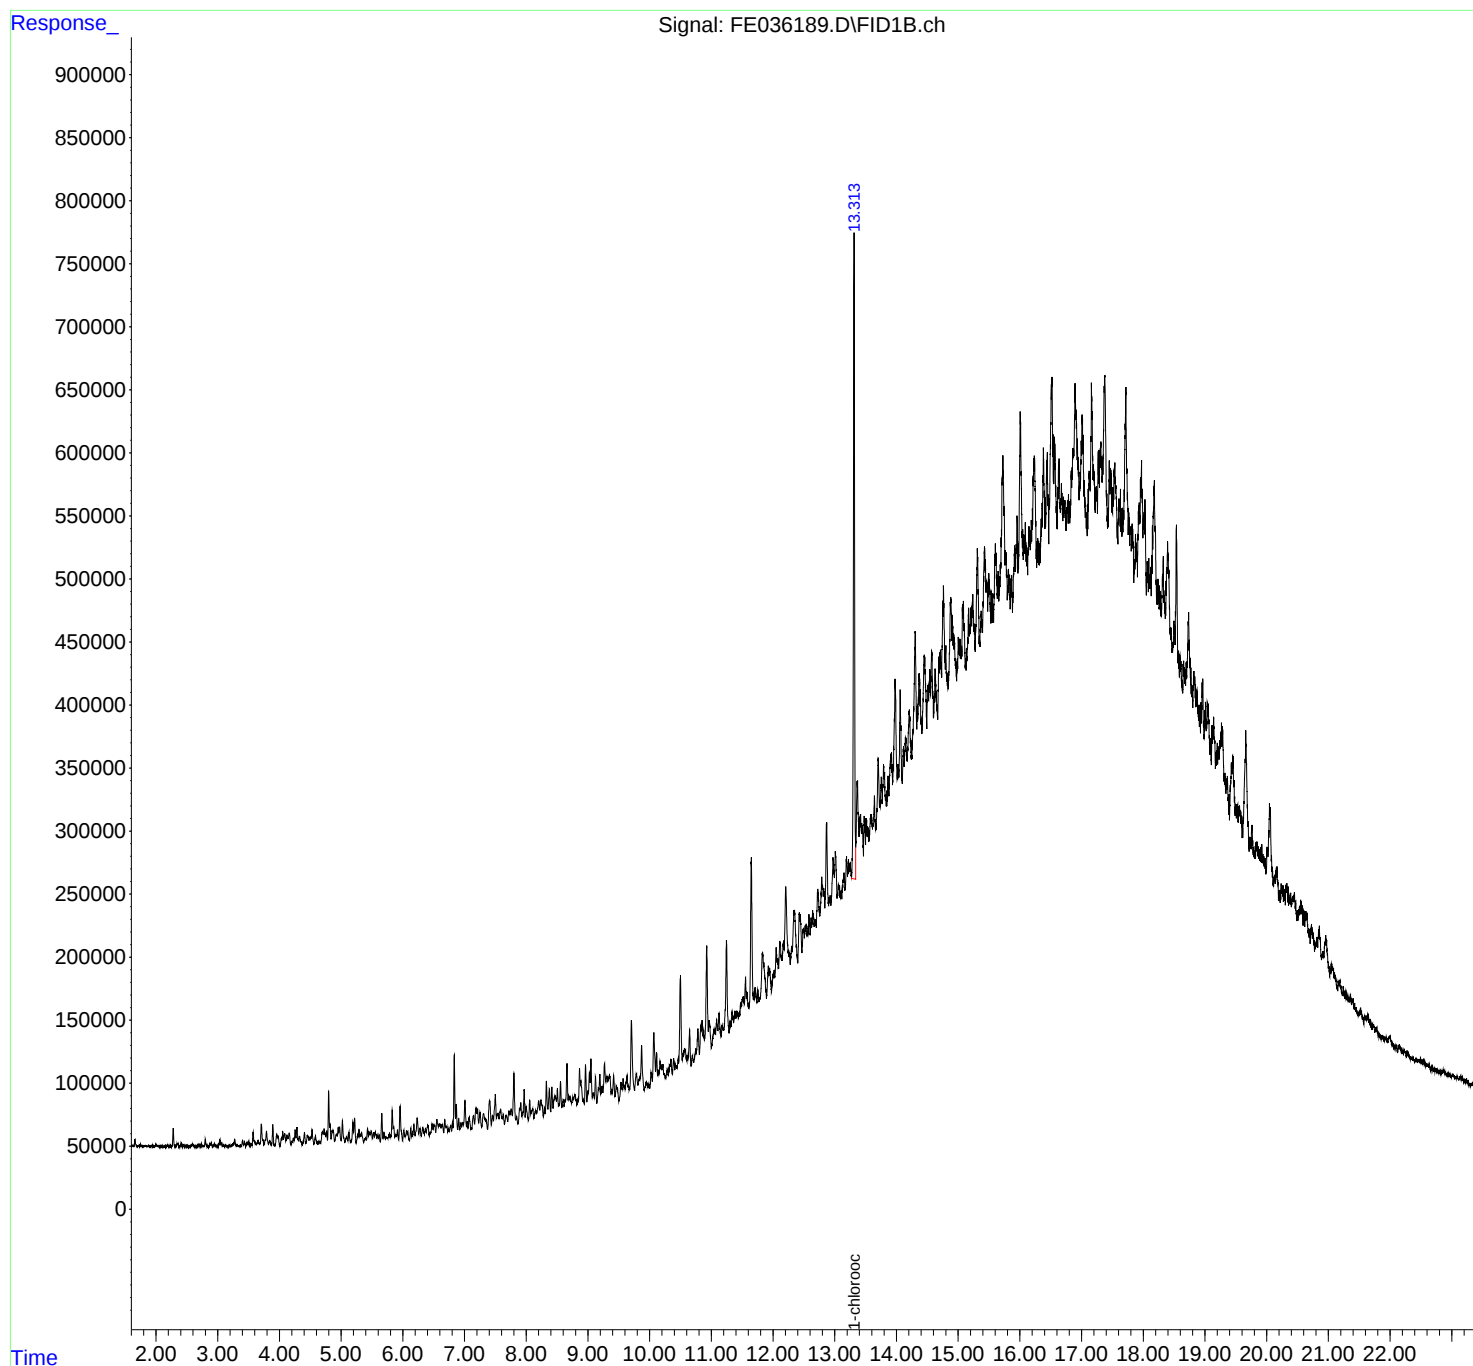

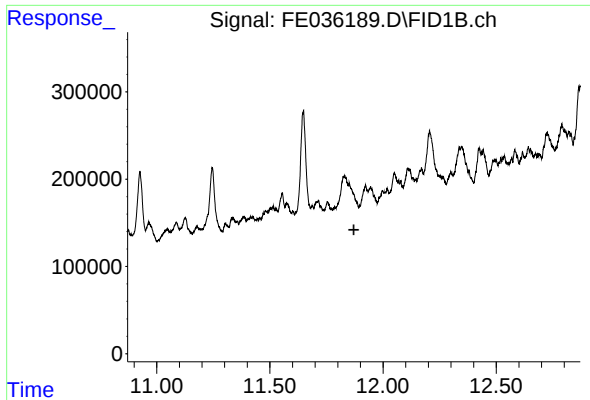


#9 ortho-Terphenyl (SURR)

R.T.: 0.000 min  
Exp R.T.: 11.871 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_E  
ClientSampleId :  
WC-14A-1A-12-GR

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 06/27/2022  
Supervised By :Ankita Jodhani 06/27/2022

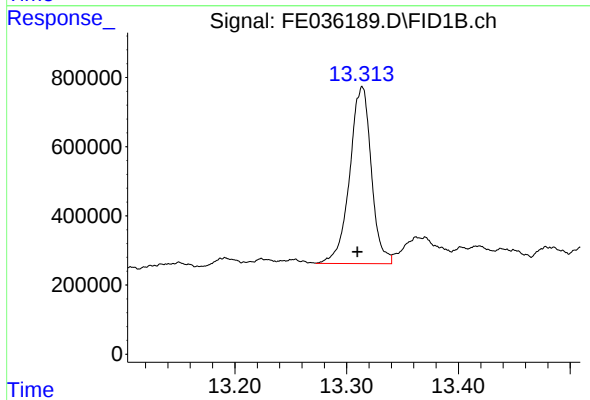

#12 1-chlorooctadecane (SURR)

R.T.: 13.313 min  
Delta R.T.: 0.004 min  
Response: 6871705  
Conc: 44.39 ug/ml m