

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062620\
 Data File : FE032265.D
 Signal(s) : FID1B.CH
 Acq On : 26 Jun 2020 16:10
 Operator : DD\AJ
 Sample : L2817-11MSD
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jun 27 00:00:58 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
 Quant Title :
 QLast Update : Thu Jun 11 13:38:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.750	5732859	17.931 ug/ml
Target Compounds			
2) N-DECANE	4.495	7833978	21.079 ug/ml
3) N-DODECANE	6.509	7952495	21.336 ug/ml
4) N-TETRADECANE	8.303	8322848	22.474 ug/ml
5) N-HEXADECANE	9.903	7855812	21.199 ug/ml
6) N-OCTADECANE	11.346	8129868	21.690 ug/ml
7) N-EICOSANE	12.656	9120639	24.553 ug/ml
8) N-DOCOSANE	13.852	8397251	22.703 ug/ml
10) N-TETRACOSANE	14.954	12878926	34.697 ug/ml
11) N-HEXACOSANE	15.977	7885238	21.534 ug/ml
12) N-OCTACOSANE	16.926	9063850	24.799 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062620\
Data File : FE032265.D
Signal(s) : FID1B.CH
Acq On : 26 Jun 2020 16:10
Operator : DD\AJ
Sample : L2817-11MSD
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 27 00:00:58 2020
Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
Quant Title :
QLast Update : Thu Jun 11 13:38:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

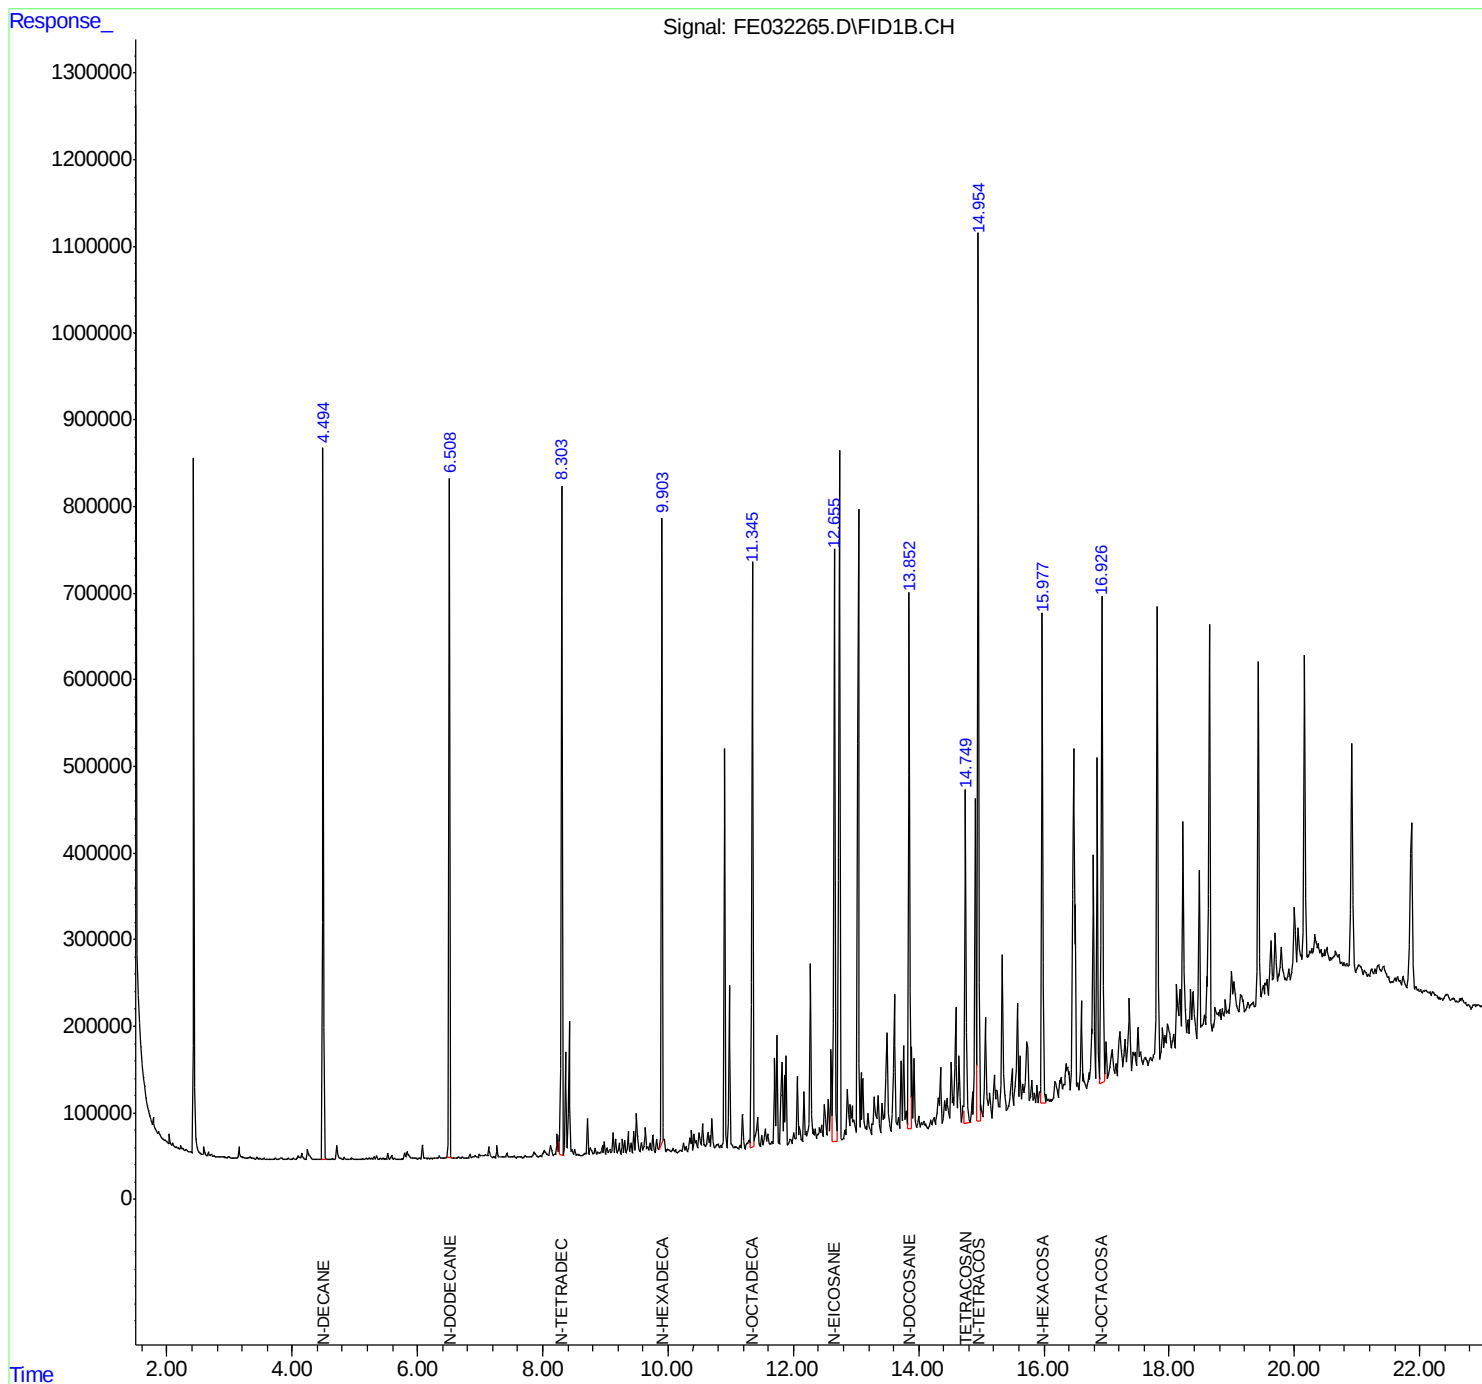

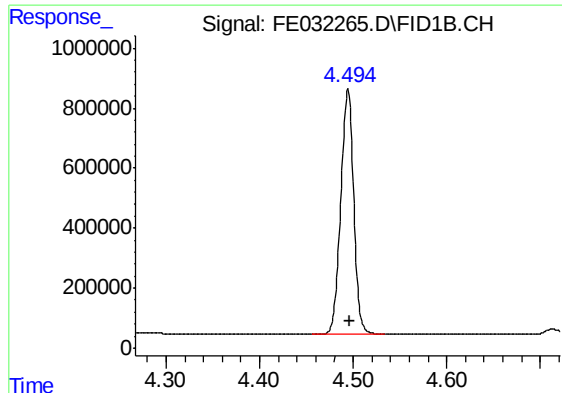


#2 N-DECANE

R.T.: 4.495 min
Delta R.T.: -0.002 min
Response: 7833978
Conc: 21.08 ug/ml

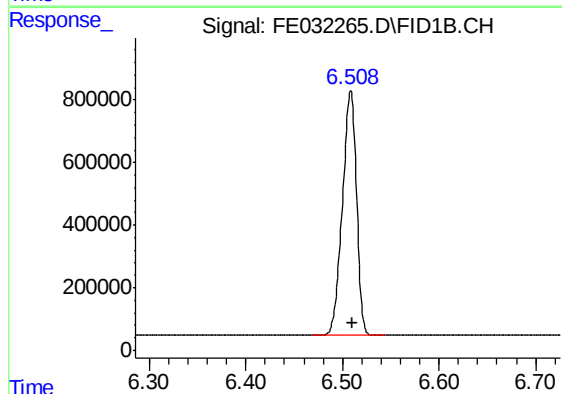


#3 N-DODECANE

R.T.: 6.509 min
Delta R.T.: -0.002 min
Response: 7952495
Conc: 21.34 ug/ml

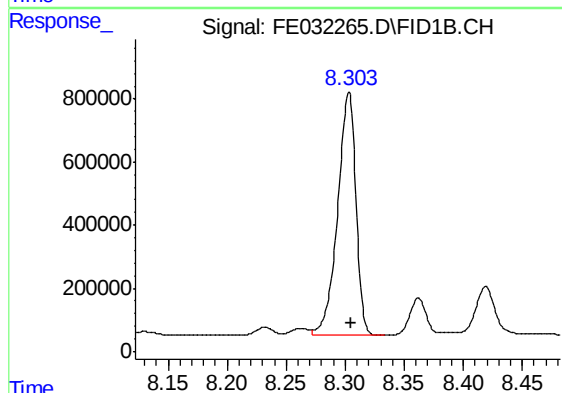


#4 N-TETRADECANE

R.T.: 8.303 min
Delta R.T.: -0.001 min
Response: 8322848
Conc: 22.47 ug/ml

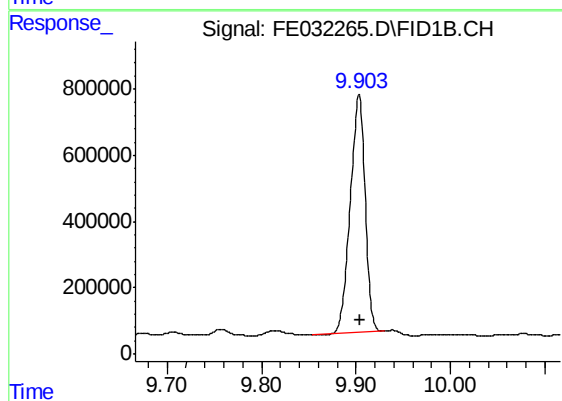


#5 N-HEXADECANE

R.T.: 9.903 min
Delta R.T.: -0.001 min
Response: 7855812
Conc: 21.20 ug/ml

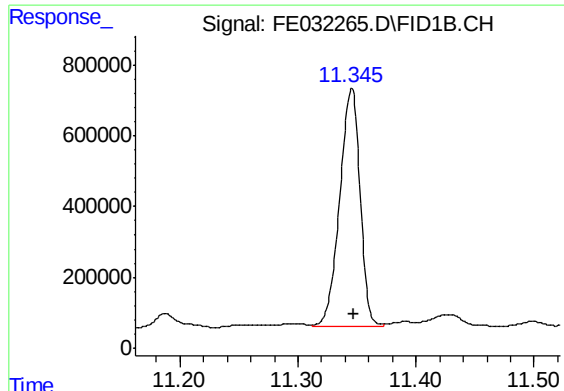


#6 N-OCTADECANE

R.T.: 11.346 min
Delta R.T.: -0.001 min
Response: 8129868
Conc: 21.69 ug/ml

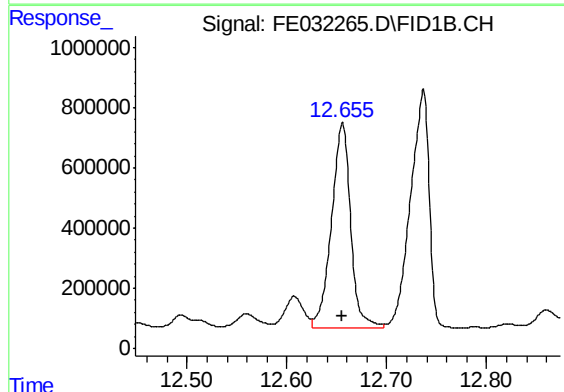


#7 N-EICOSANE

R.T.: 12.656 min
Delta R.T.: 0.000 min
Response: 9120639
Conc: 24.55 ug/ml

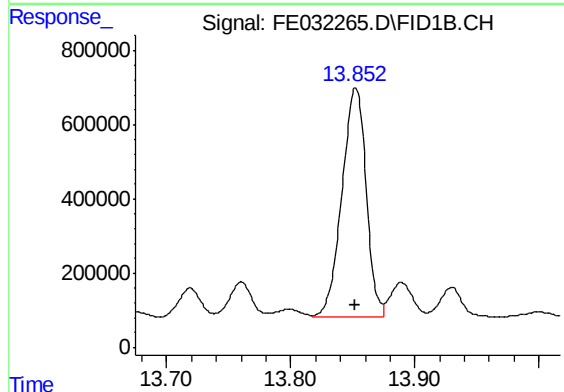


#8 N-DOCOSANE

R.T.: 13.852 min
Delta R.T.: 0.000 min
Response: 8397251
Conc: 22.70 ug/ml

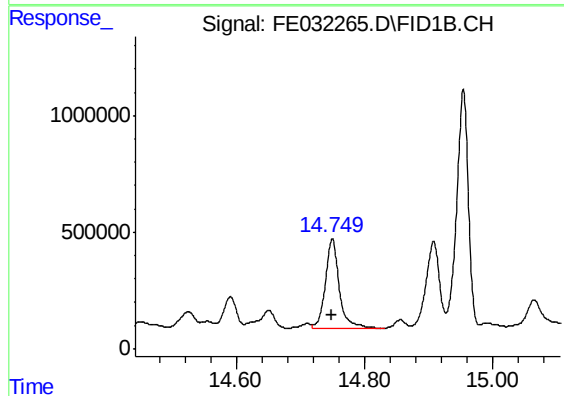


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.750 min
Delta R.T.: 0.001 min
Response: 5732859
Conc: 17.93 ug/ml

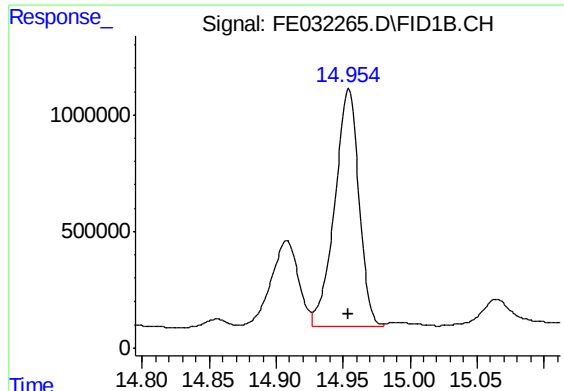


#10 N-TETRACOSANE

R.T.: 14.954 min
Delta R.T.: 0.000 min
Response: 12878926
Conc: 34.70 ug/ml

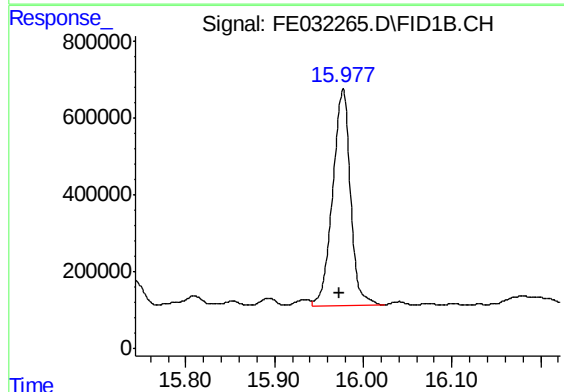

#11 N-HEXACOSANE

R.T.: 15.977 min
Delta R.T.: 0.004 min
Response: 7885238
Conc: 21.53 ug/ml

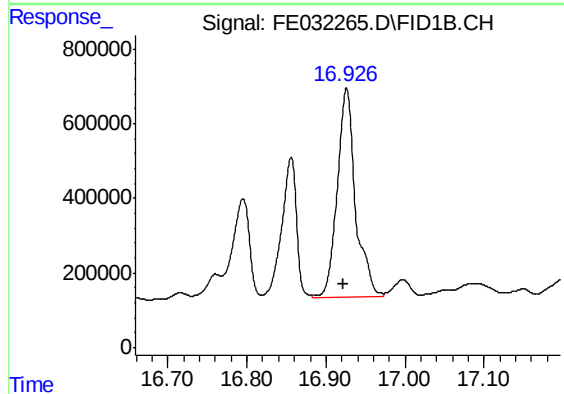

#12 N-OCTACOSANE

R.T.: 16.926 min
Delta R.T.: 0.005 min
Response: 9063850
Conc: 24.80 ug/ml