

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062722AL\
Data File : FE036231.D
Signal(s) : FID1B.ch
Acq On : 27 Jun 2022 12:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 03:10:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
19) T	n-Tetratriacontane (C34)	19.657	1336817	9.660 ug/ml
20) T	n-Hexatriacontane (C36)	20.391	179236	1.335 ug/ml
21) T	n-Octatriacontane (C38)	21.054	1288731	9.690 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062722AL\
Data File : FE036231.D
Signal(s) : FID1B.ch
Acq On : 27 Jun 2022 12:57
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 28 03:10:47 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

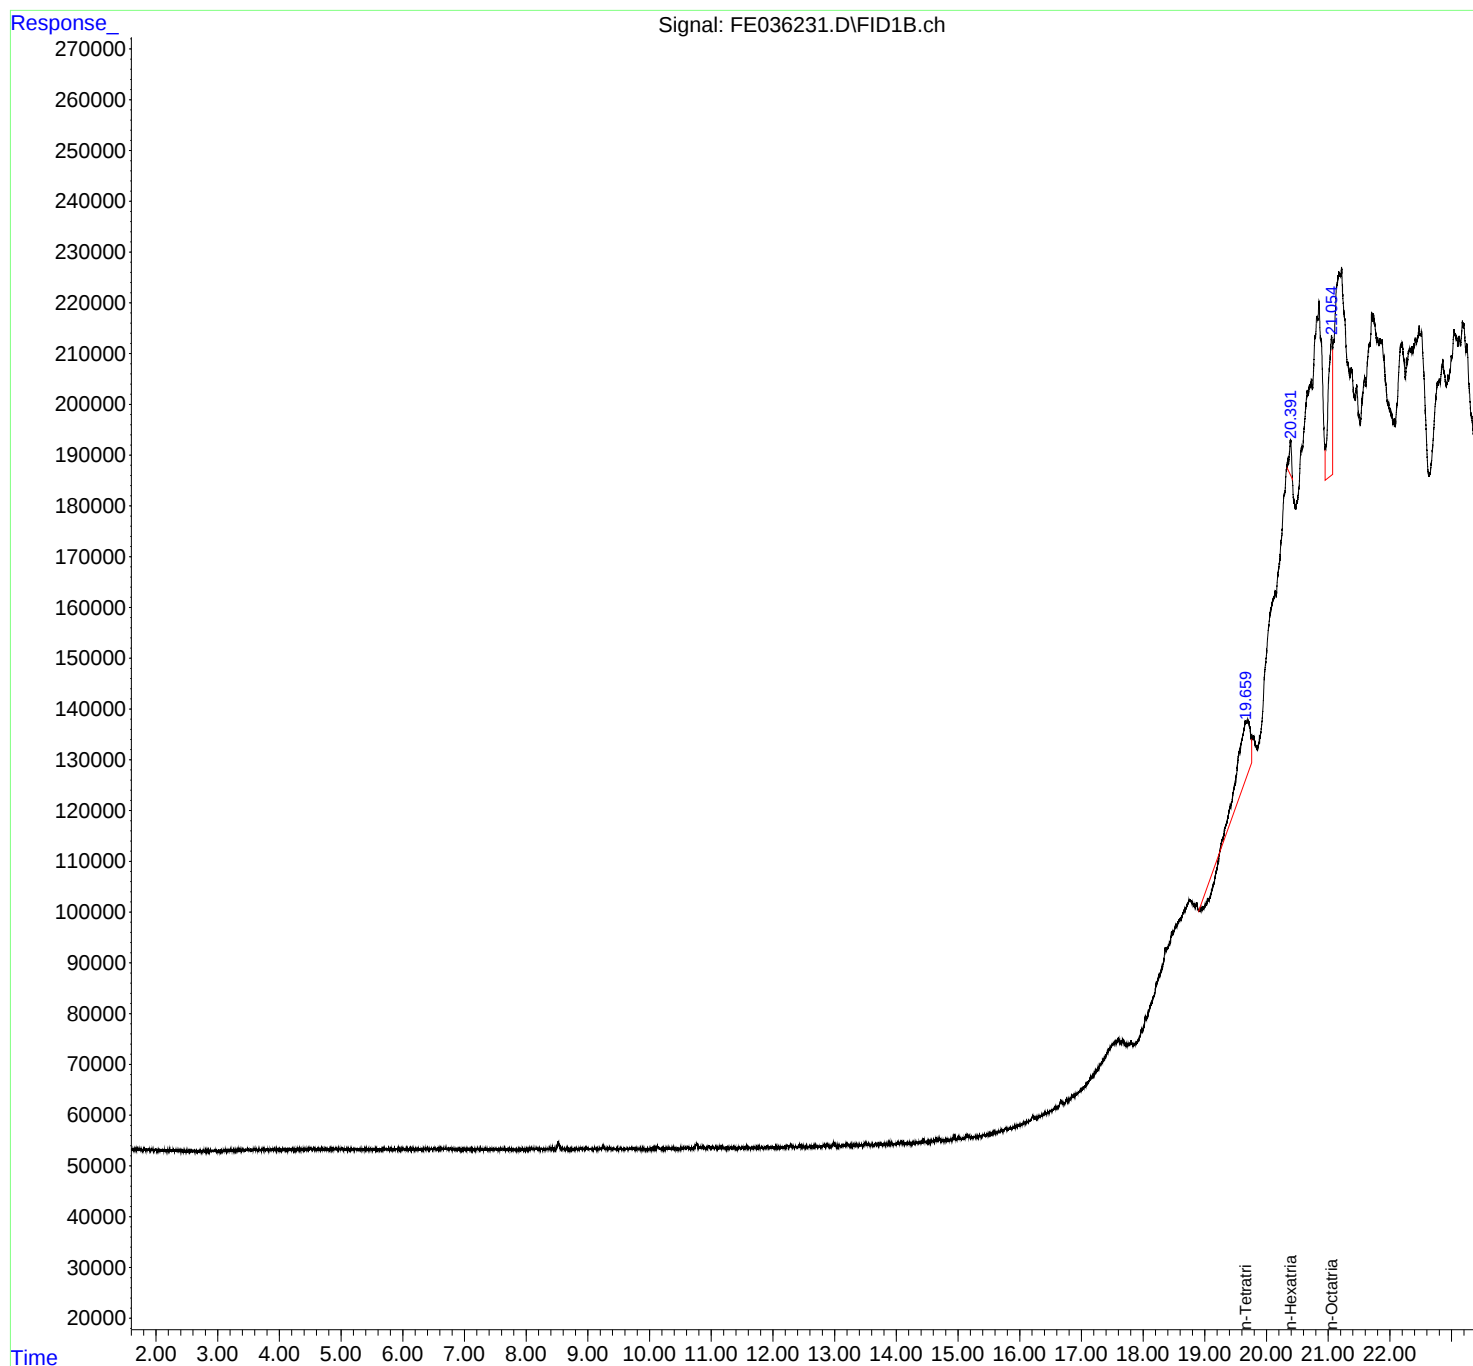


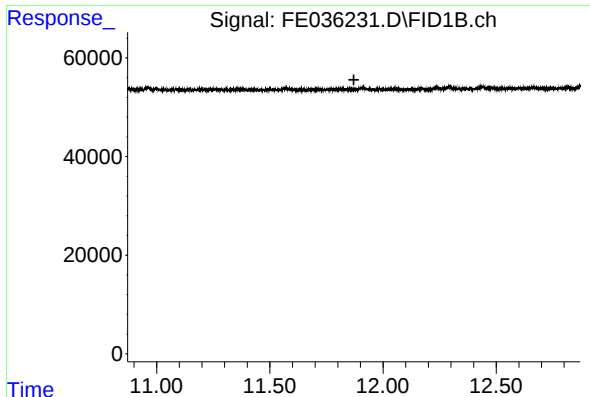

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.871 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

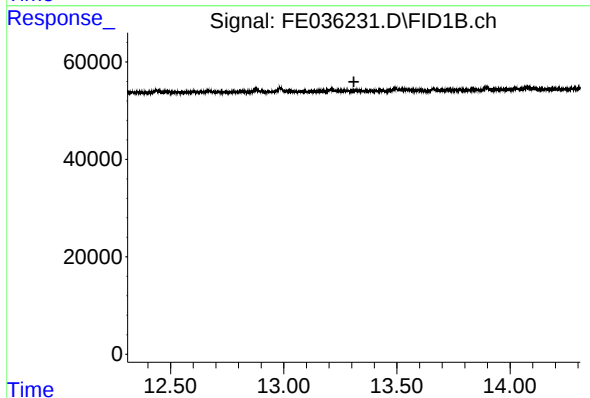


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.310 min
Response: 0
Conc: N.D.

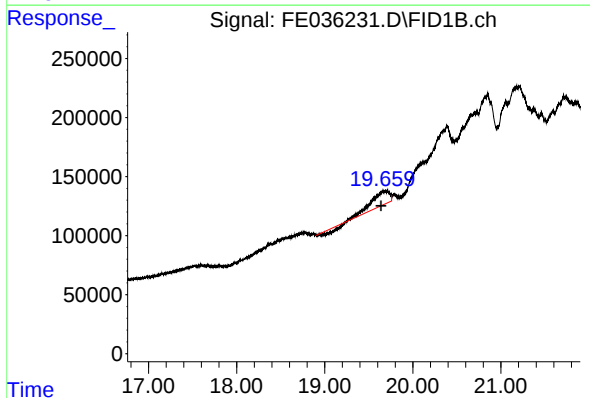


#19 n-Tetratriacontane (C34)

R.T.: 19.657 min
Delta R.T.: 0.017 min
Response: 1336817
Conc: 9.66 ug/ml

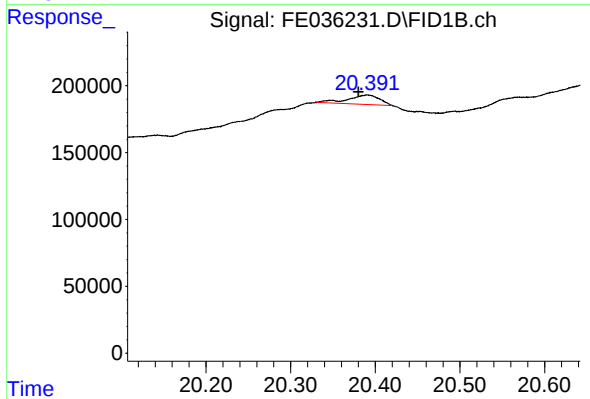

#20 n-Hexatriacontane (C36)

R.T.: 20.391 min
Delta R.T.: 0.011 min
Response: 179236
Conc: 1.34 ug/ml

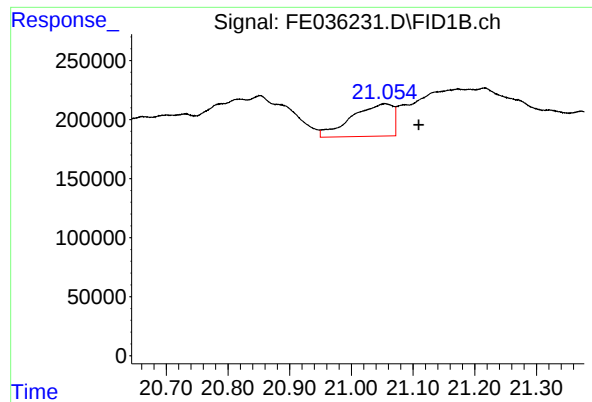

#21 n-Octatriacontane (C38)

R.T.: 21.054 min
Delta R.T.: -0.055 min
Response: 1288731
Conc: 9.69 ug/ml

Instrument :
FID_E
ClientSampleId :