

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE062724AL\  
 Data File : FE048910.D  
 Signal(s) : FID1B.ch  
 Acq On : 27 Jun 2024 10:53  
 Operator : YP\AJ  
 Sample : P3064-01DL 5X  
 Misc :  
 ALS Vial : 7 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 HD-02-062524DL

Integration File: autoint1.e  
 Quant Time: Jun 28 01:26:11 2024  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062124.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Jun 20 17:53:58 2024  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units  |
|--------------------------------|--------|------------|-------------|
| -----                          |        |            |             |
| System Monitoring Compounds    |        |            |             |
| 9) S ortho-Terphenyl (SURR)    | 11.936 | 1074206    | 6.424 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 12.85%      |
| 12) S 1-chlorooctadecane (S... | 13.372 | 904705     | 7.036 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 14.07%      |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE062724AL\  
Data File : FE048910.D  
Signal(s) : FID1B.ch  
Acq On : 27 Jun 2024 10:53  
Operator : YP\AJ  
Sample : P3064-01DL 5X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
HD-02-062524DL

Integration File: autoint1.e  
Quant Time: Jun 28 01:26:11 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062124.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 20 17:53:58 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

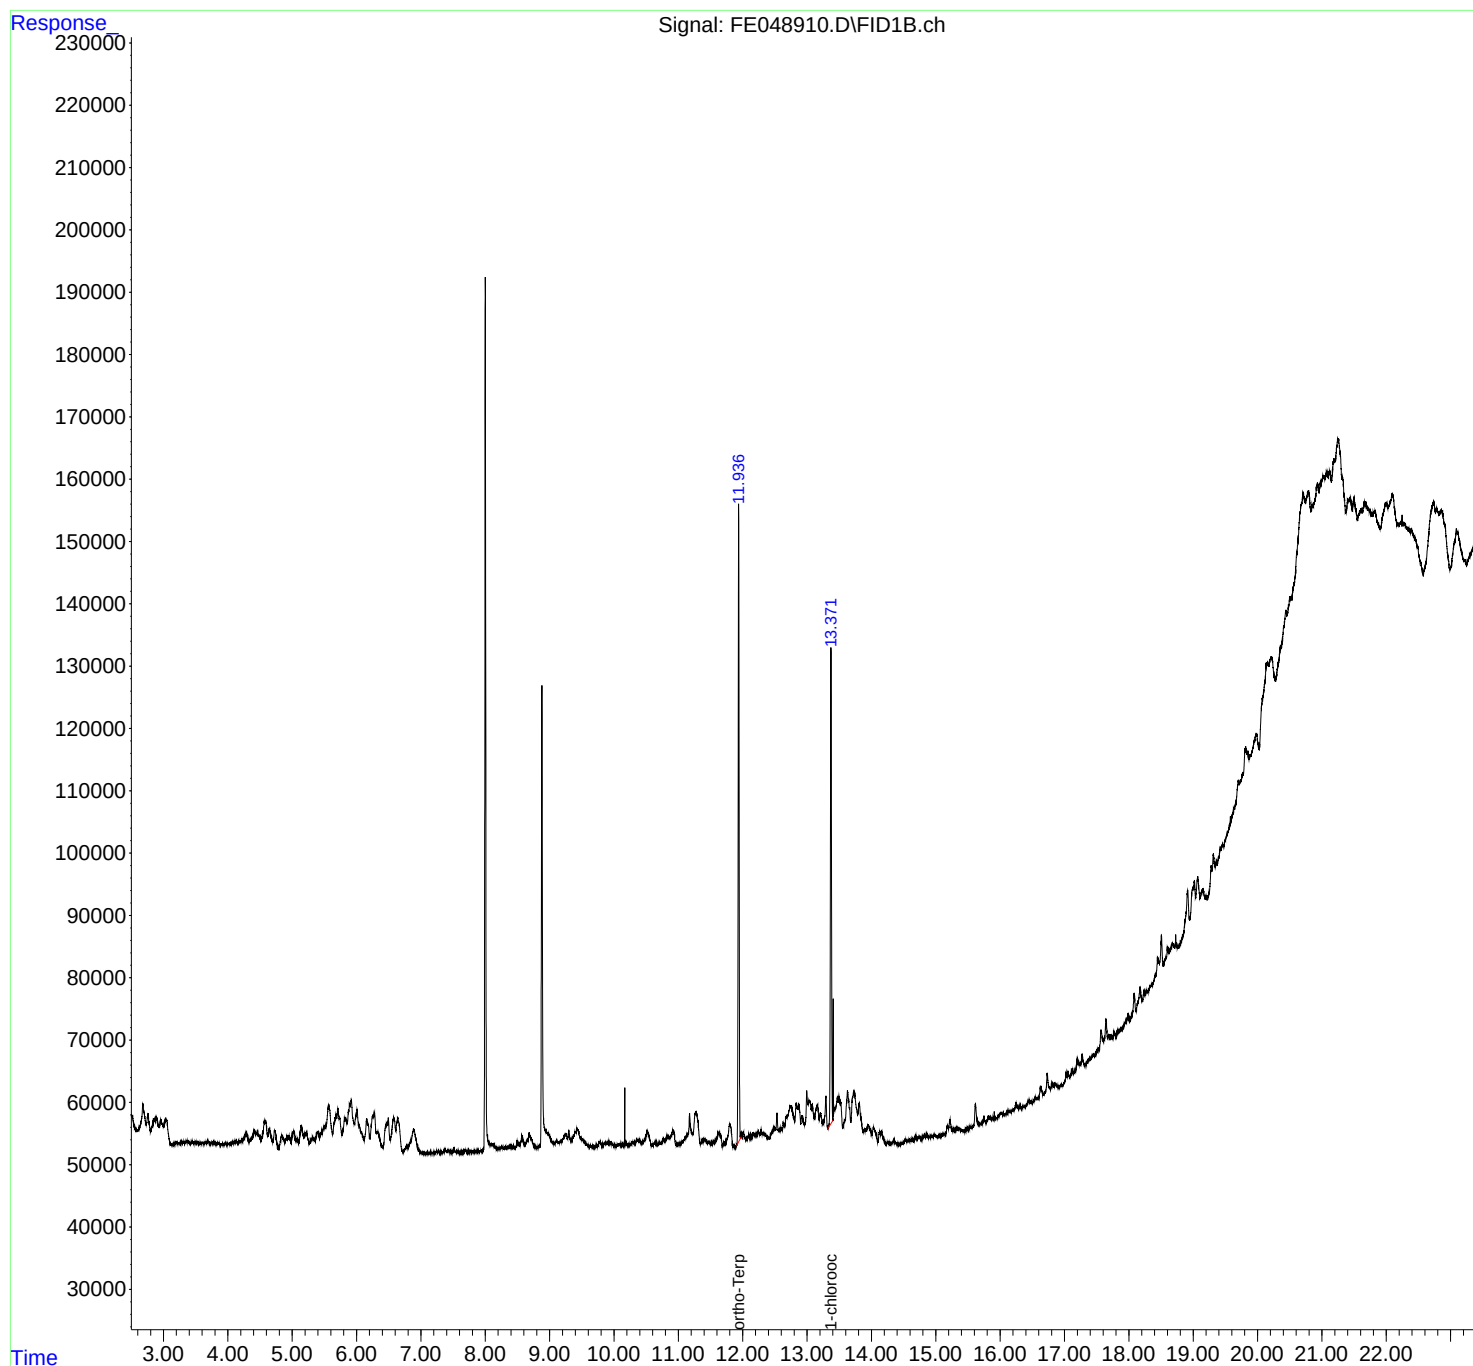


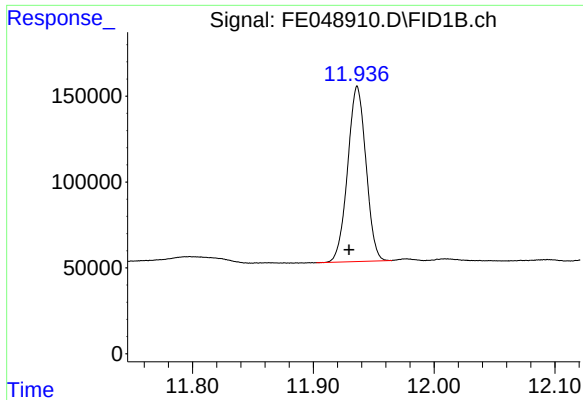

#9 ortho-Terphenyl (SURR)

R.T.: 11.936 min  
Delta R.T.: 0.007 min  
Response: 1074206  
Conc: 6.42 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
HD-02-062524DL

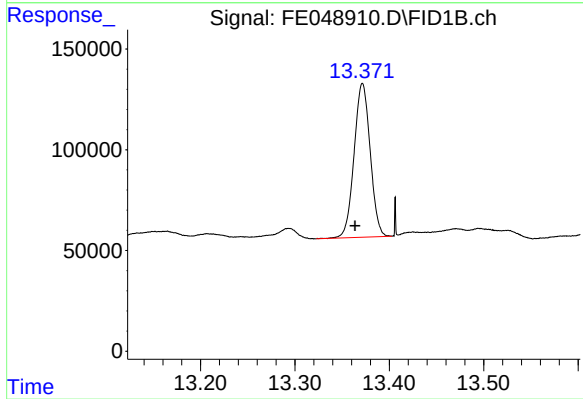

#12 1-chlorooctadecane (SURR)

R.T.: 13.372 min  
Delta R.T.: 0.008 min  
Response: 904705  
Conc: 7.04 ug/ml