

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062818\
Data File : FE027994.D
Signal(s) : FID1B.CH
Acq On : 28 Jun 2018 19:54
Operator : UA/AJ
Sample : J3715-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 29 05:12:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
13) S	TETRACOSANE-d50 (SURR...	15.042	3567960	10.692 ug/ml
Target Compounds				
3)	N-DECANE	4.761	1512847	7.015 ug/ml
6)	N-TETRADECANE	8.553	308090	1.548 ug/ml
7)	N-HEXADECANE	10.162	531362	2.306 ug/ml
8)	N-OCTADECANE	11.612	220969	0.857 ug/ml
12)	N-DOTRIACONTANE	18.947	198859	0.858 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062818\
Data File : FE027994.D
Signal(s) : FID1B.CH
Acq On : 28 Jun 2018 19:54
Operator : UA/AJ
Sample : J3715-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jun 29 05:12:33 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\C44-FE062618.M
Quant Title :
QLast Update : Tue Jun 26 18:10:02 2018
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20m x 0.18mm x 0.18um

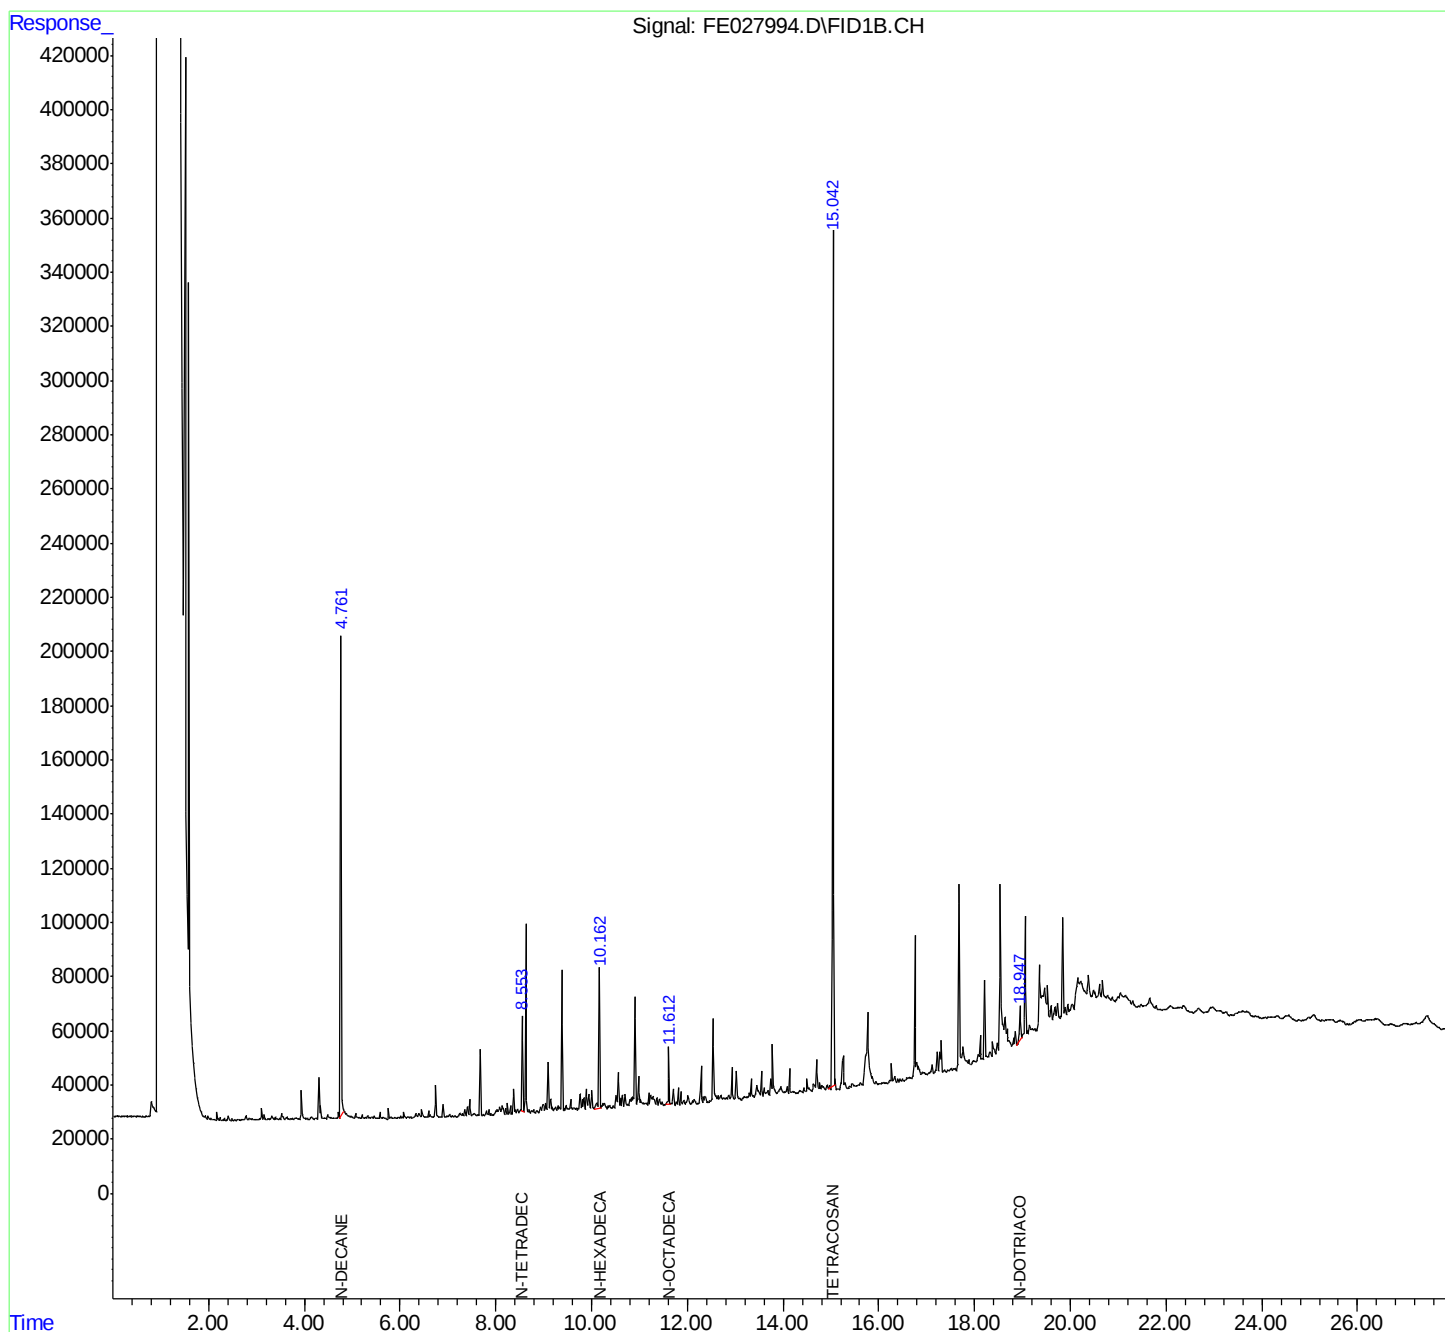

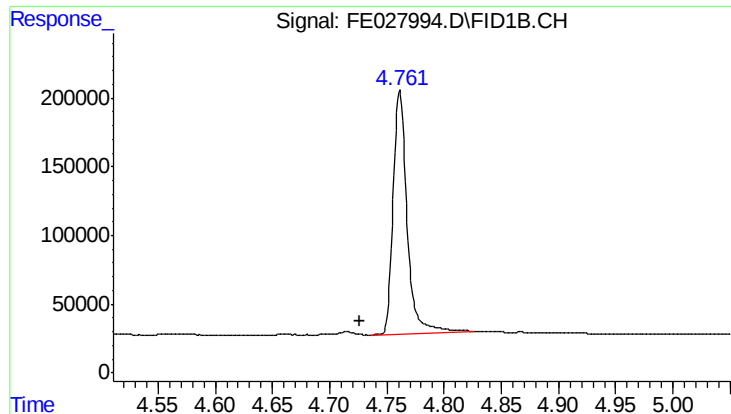


#3 N-DECANE

R.T.: 4.761 min
Delta R.T.: 0.035 min
Response: 1512847
Conc: 7.01 ug/ml

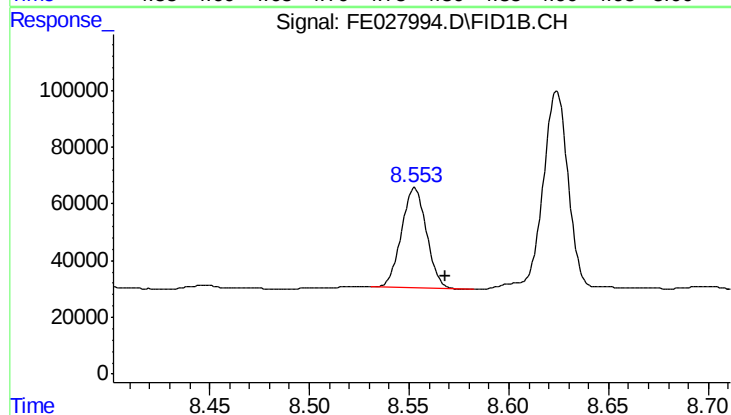


#6 N-TETRADECANE

R.T.: 8.553 min
Delta R.T.: -0.015 min
Response: 308090
Conc: 1.55 ug/ml

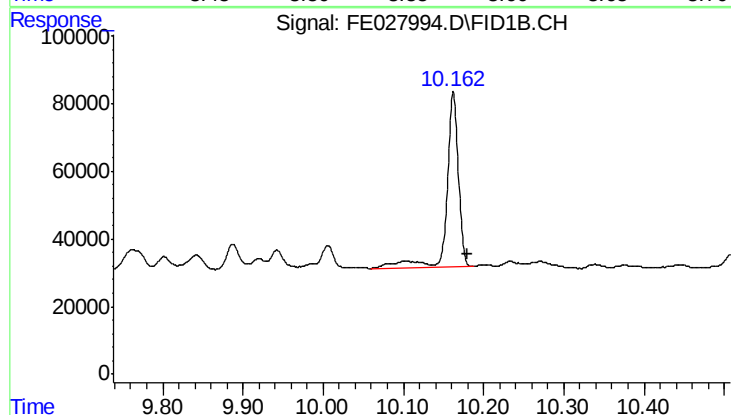


#7 N-HEXADECANE

R.T.: 10.162 min
Delta R.T.: -0.017 min
Response: 531362
Conc: 2.31 ug/ml

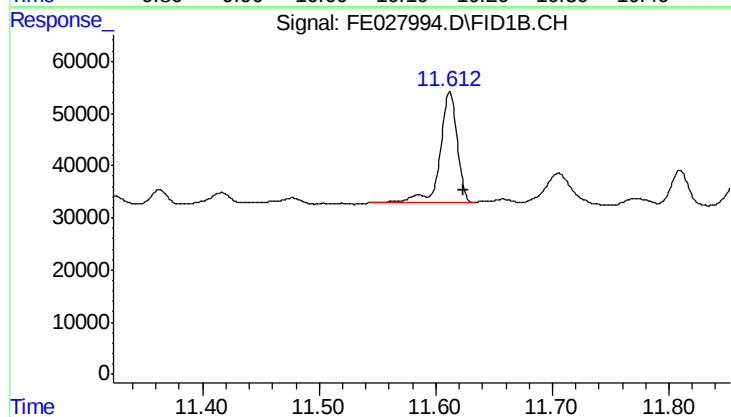


#8 N-OCTADECANE

R.T.: 11.612 min
Delta R.T.: -0.011 min
Response: 220969
Conc: 0.86 ug/ml

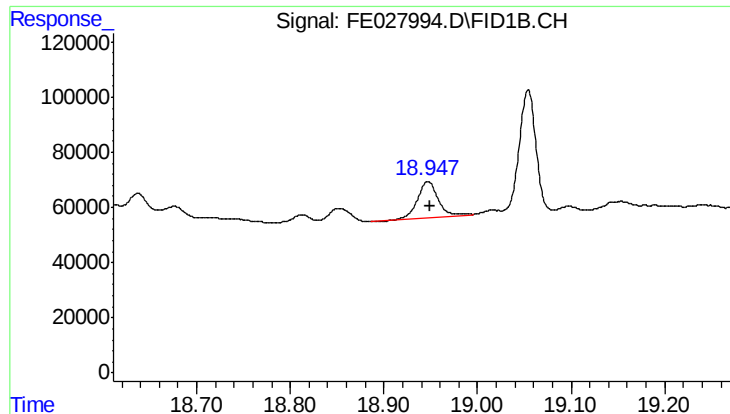

#12 N-DOTRIACONTANE

R.T.: 18.947 min
Delta R.T.: -0.002 min
Response: 198859
Conc: 0.86 ug/ml

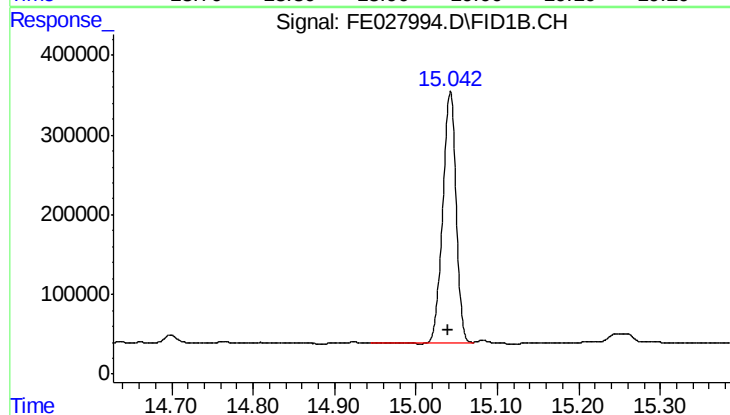

#13 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.042 min
Delta R.T.: 0.002 min
Response: 3567960
Conc: 10.69 ug/ml