

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062823AL\
 Data File : FE042975.D
 Signal(s) : FID1B.ch
 Acq On : 28 Jun 2023 09:19
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 29 02:47:13 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 11:03:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.897	753659	5.373 ug/ml
19) T	n-Tetratriacontane (C34)	19.681	1902338	13.901 ug/ml
20) T	n-Hexatriacontane (C36)	20.423	2263695	16.927 ug/ml
21) T	n-Octatriacontane (C38)	21.165	1992330	14.613 ug/ml
22) T	n-Tetracontane (C40)	22.080	1242921	8.934 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062823AL\
Data File : FE042975.D
Signal(s) : FID1B.ch
Acq On : 28 Jun 2023 09:19
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 29 02:47:13 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 11:03:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

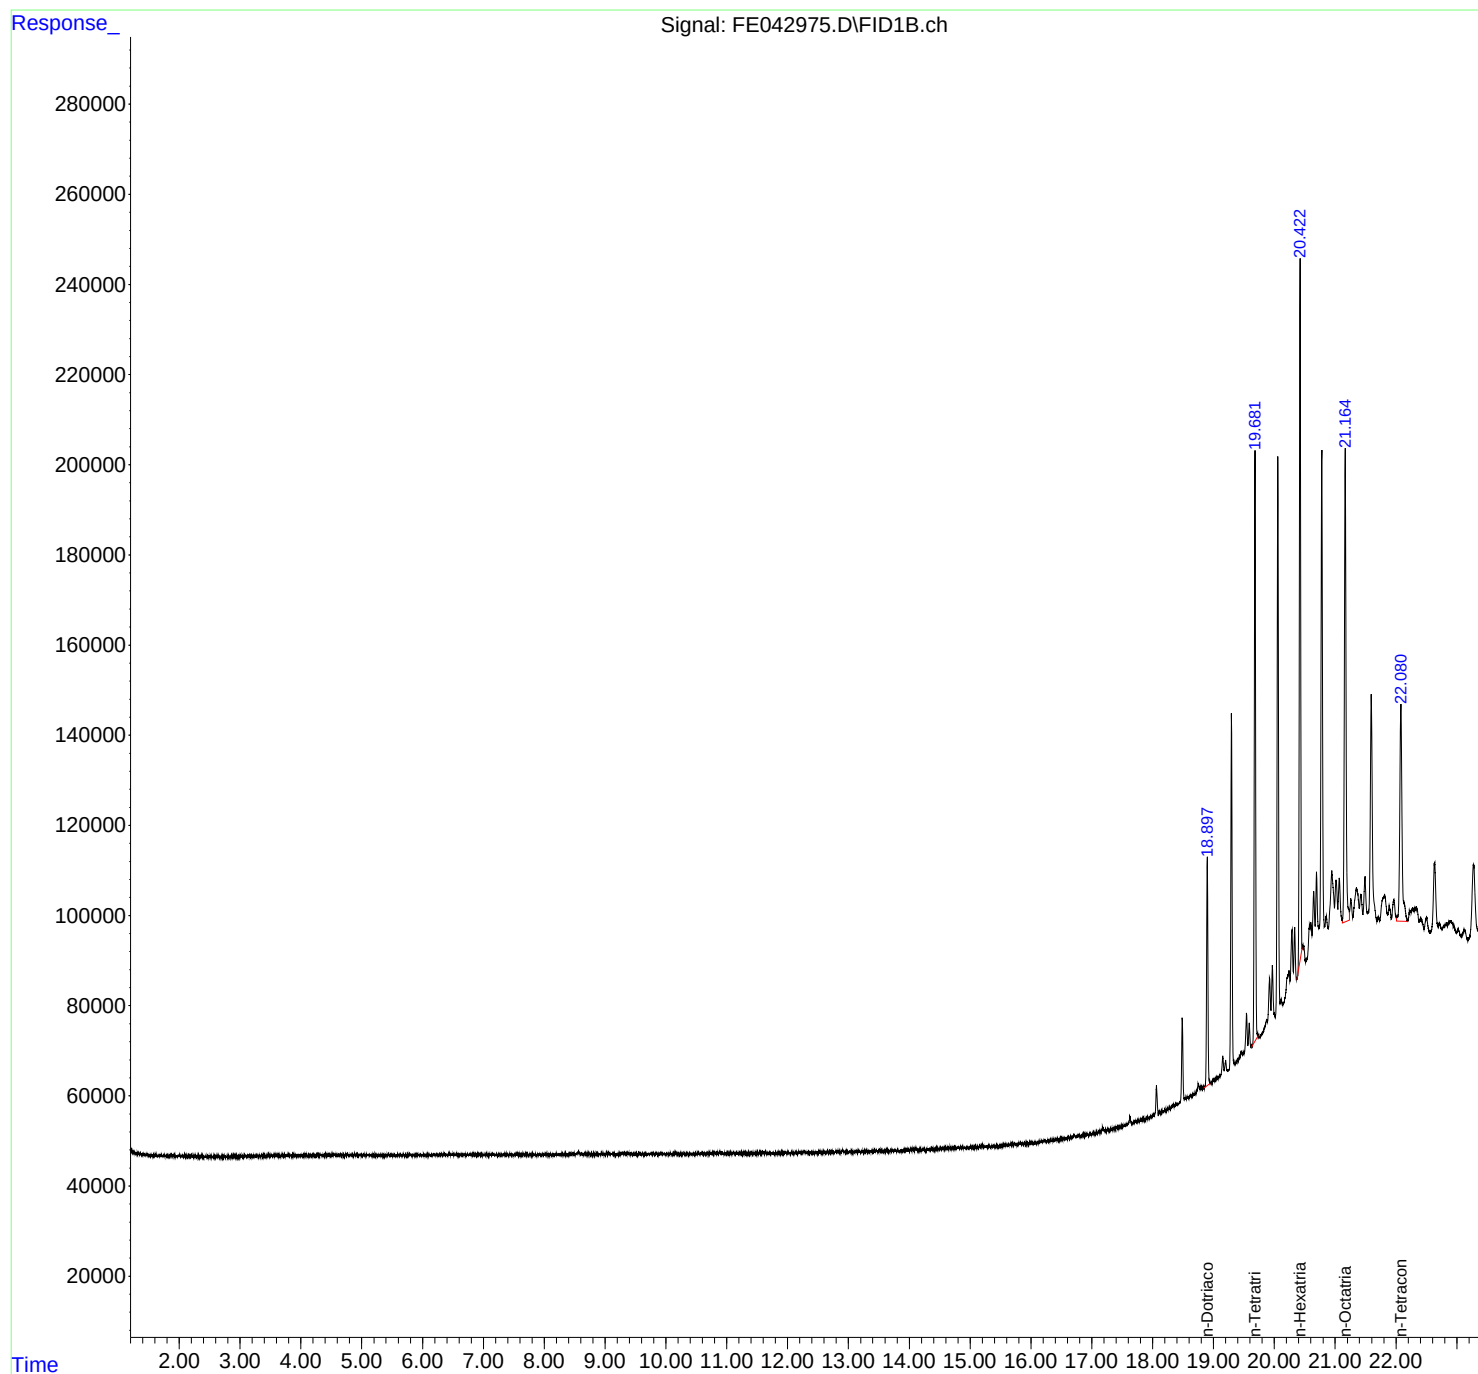


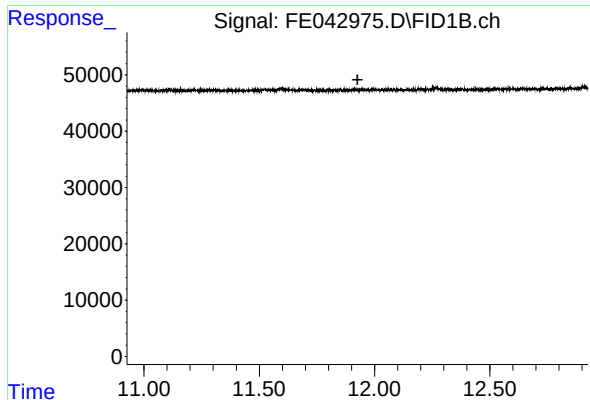

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T.: 11.926 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

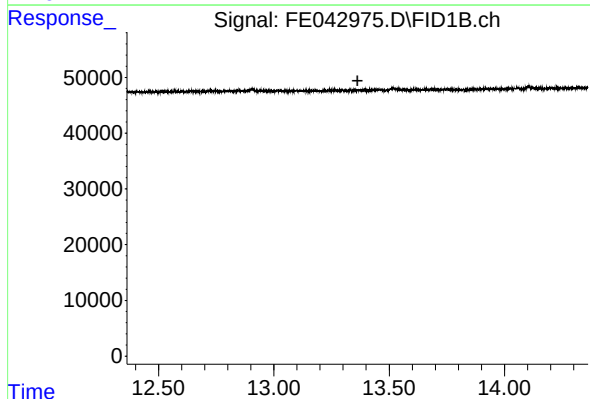


#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T.: 13.363 min
Response: 0
Conc: N.D.

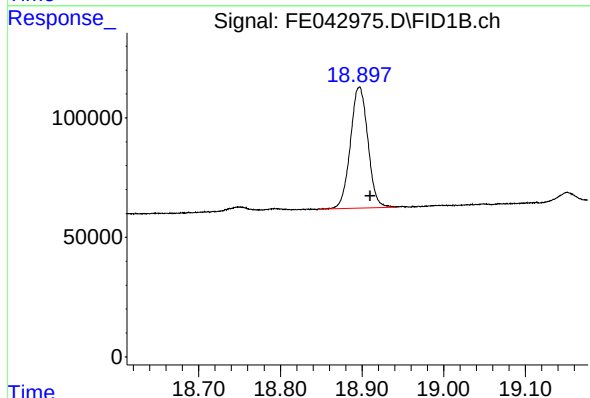


#18 n-Dotriacontane (C32)

R.T.: 18.897 min
Delta R.T.: -0.013 min
Response: 753659
Conc: 5.37 ug/ml

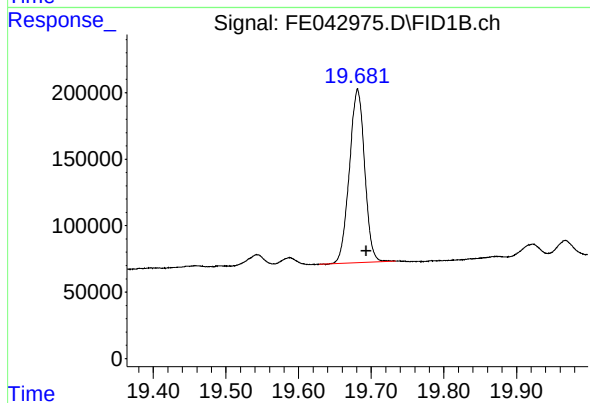

#19 n-Tetratriacontane (C34)

R.T.: 19.681 min
Delta R.T.: -0.012 min
Response: 1902338
Conc: 13.90 ug/ml

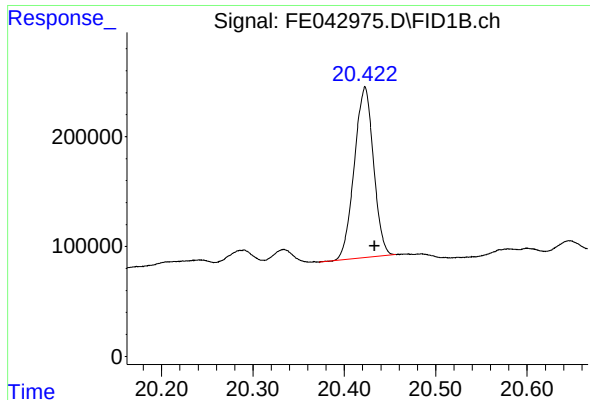


#20 n-Hexatriacontane (C36)

R.T.: 20.423 min
Delta R.T.: -0.010 min
Response: 2263695
Conc: 16.93 ug/ml

Instrument :


FID_E

ClientSampleId :

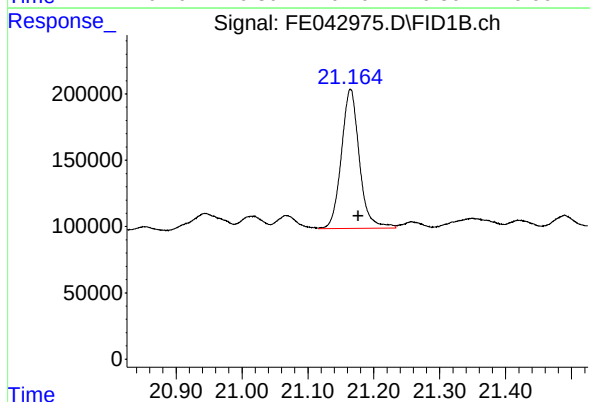

#21 n-Octatriacontane (C38)

R.T.: 21.165 min
Delta R.T.: -0.012 min
Response: 1992330
Conc: 14.61 ug/ml

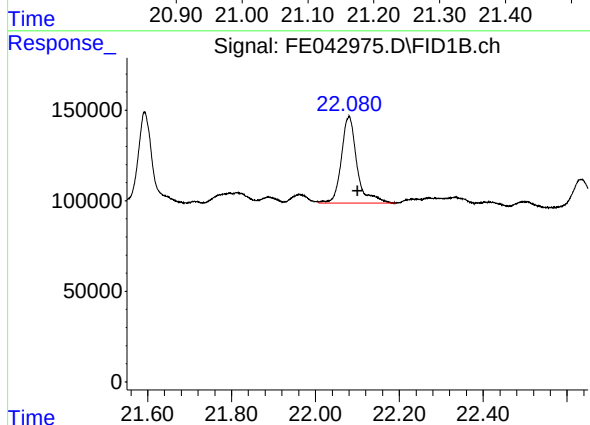

#22 n-Tetracontane (C40)

R.T.: 22.080 min
Delta R.T.: -0.021 min
Response: 1242921
Conc: 8.93 ug/ml