

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
 Data File : FE036280.D
 Signal(s) : FID1B.ch
 Acq On : 29 Jun 2022 09:03
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 30 01:26:51 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 21 03:08:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.850	208152	1.149 ug/ml
11) T n-Heneicosane (C21)	13.474	273182	1.521 ug/ml
13) T n-Docosane (C22)	14.062	235968	1.335 ug/ml
14) T n-Tetracosane (C24)	15.165	134423	<MDL ug/ml
15) T n-Hexacosane (C26)	16.199	288743	1.748 ug/ml
16) T n-Octacosane (C28)	17.141	137049	<MDL ug/ml
17) T n-Tricontane (C30)	18.031	118932	<MDL ug/ml
18) T n-Dotriacontane (C32)	18.860	147932	1.012 ug/ml
19) T n-Tetratriacontane (C34)	19.615	477320	3.449 ug/ml
20) T n-Hexatriacontane (C36)	20.385	17805	<MDL ug/ml
21) T n-Octatriacontane (C38)	21.150	41670	<MDL ug/ml
22) T n-Tetracontane (C40)	21.986	405745	2.902 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
Data File : FE036280.D
Signal(s) : FID1B.ch
Acq On : 29 Jun 2022 09:03
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 30 01:26:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

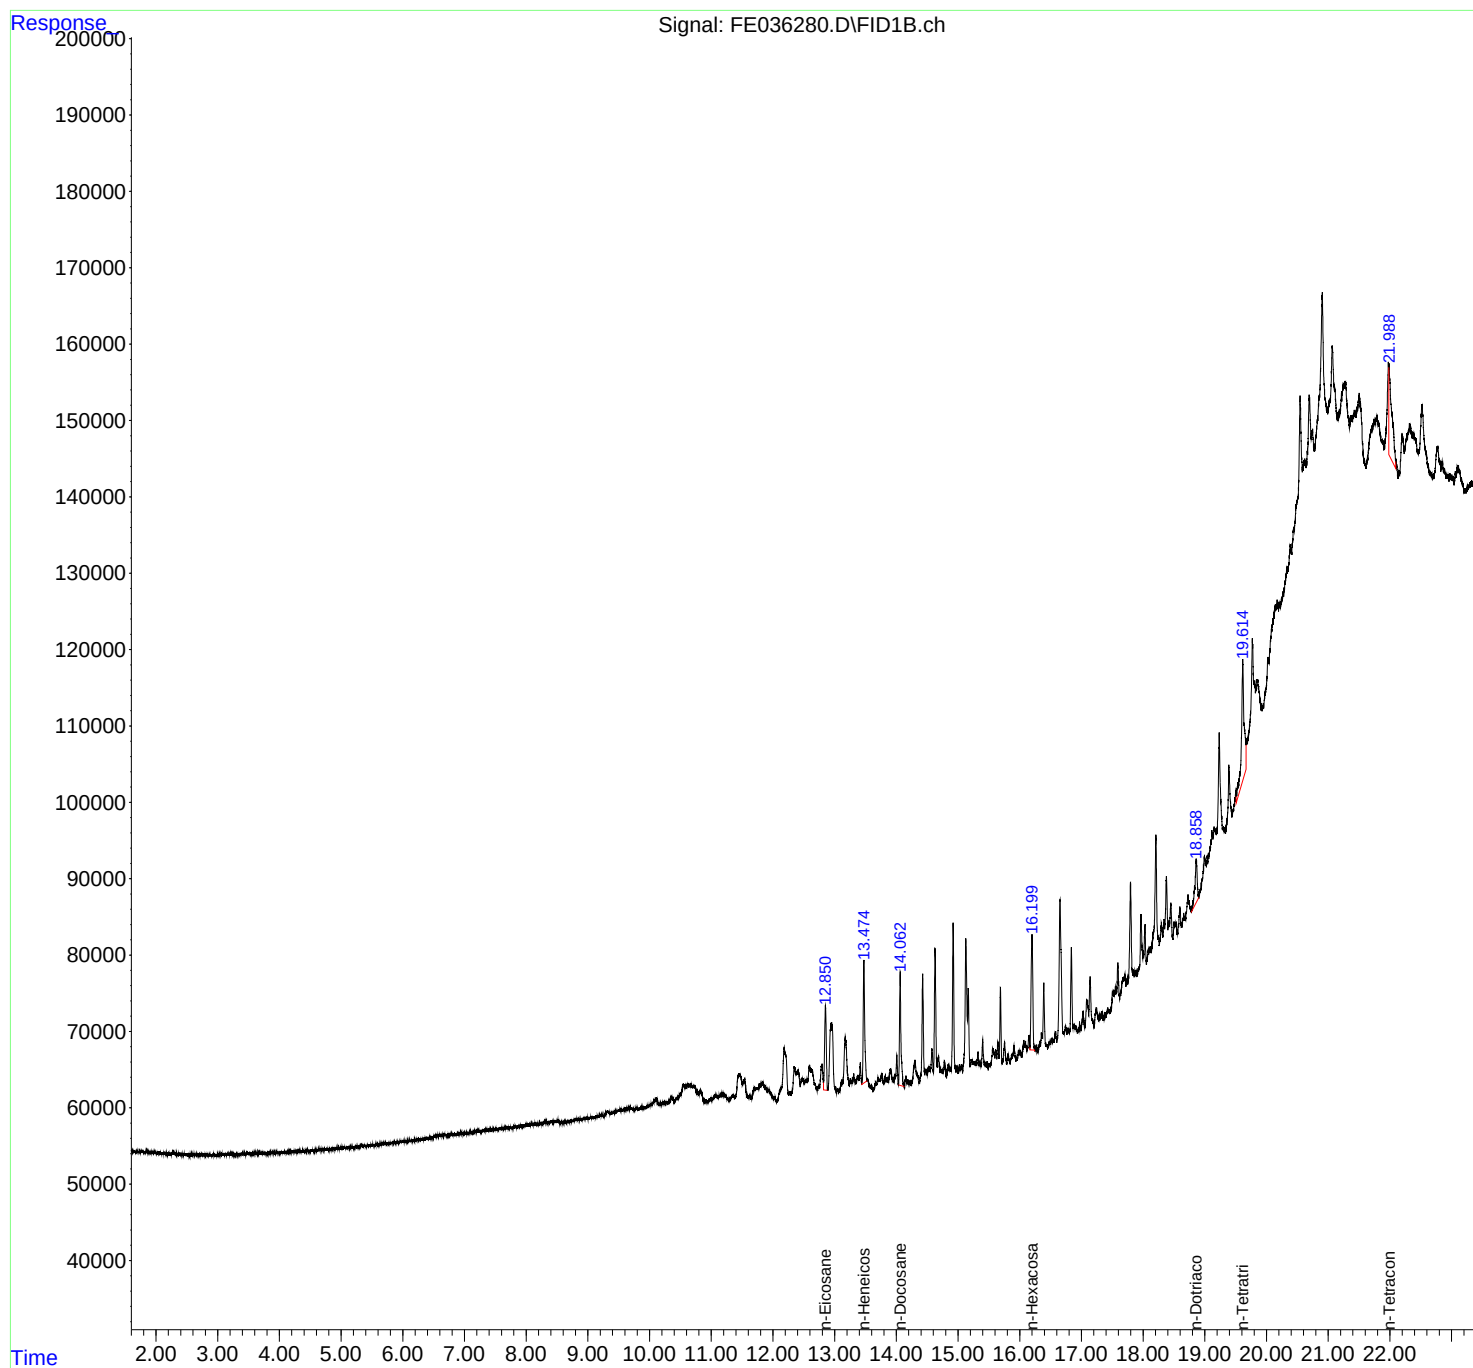


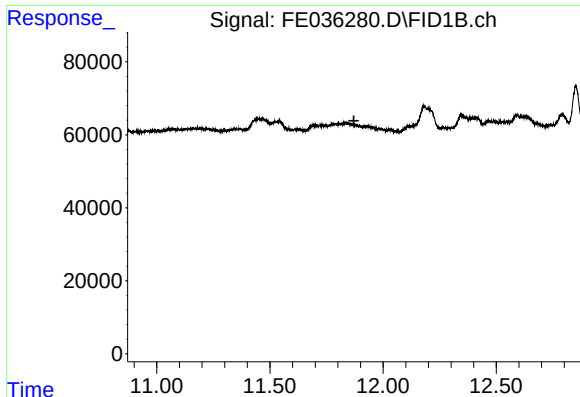

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.871 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

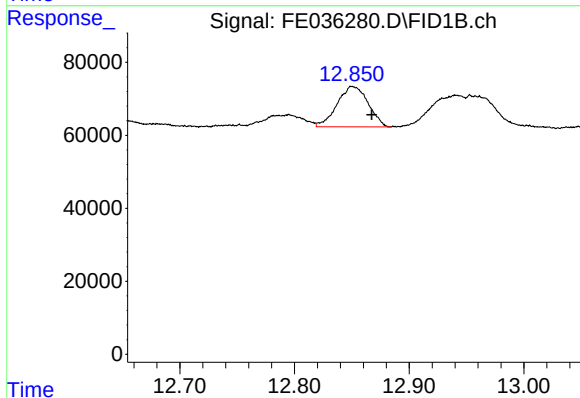


#10 n-Eicosane (C20)

R.T.: 12.850 min
Delta R.T.: -0.017 min
Response: 208152
Conc: 1.15 ug/ml

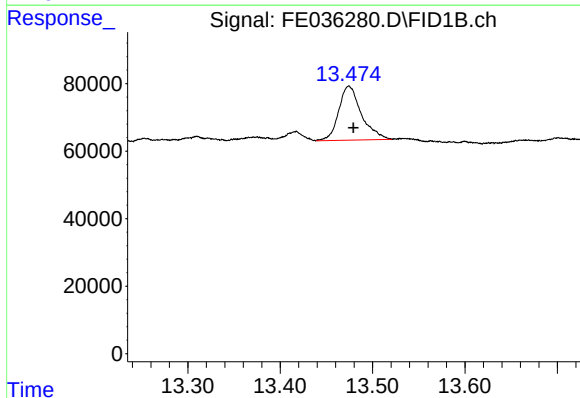


#11 n-Heneicosane (C21)

R.T.: 13.474 min
Delta R.T.: -0.005 min
Response: 273182
Conc: 1.52 ug/ml

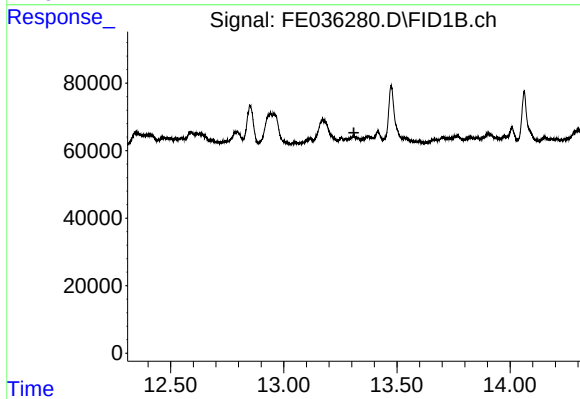

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.310 min
Response: 0
Conc: N.D.

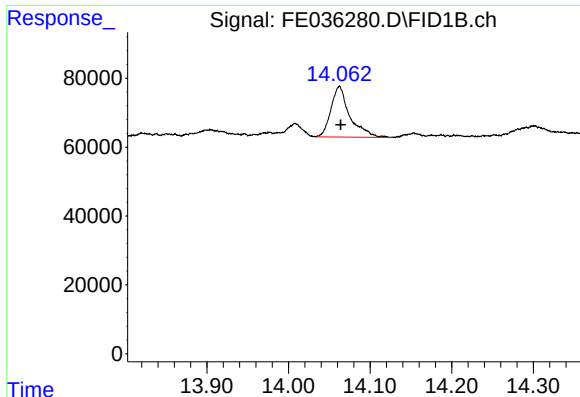

#13 n-Docosane (C22)


R.T.: 14.062 min
Delta R.T.: -0.002 min
Response: 235968
Conc: 1.33 ug/ml

Instrument :
FID_E
ClientSampleId :

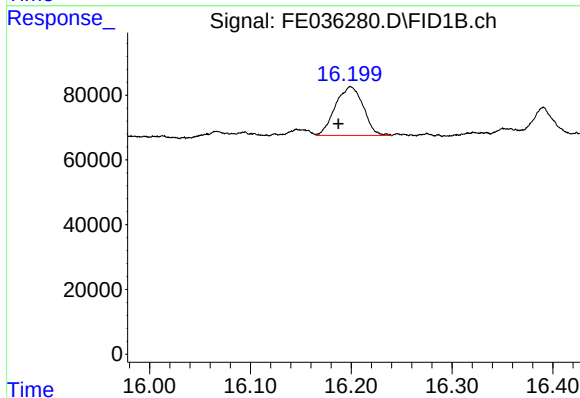


#15 n-Hexacosane (C26)

R.T.: 16.199 min
Delta R.T.: 0.012 min
Response: 288743
Conc: 1.75 ug/ml

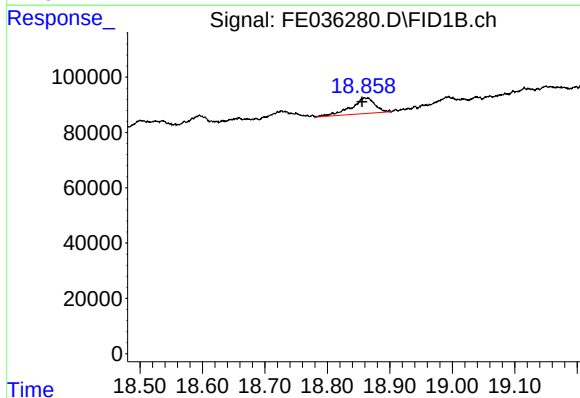


#18 n-Dotriacontane (C32)

R.T.: 18.860 min
Delta R.T.: 0.004 min
Response: 147932
Conc: 1.01 ug/ml

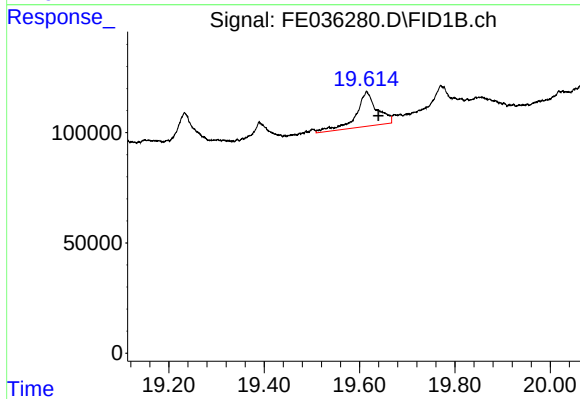

#19 n-Tetratriacontane (C34)

R.T.: 19.615 min
Delta R.T.: -0.025 min
Response: 477320
Conc: 3.45 ug/ml

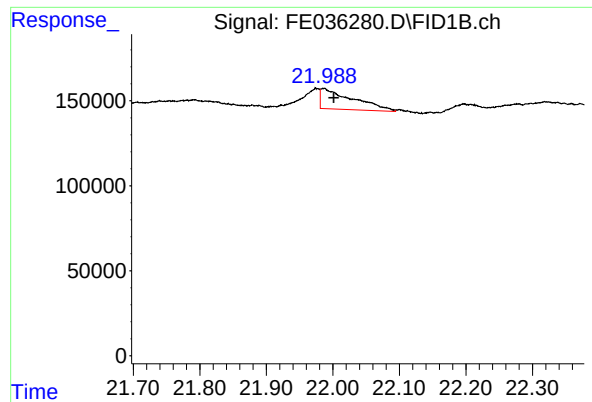

#22 n-Tetracontane (C40)

R.T.: 21.986 min
Delta R.T.: -0.015 min
Response: 405745
Conc: 2.90 ug/ml

Instrument :

FID_E

ClientSampleId :