

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
 Data File : FE036287.D
 Signal(s) : FID1B.ch
 Acq On : 29 Jun 2022 12:46
 Operator : YP\AJ
 Sample : N3514-02DL 100X
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jun 30 01:28:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 21 03:08:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.831	43073	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
12) S 1-chlorooctadecane (S...	13.312	85193	<MDL ug/ml
Spiked Amount 50.000		Recovery =	0.00%
Target Compounds			
1) T n-Nonane (C9)	3.282	65602	<MDL ug/ml
2) T n-Decane (C10)	4.458f	64259	<MDL ug/ml
3) T A~Naphthalene (C11.7)	6.218	121386	<MDL ug/ml
4) T n-Dodecane (C12)	6.705	62184	<MDL ug/ml
5) T A~2-methylnaphthalene...	7.315	108943	<MDL ug/ml
6) T n-Tetradecane (C14)	8.511	62302	<MDL ug/ml
7) T n-Hexadecane (C16)	10.120	31838	<MDL ug/ml
21) T n-Octatriacontane (C38)	21.105	96937	<MDL ug/ml
22) T n-Tetracontane (C40)	21.992	260678	1.864 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
Data File : FE036287.D
Signal(s) : FID1B.ch
Acq On : 29 Jun 2022 12:46
Operator : YP\AJ
Sample : N3514-02DL 100X
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 30 01:28:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

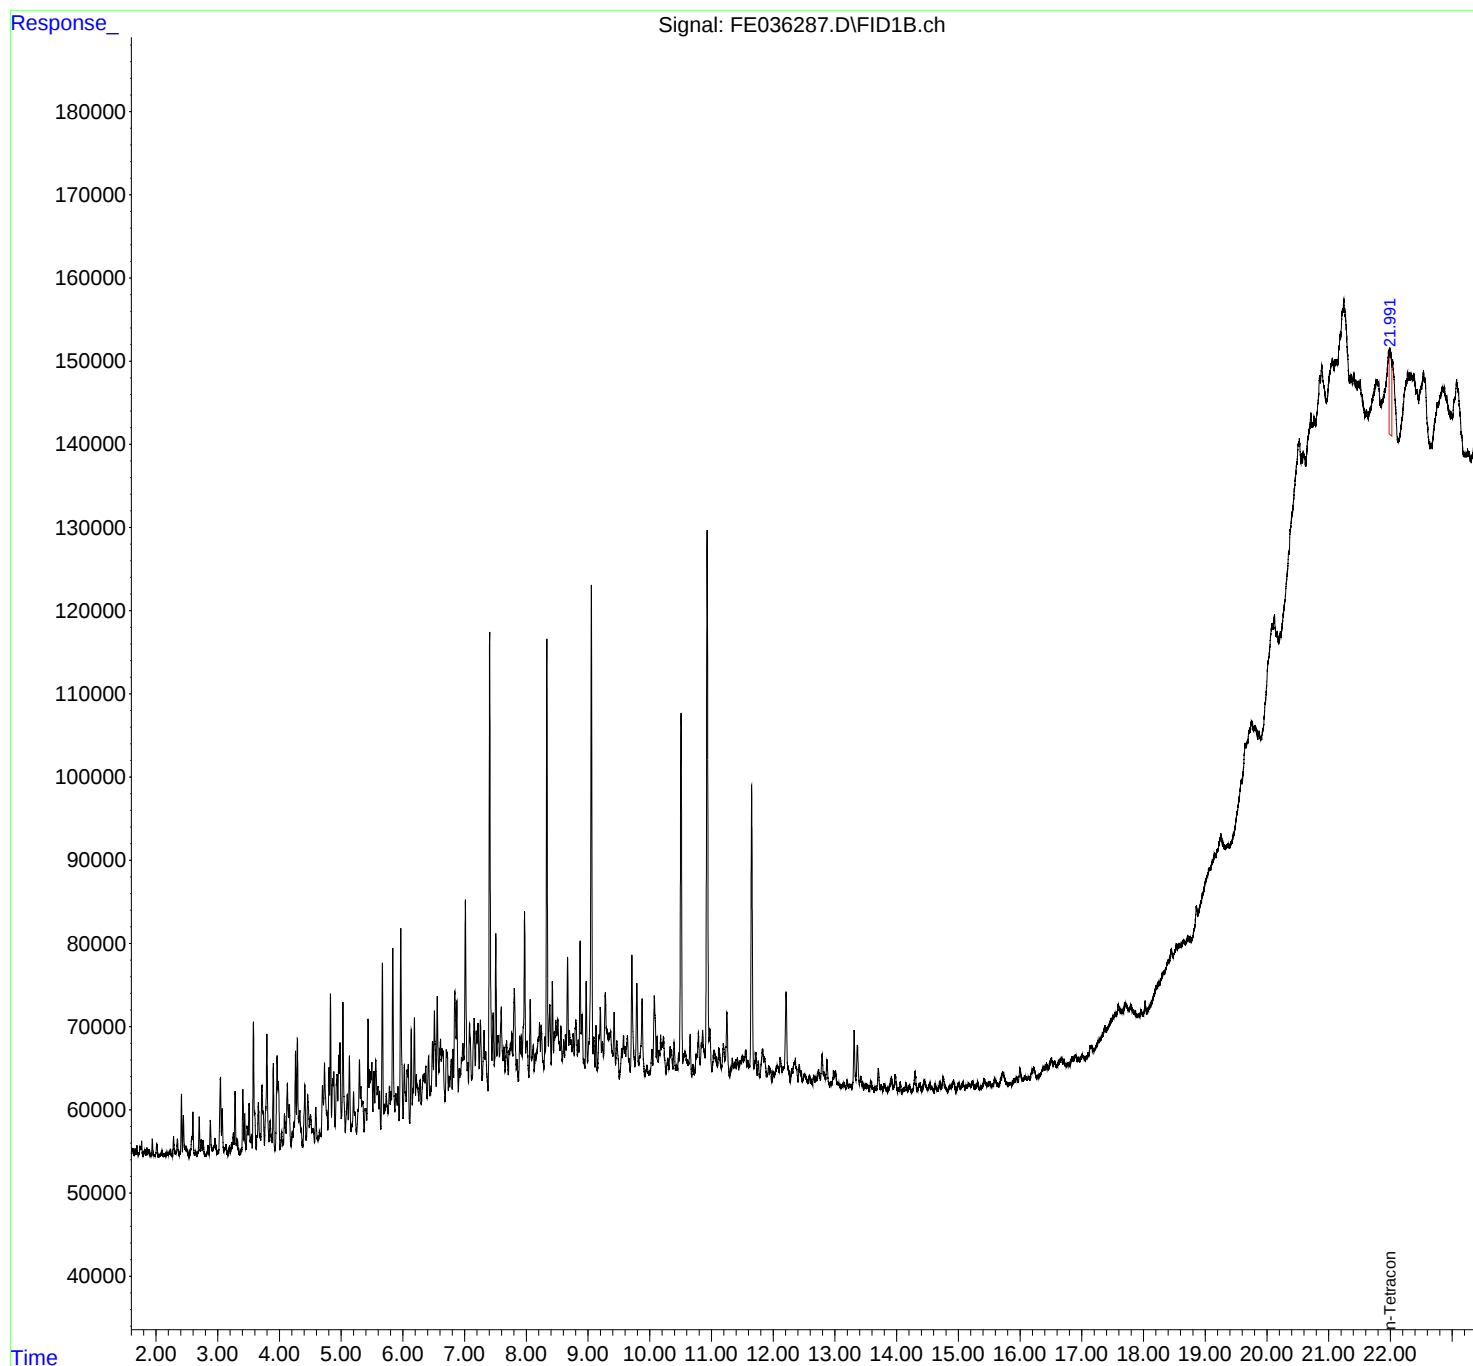


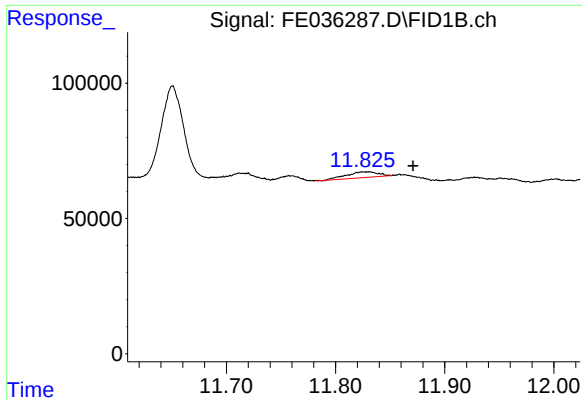

#9 ortho-Terphenyl (SURR)


R.T.: 11.831 min
Delta R.T.: -0.040 min
Response: 43073
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

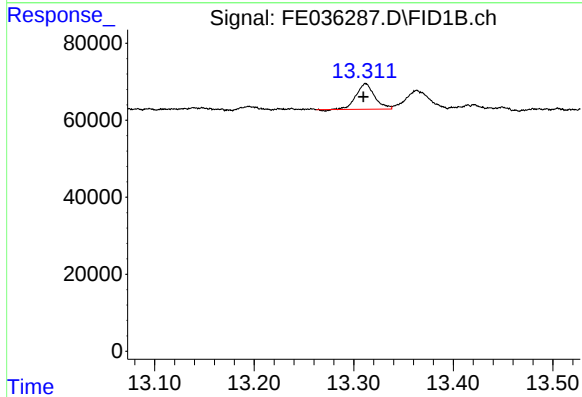

#12 1-chlorooctadecane (SURR)

R.T.: 13.312 min
Delta R.T.: 0.002 min
Response: 85193
Conc: N.D.

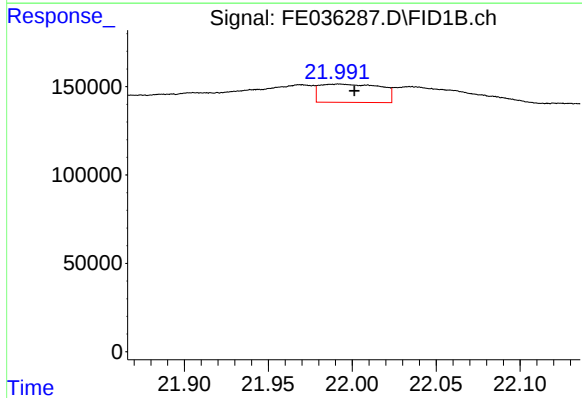

#22 n-Tetracontane (C40)

R.T.: 21.992 min
Delta R.T.: -0.009 min
Response: 260678
Conc: 1.86 ug/ml