

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
Data File : FE036291.D
Signal(s) : FID1B.ch
Acq On : 29 Jun 2022 14:48
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 30 01:29:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
22) T n-Tetracontane (C40)	21.966	1500339	10.730 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE062922AL\
Data File : FE036291.D
Signal(s) : FID1B.ch
Acq On : 29 Jun 2022 14:48
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jun 30 01:29:00 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

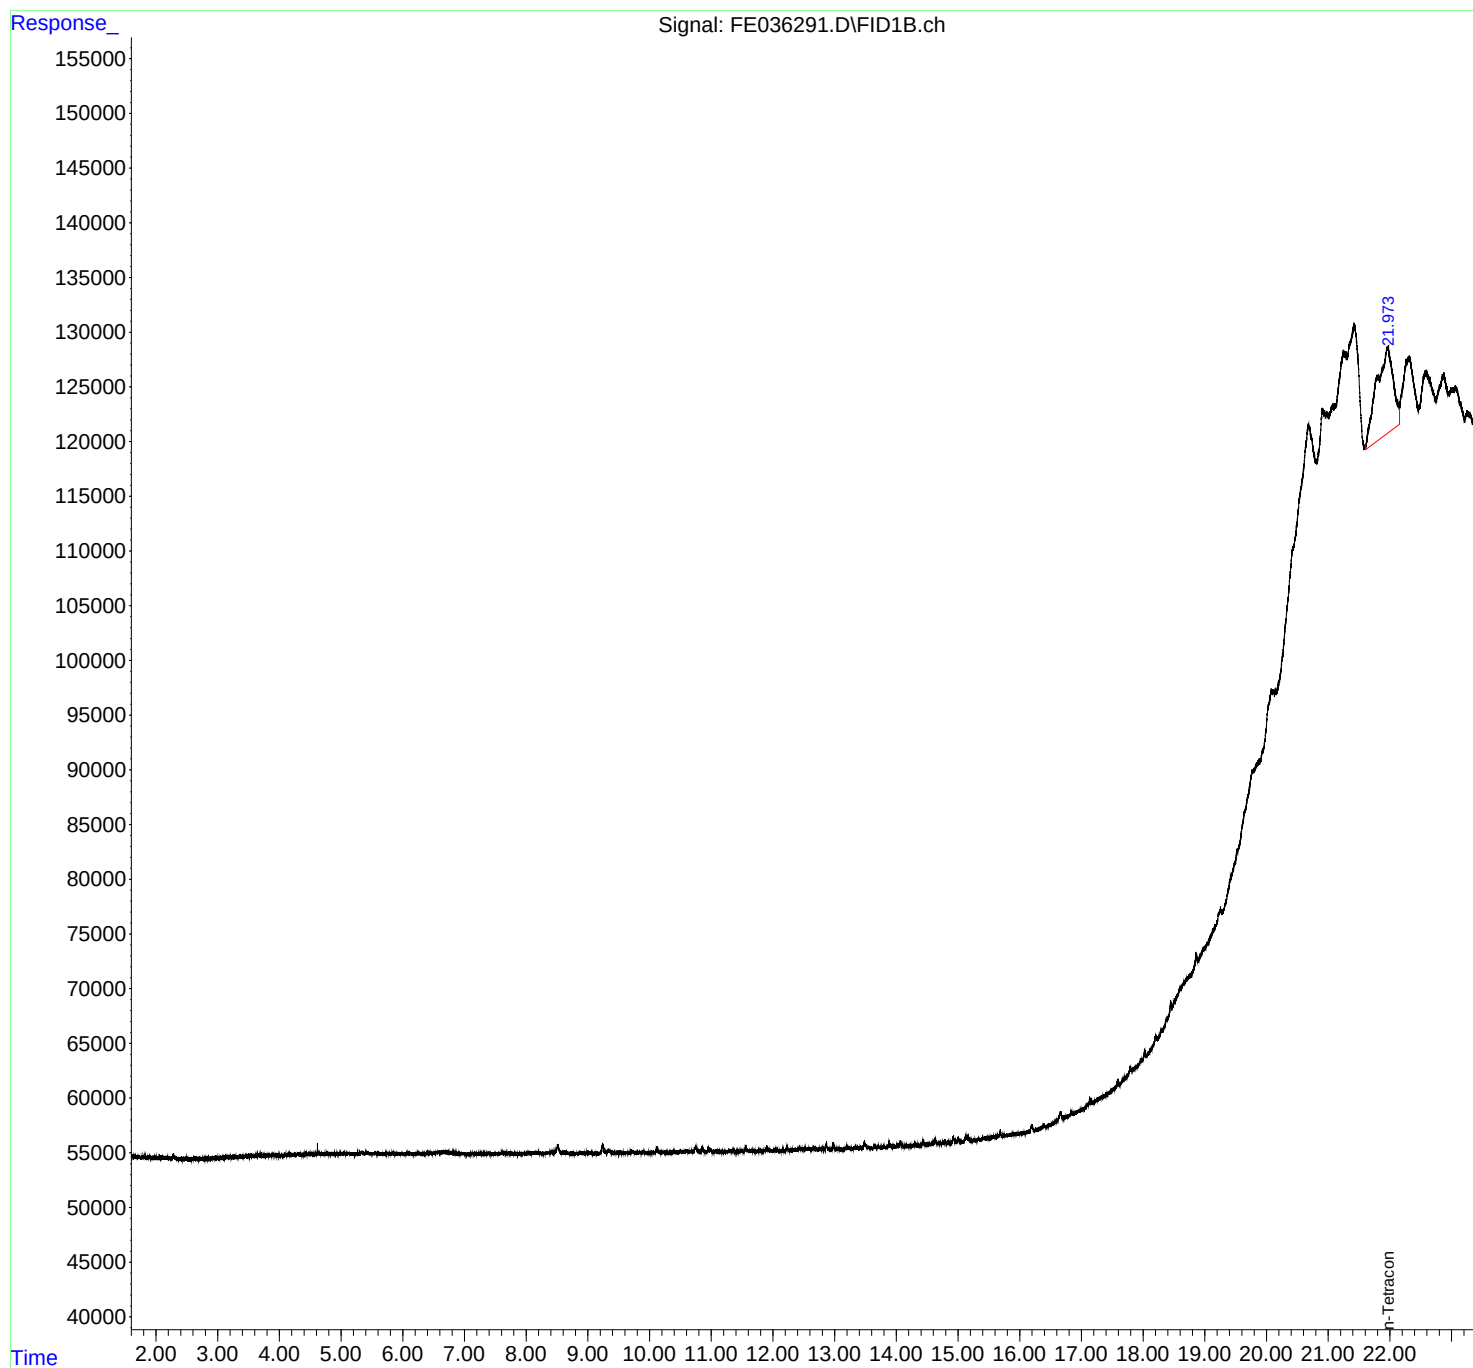


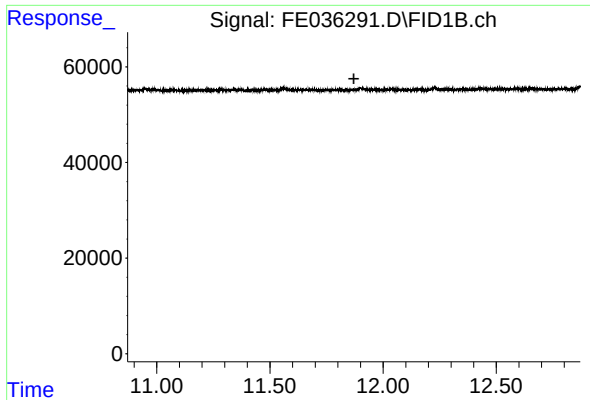

#9 ortho-Terphenyl (SURRE)


R.T.: 0.000 min
Exp R.T. : 11.871 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

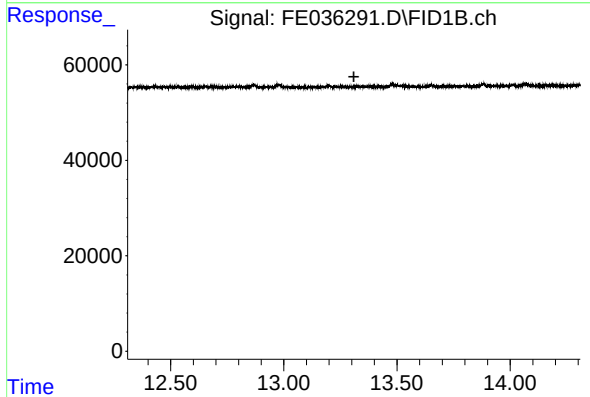

#12 1-chlorooctadecane (SURRE)

R.T.: 0.000 min
Exp R.T. : 13.310 min
Response: 0
Conc: N.D.

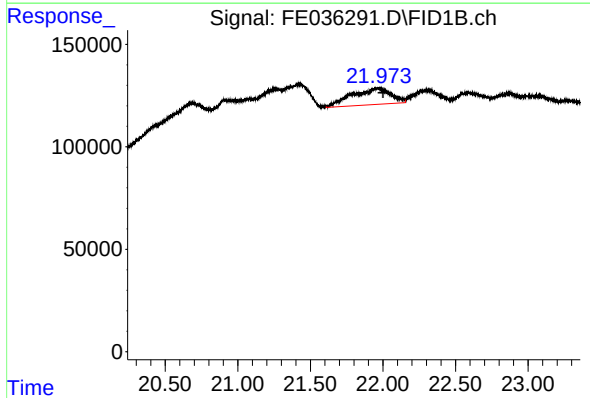

#22 n-Tetracontane (C40)

R.T.: 21.966 min
Delta R.T.: -0.035 min
Response: 1500339
Conc: 10.73 ug/ml