

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070120\
 Data File : FE032295.D
 Signal(s) : FID1B.CH
 Acq On : 01 Jul 2020 17:18
 Operator : DD\AJ
 Sample : L2811-05 2X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 NB-7-063020

Integration File: autoint1.e
 Quant Time: Jul 02 01:19:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
 Quant Title :
 QLast Update : Thu Jun 11 13:38:20 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.763	3235613	10.120 ug/ml
Target Compounds			
4) N-TETRADECANE	8.279	1469559	3.968 ug/ml
7) N-EICOSANE	12.663	190772	0.514 ug/ml
8) N-DOCOSANE	13.862	222081	0.600 ug/ml
10) N-TETRACOSANE	14.964	277989	0.749 ug/ml
11) N-HEXACOSANE	15.960	115995	0.317 ug/ml
12) N-OCTACOSANE	16.945	827848	2.265 ug/ml
13) N-TRIACONTANE	17.790	994991	2.733 ug/ml
14) N-DOTRIACONTANE	18.612	2851506	8.327 ug/ml
15) N-TETRATRIACONTANE	19.417	9907161	34.733 ug/ml
16) N-HEXATRIACONTANE	20.157	17995939	83.470 ug/ml
17) N-OCTATRIACONTANE	20.883	13918222	81.440 ug/ml
18) N-TETRACONTANE	21.843	66749	0.441 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070120\
Data File : FE032295.D
Signal(s) : FID1B.CH
Acq On : 01 Jul 2020 17:18
Operator : DD\AJ
Sample : L2811-05 2X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
FID_E
ClientSampled :
NB-7-063020

Integration File: autoint1.e
Quant Time: Jul 02 01:19:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE061120.M
Quant Title :
QLast Update : Thu Jun 11 13:38:20 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

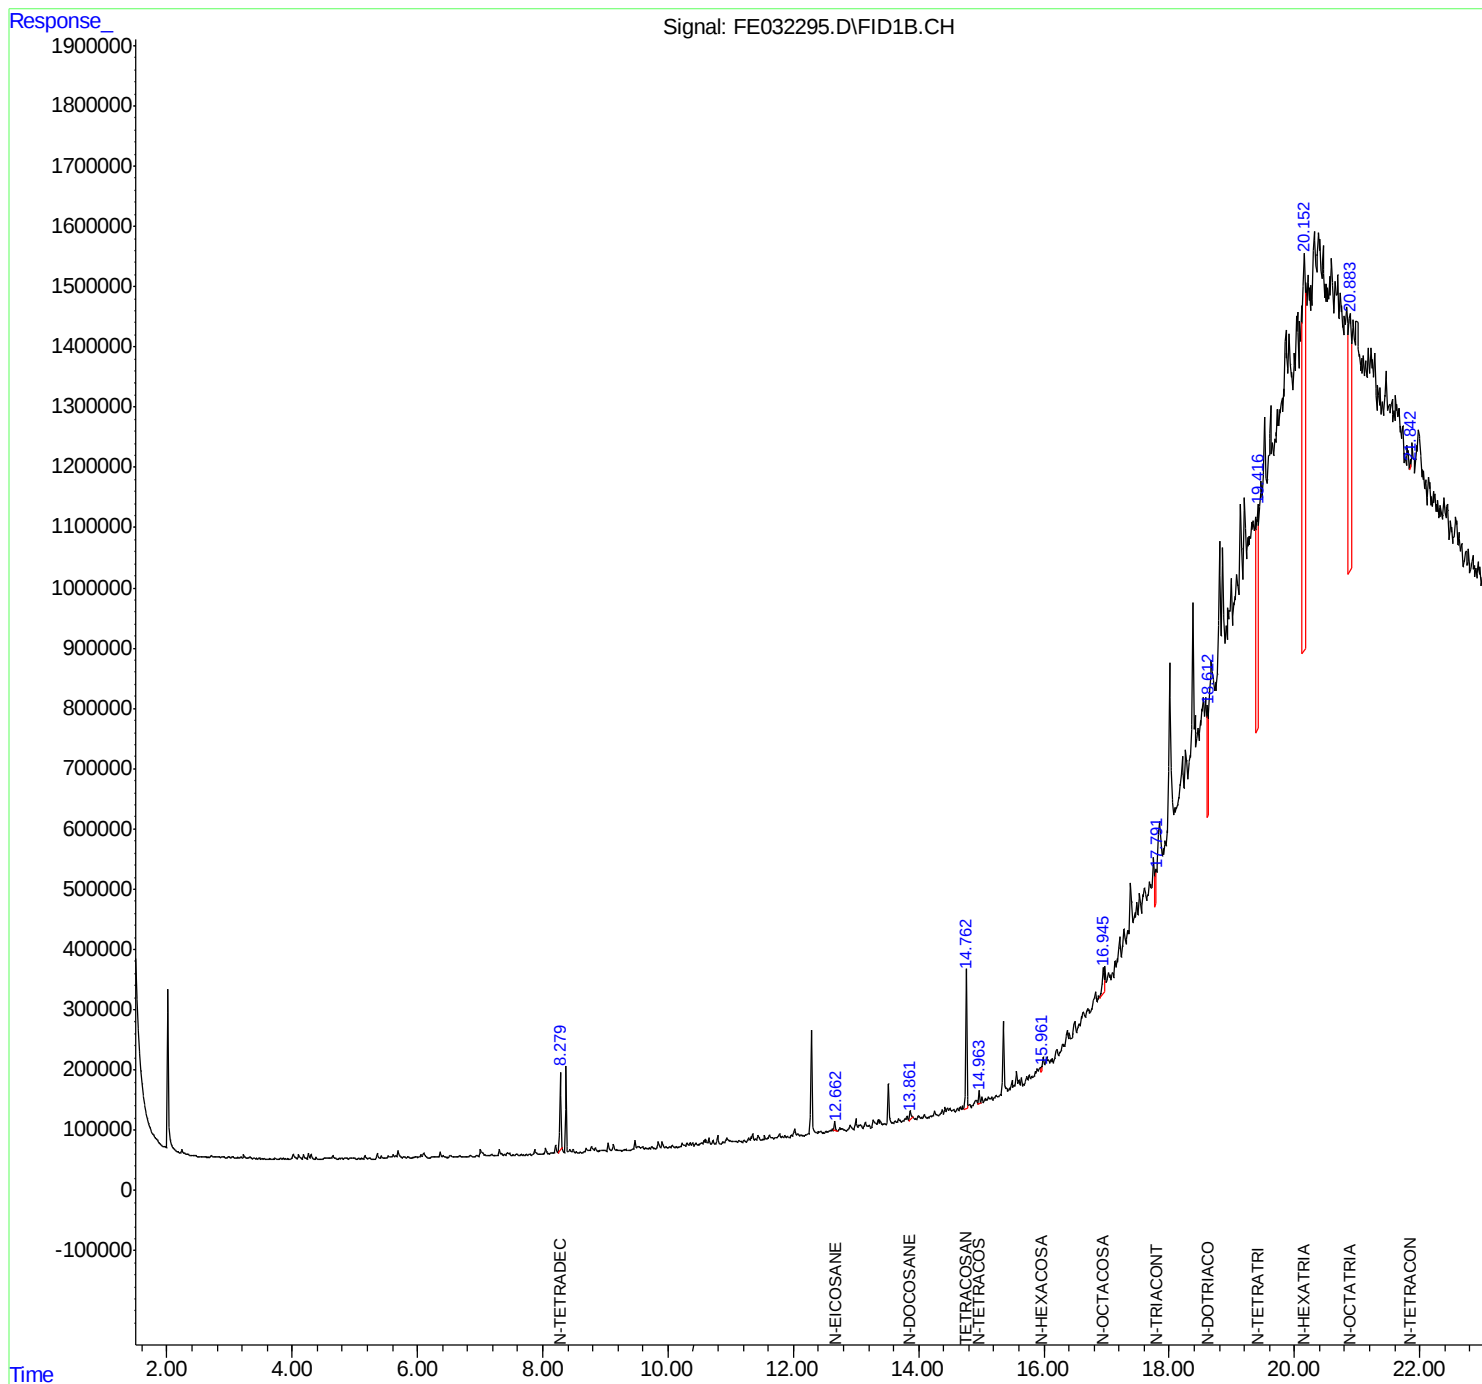


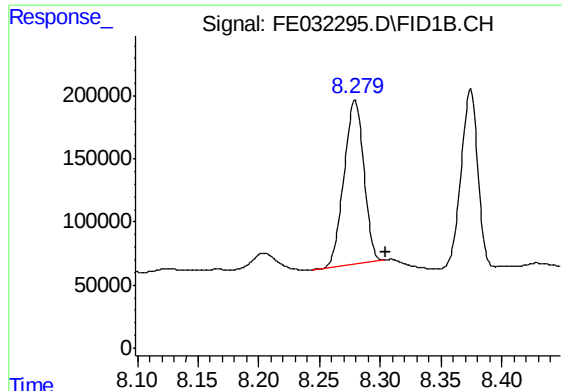

#4 N-TETRADECANE


R.T.: 8.279 min
Delta R.T.: -0.025 min
Response: 1469559
Conc: 3.97 ug/ml

Instrument :
FID_E
ClientSampleId :
NB-7-063020

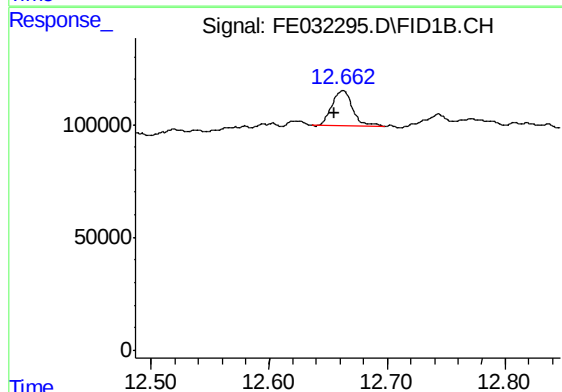


#7 N-EICOSANE

R.T.: 12.663 min
Delta R.T.: 0.008 min
Response: 190772
Conc: 0.51 ug/ml

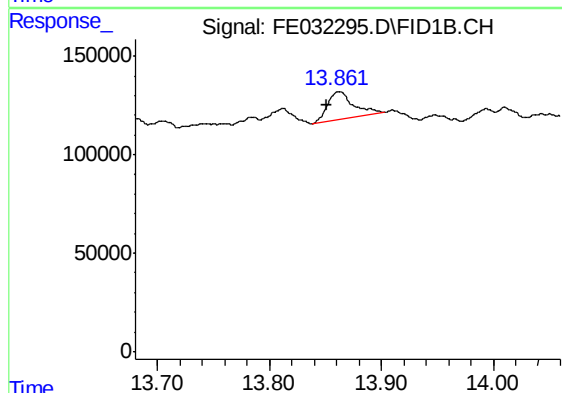


#8 N-DOCOSANE

R.T.: 13.862 min
Delta R.T.: 0.010 min
Response: 222081
Conc: 0.60 ug/ml

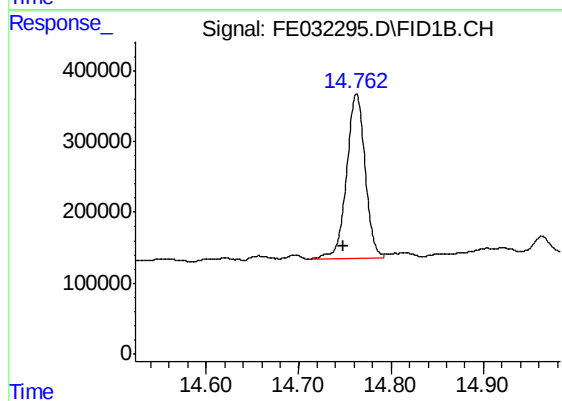

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.763 min
Delta R.T.: 0.014 min
Response: 3235613
Conc: 10.12 ug/ml

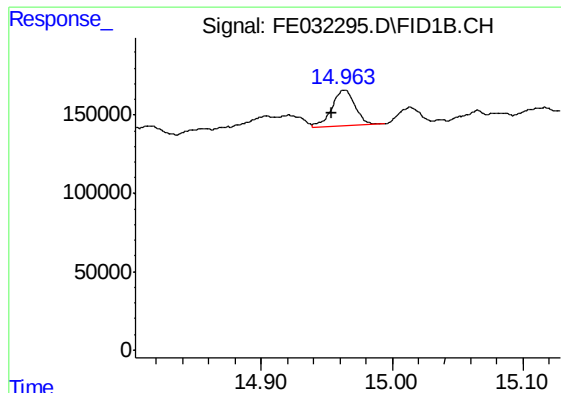

#10 N-TETRACOSANE


R.T.: 14.964 min
Delta R.T.: 0.009 min
Response: 277989
Conc: 0.75 ug/ml

Instrument :
FID_E
ClientSampleId :
NB-7-063020

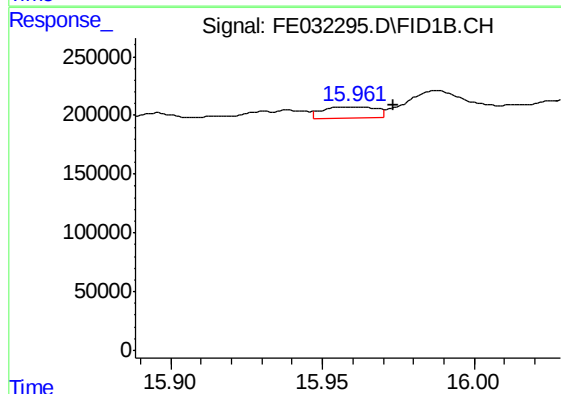


#11 N-HEXACOSANE

R.T.: 15.960 min
Delta R.T.: -0.013 min
Response: 115995
Conc: 0.32 ug/ml

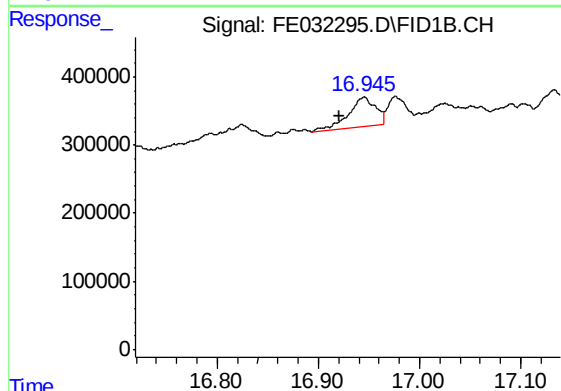


#12 N-OCTACOSANE

R.T.: 16.945 min
Delta R.T.: 0.024 min
Response: 827848
Conc: 2.27 ug/ml

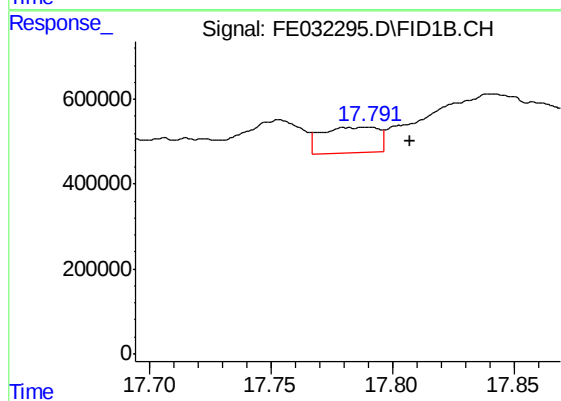

#13 N-TRIACONTANE


R.T.: 17.790 min
Delta R.T.: -0.017 min
Response: 994991
Conc: 2.73 ug/ml

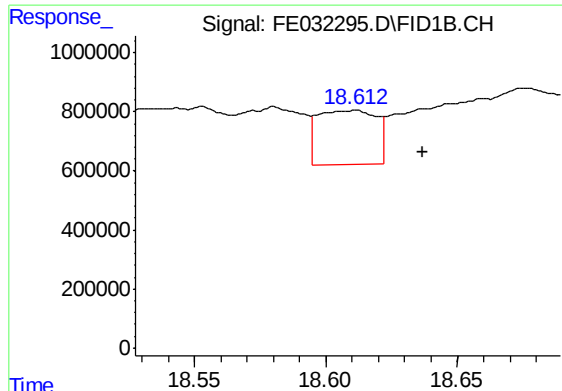

#14 N-DOTRIACONTANE


R.T.: 18.612 min
Delta R.T.: -0.025 min
Response: 2851506
Conc: 8.33 ug/ml

Instrument :
FID_E
ClientSampleId :
NB-7-063020

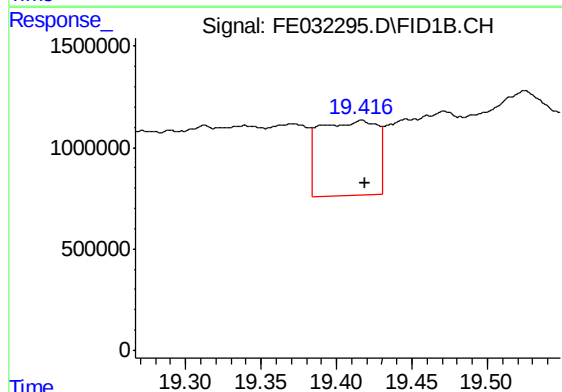


#15 N-TETRATRIACONTANE

R.T.: 19.417 min
Delta R.T.: -0.003 min
Response: 9907161
Conc: 34.73 ug/ml

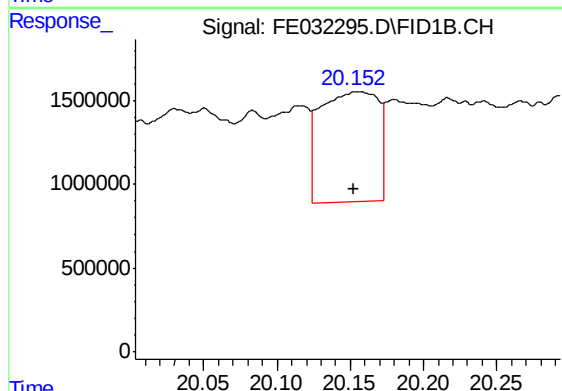


#16 N-HEXATRIACONTANE

R.T.: 20.157 min
Delta R.T.: 0.005 min
Response: 17995939
Conc: 83.47 ug/ml

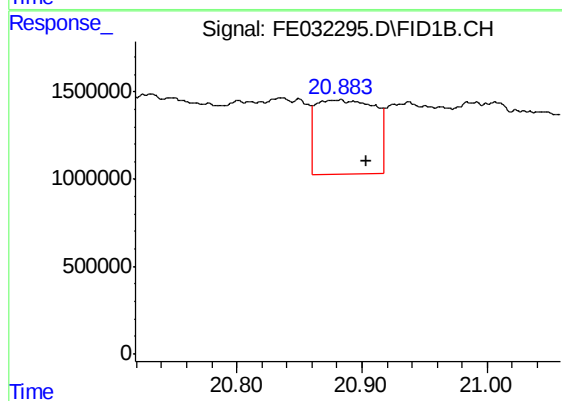

#17 N-OCTATRIACONTANE

R.T.: 20.883 min
Delta R.T.: -0.021 min
Response: 13918222
Conc: 81.44 ug/ml

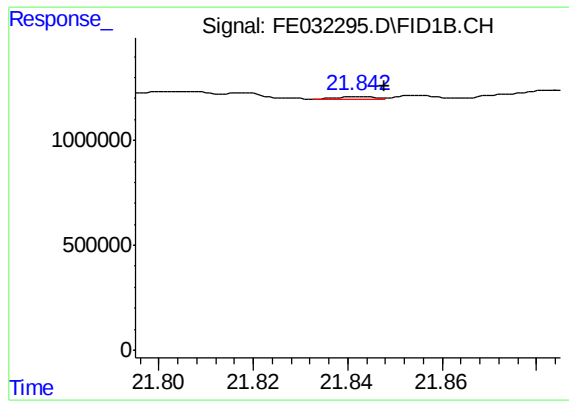

#18 N-TETRACONTANE

R.T.: 21.843 min
Delta R.T.: -0.005 min
Response: 66749
Conc: 0.44 ug/ml

Instrument :
FID_E
ClientSampleId :
NB-7-063020