

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070122AL\
 Data File : FE036329.D
 Signal(s) : FID1B.ch
 Acq On : 01 Jul 2022 08:47
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 02 03:32:08 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
 Quant Title : GC Extractables
 QLast Update : Tue Jun 21 03:08:45 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

10) T	n-Eicosane (C20)	12.859	111944	<MDL	ug/ml
11) T	n-Heneicosane (C21)	13.475	153121	<MDL	ug/ml
13) T	n-Docosane (C22)	14.061	126614	<MDL	ug/ml
14) T	n-Tetracosane (C24)	15.164	76717	<MDL	ug/ml
15) T	n-Hexacosane (C26)	16.195	140837	<MDL	ug/ml
16) T	n-Octacosane (C28)	17.134	57947	<MDL	ug/ml
17) T	n-Tricontane (C30)	17.964	26769	<MDL	ug/ml
18) T	n-Dotriacontane (C32)	18.851	228236	1.562	ug/ml
19) T	n-Tetratriacontane (C34)	19.644	24601	<MDL	ug/ml
20) T	n-Hexatriacontane (C36)	20.394	52071	<MDL	ug/ml
21) T	n-Octatriacontane (C38)	21.096	129996	<MDL	ug/ml
22) T	n-Tetracontane (C40)	21.977	858165	6.137	ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070122AL\
Data File : FE036329.D
Signal(s) : FID1B.ch
Acq On : 01 Jul 2022 08:47
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 02 03:32:08 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062022.M
Quant Title : GC Extractables
QLast Update : Tue Jun 21 03:08:45 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

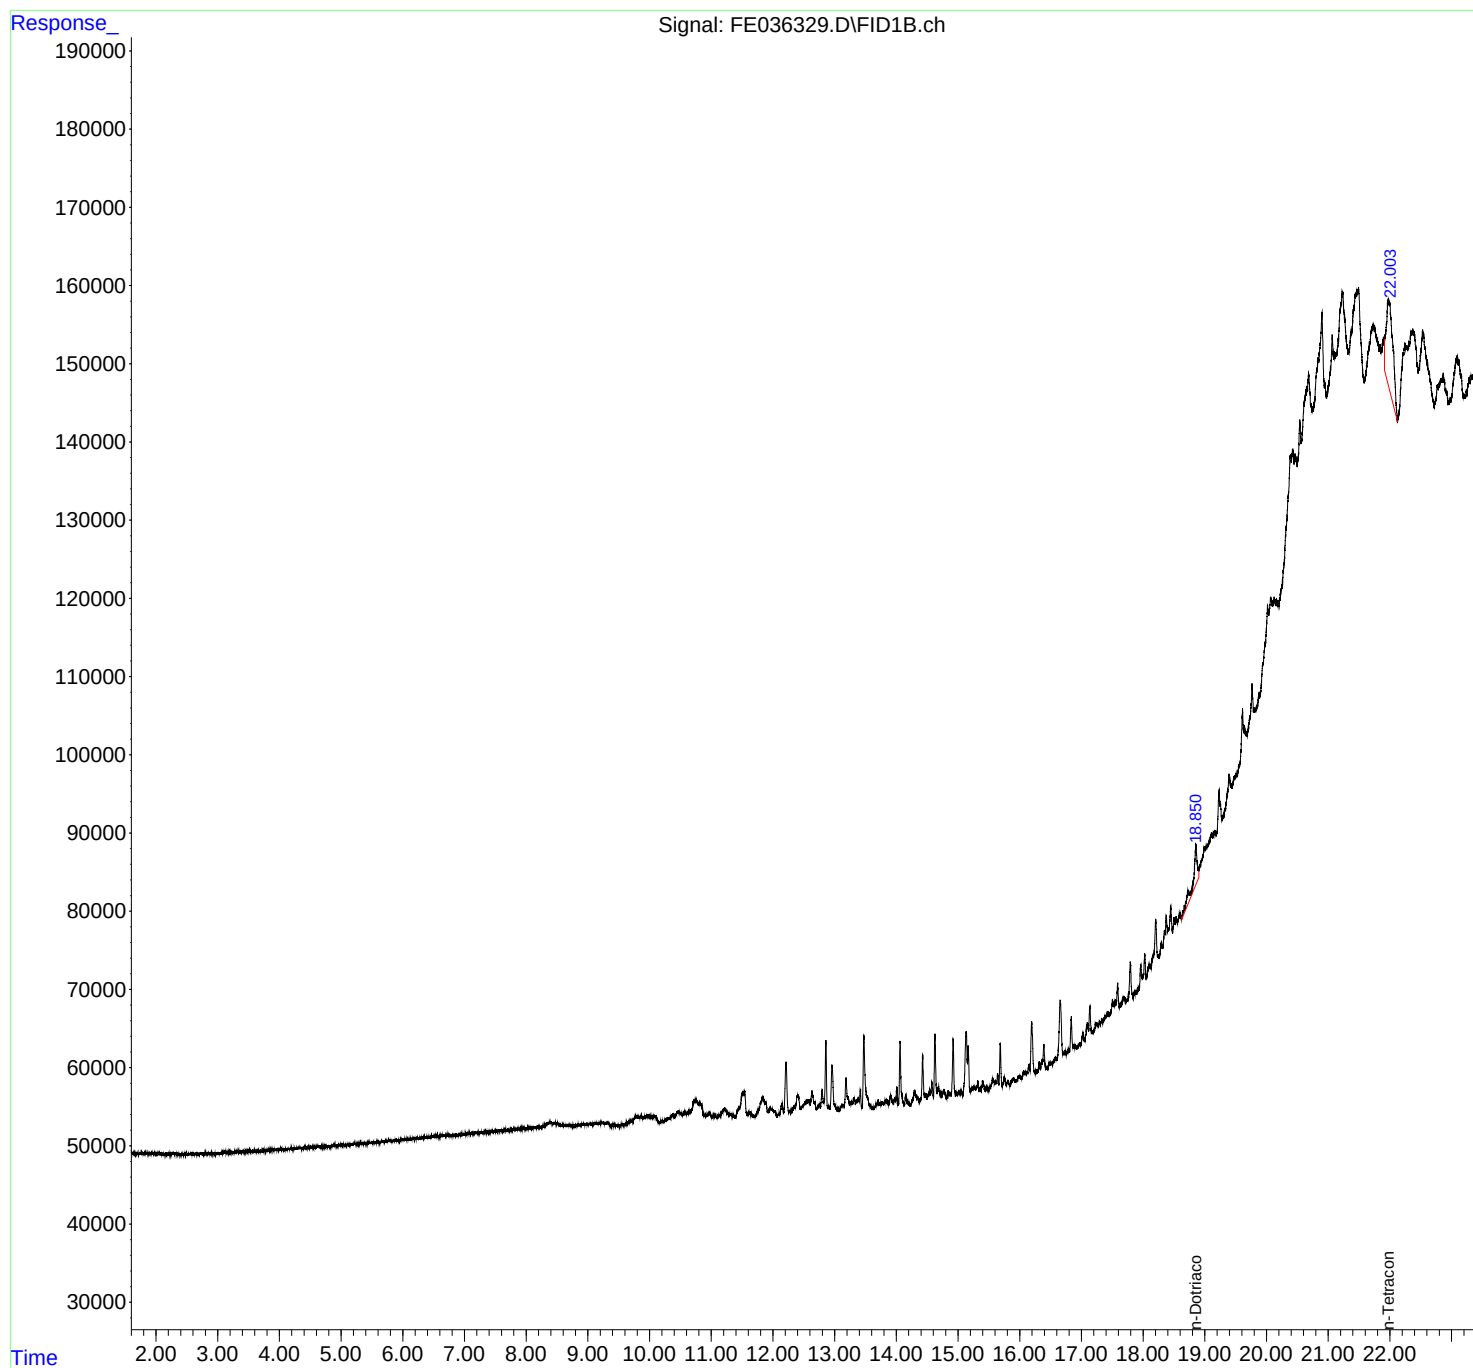


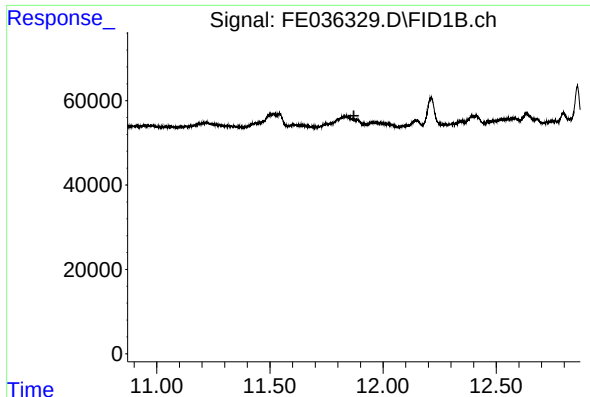

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.871 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

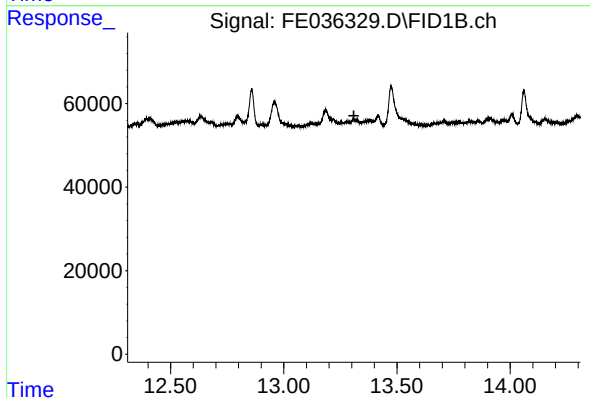


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.310 min
Response: 0
Conc: N.D.

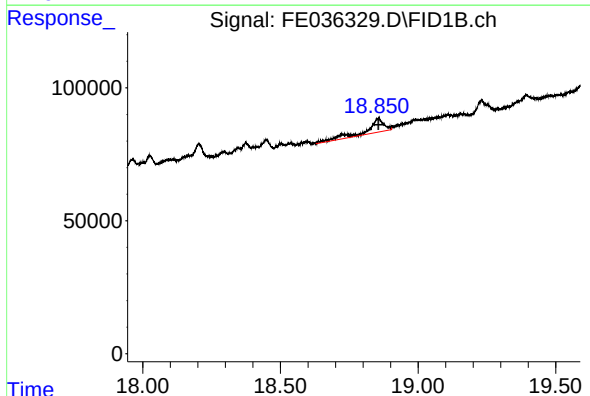

#18 n-Dotriacontane (C32)

R.T.: 18.851 min
Delta R.T.: -0.004 min
Response: 228236
Conc: 1.56 ug/ml

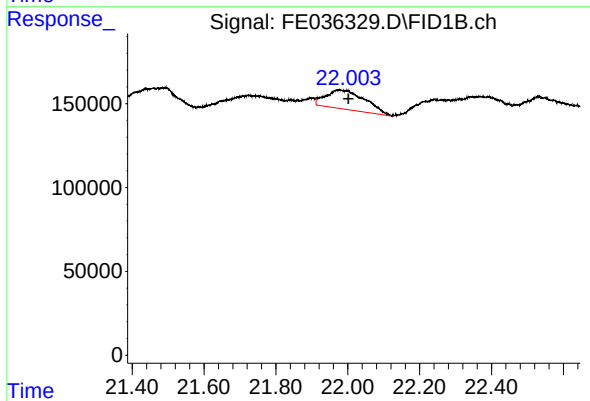

#22 n-Tetracontane (C40)

R.T.: 21.977 min
Delta R.T.: -0.024 min
Response: 858165
Conc: 6.14 ug/ml