

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070122AL\  
 Data File : FE036338.D  
 Signal(s) : FID1B.ch  
 Acq On : 01 Jul 2022 14:08  
 Operator : YP\AJ  
 Sample : N3550-01DL 10X  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 HR-02-06292022DL

Integration File: sample.E  
 Quant Time: Jul 02 03:33:36 2022  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062022.M  
 Quant Title : GC Extractables  
 QLast Update : Tue Jun 21 03:08:45 2022  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.870 | 893787     | 4.474 ug/ml  |
| Spiked Amount 50.000           |        | Recovery = | 8.95%        |
| 12) S 1-chlorooctadecane (S... | 13.295 | 3151120    | 20.354 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 40.71%       |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070122AL\  
Data File : FE036338.D  
Signal(s) : FID1B.ch  
Acq On : 01 Jul 2022 14:08  
Operator : YP\AJ  
Sample : N3550-01DL 10X  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
HR-02-06292022DL

Integration File: sample.E  
Quant Time: Jul 02 03:33:36 2022  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062022.M  
Quant Title : GC Extractables  
QLast Update : Tue Jun 21 03:08:45 2022  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

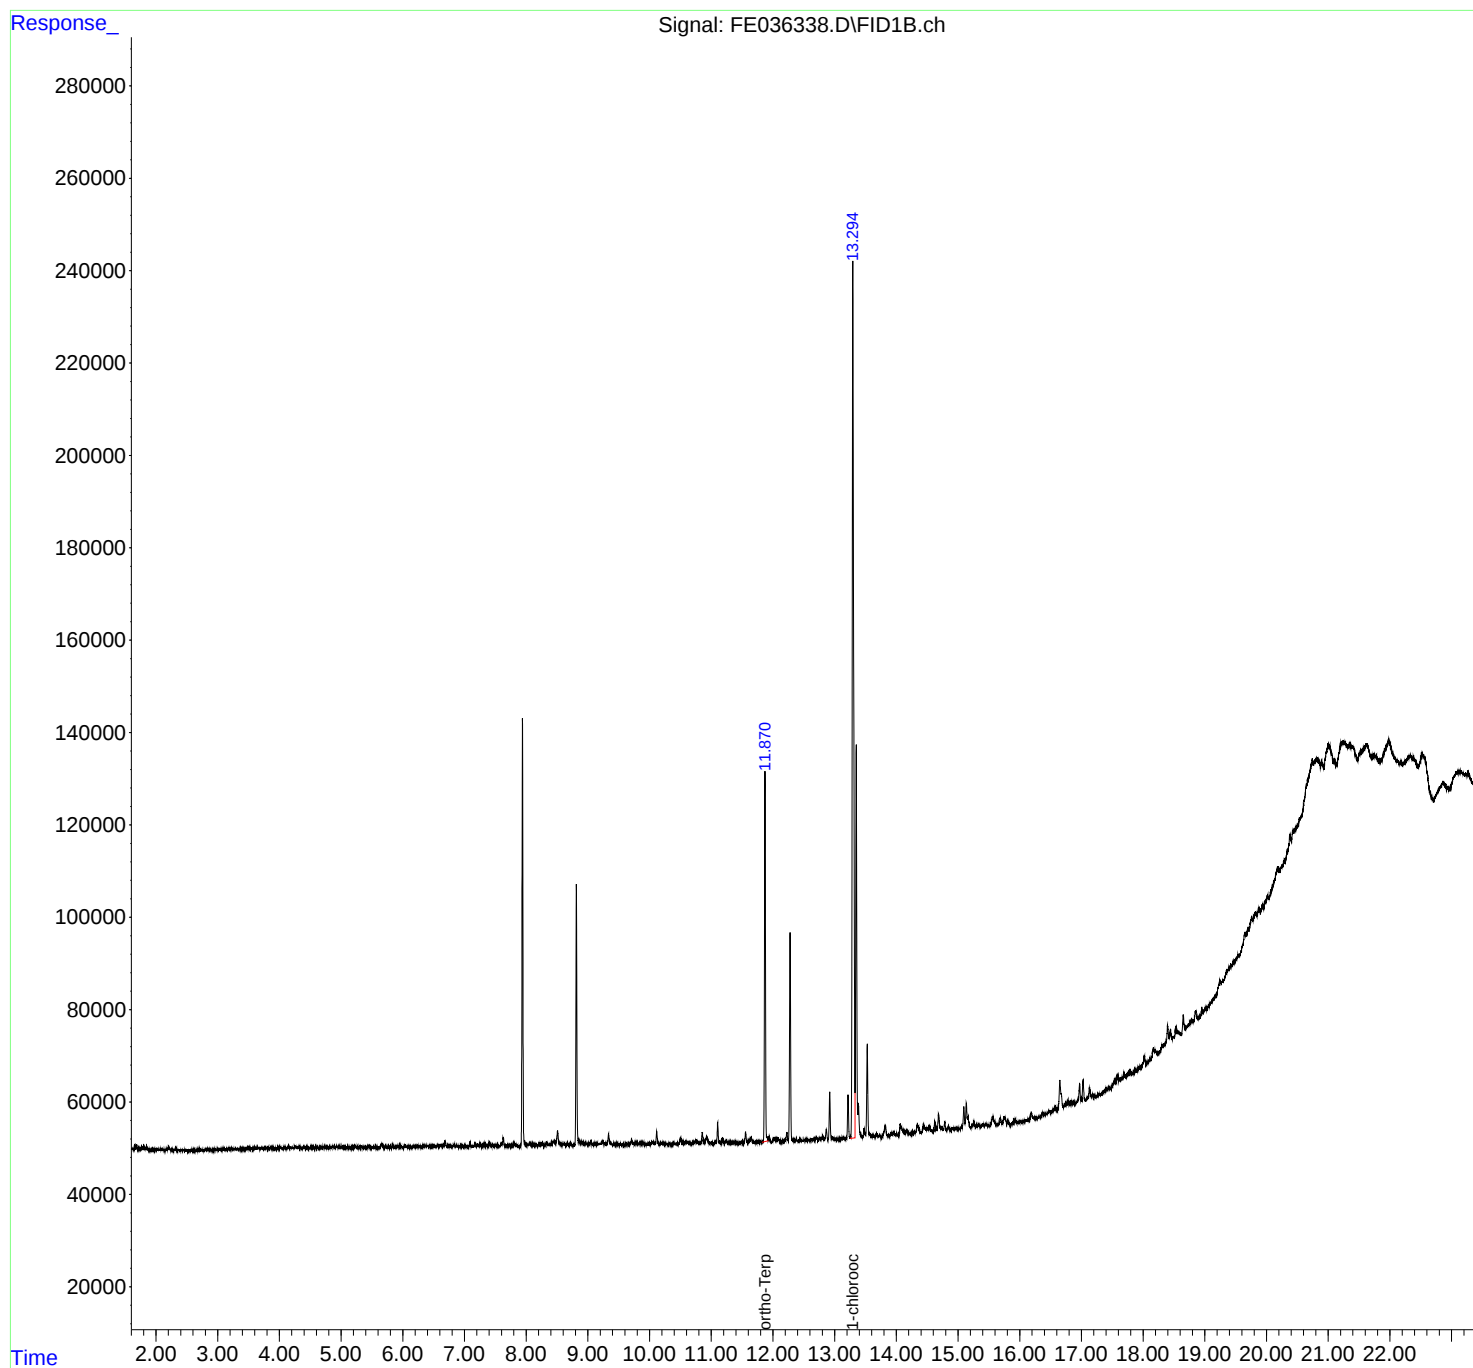


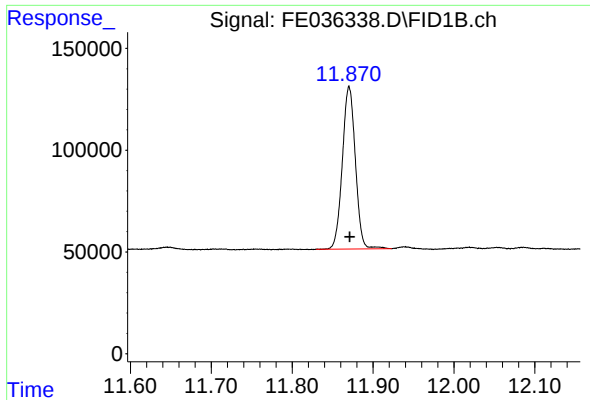

#9 ortho-Terphenyl (SURR)

R.T.: 11.870 min  
Delta R.T.: 0.000 min  
Response: 893787  
Conc: 4.47 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
HR-02-06292022DL

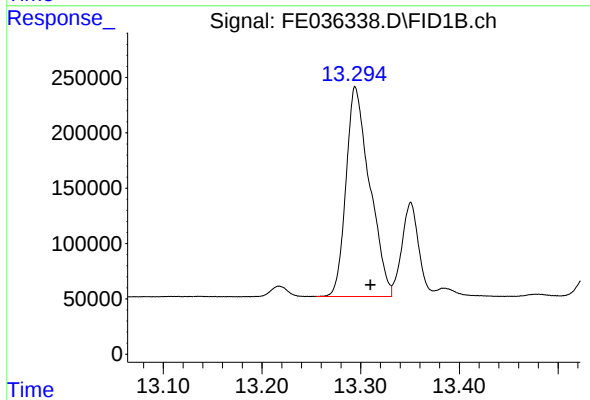

#12 1-chlorooctadecane (SURR)

R.T.: 13.295 min  
Delta R.T.: -0.015 min  
Response: 3151120  
Conc: 20.35 ug/ml