

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070124AL\
Data File : FE048937.D
Signal(s) : FID1B.ch
Acq On : 01 Jul 2024 08:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 11:38:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
Quant Title : GC Extractables
QLast Update : Thu Jun 20 17:53:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
Target Compounds				
18) T	n-Dotriacontane (C32)	18.970f	814450	5.696 ug/ml
20) T	n-Hexatriacontane (C36)	20.406	142349	1.095 ug/ml
21) T	n-Octatriacontane (C38)	21.205	2846884	22.207 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070124AL\
Data File : FE048937.D
Signal(s) : FID1B.ch
Acq On : 01 Jul 2024 08:59
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 01 11:38:51 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
Quant Title : GC Extractables
QLast Update : Thu Jun 20 17:53:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 u1
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

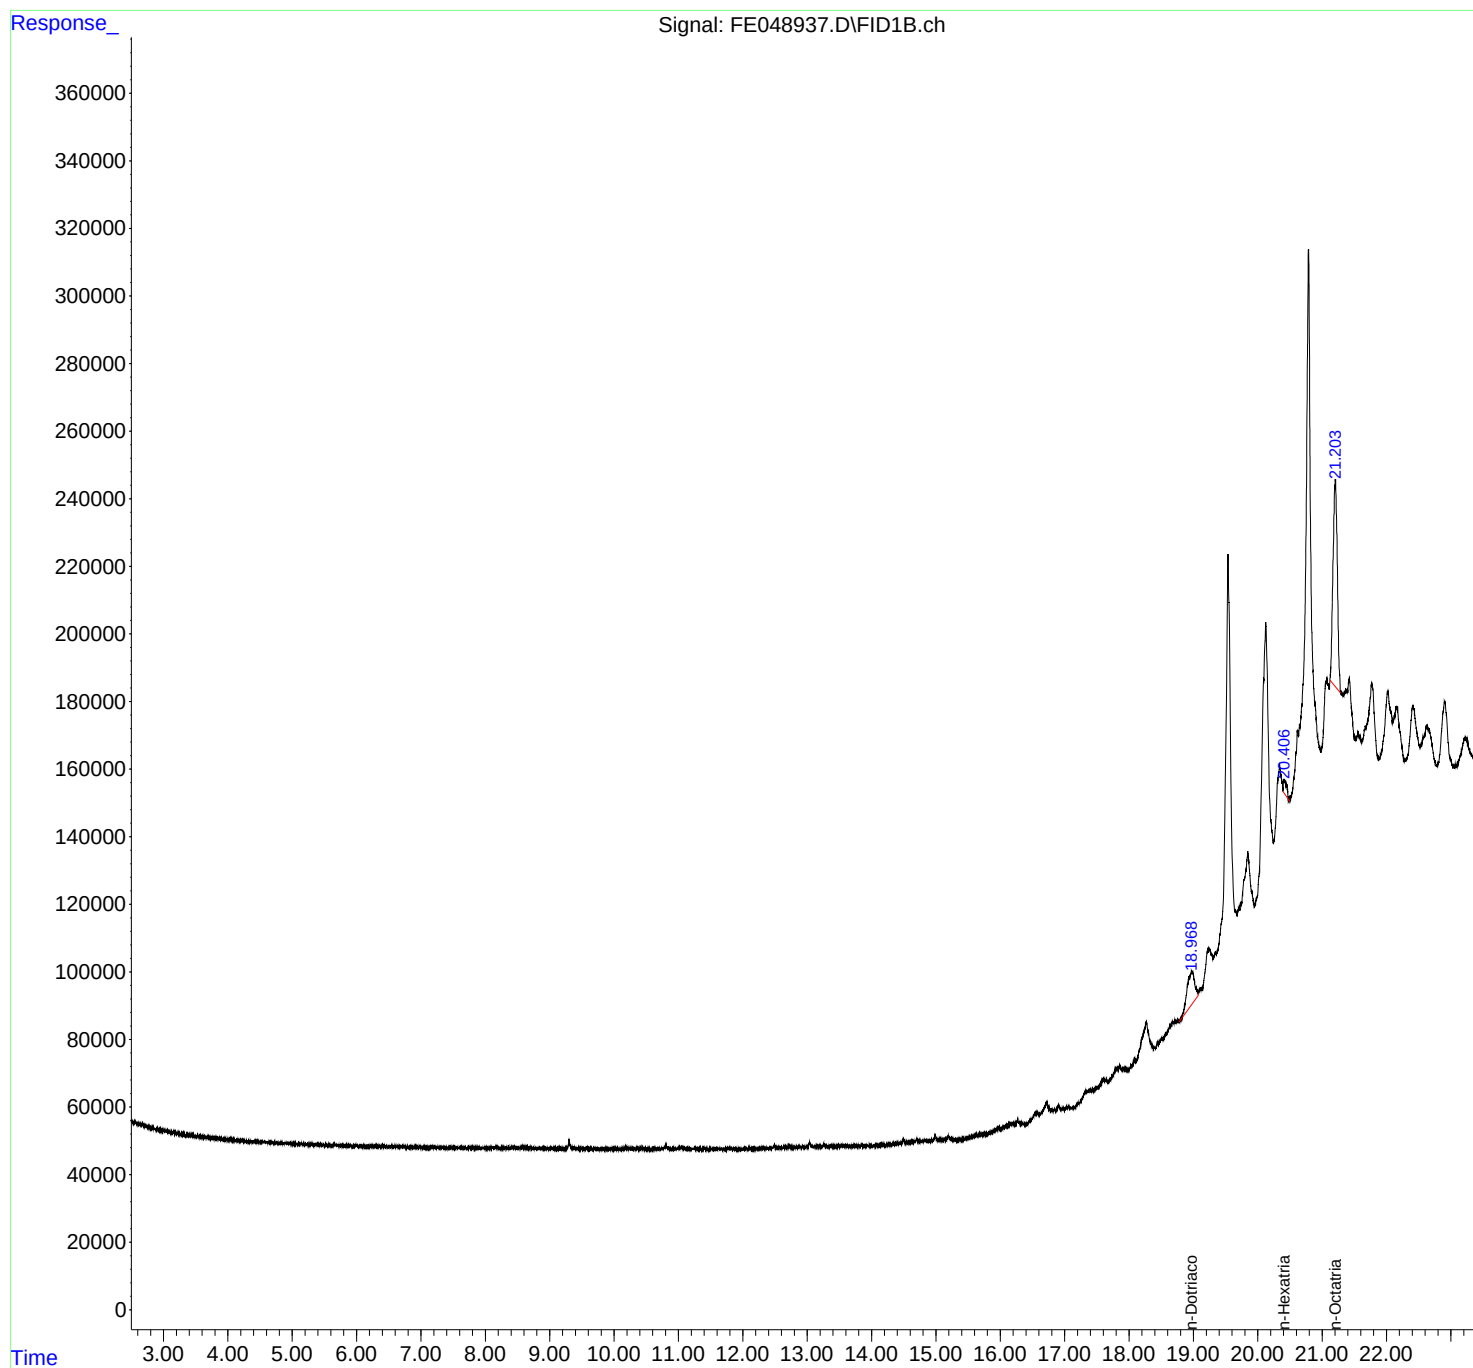


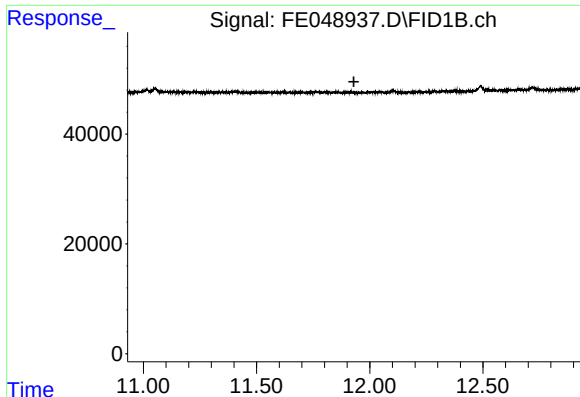

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.930 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

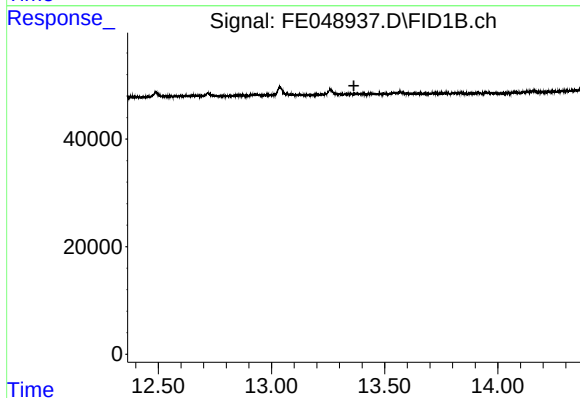


#12 1-chlorooctadecane (SURR)

R.T.: 0.000 min
Exp R.T.: 13.364 min
Response: 0
Conc: N.D.

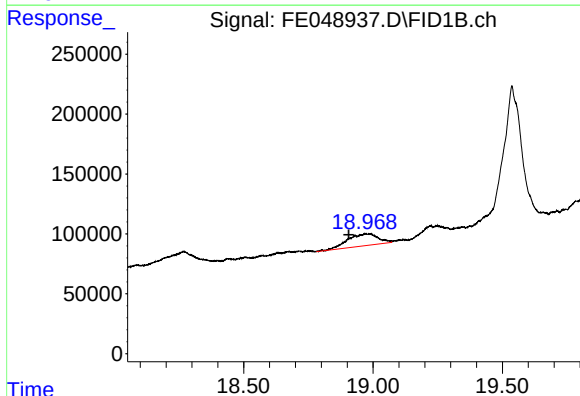


#18 n-Dotriacontane (C32)

R.T.: 18.970 min
Delta R.T.: 0.064 min
Response: 814450
Conc: 5.70 ug/ml

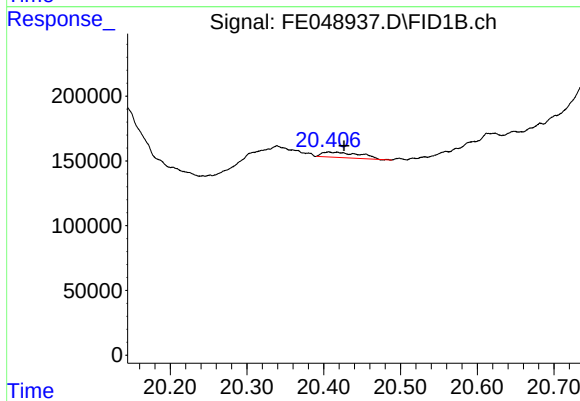

#20 n-Hexatriacontane (C36)

R.T.: 20.406 min
Delta R.T.: -0.020 min
Response: 142349
Conc: 1.10 ug/ml

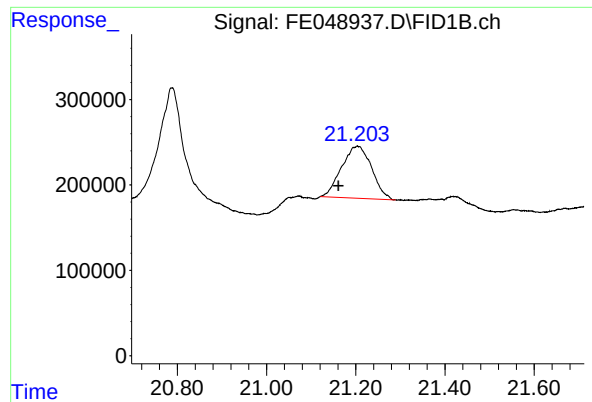

#21 n-Octatriacontane (C38)

R.T.: 21.205 min
Delta R.T.: 0.043 min
Response: 2846884
Conc: 22.21 ug/ml

Instrument :

FID_E

ClientSampleId :