

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070224AL\
 Data File : FE048959.D
 Signal(s) : FID1B.ch
 Acq On : 02 Jul 2024 06:02
 Operator : YP\AJ
 Sample : MECL2
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Jul 03 01:23:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
 Quant Title : GC Extractables
 QLast Update : Thu Jun 20 17:53:58 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
10) T n-Eicosane (C20)	12.905	127666	0.823 ug/ml
11) T n-Heneicosane (C21)	13.530	321028	2.108 ug/ml
13) T n-Docosane (C22)	14.116	110464	0.730 ug/ml
14) T n-Tetracosane (C24)	15.180	682724	4.543 ug/ml
15) T n-Hexacosane (C26)	16.259	695135	4.709 ug/ml
16) T n-Octacosane (C28)	17.189	97134	0.674 ug/ml
17) T n-Tricontane (C30)	18.079	82441	0.564 ug/ml
18) T n-Dotriacontane (C32)	18.910	102367	0.716 ug/ml
19) T n-Tetratriacontane (C34)	19.668	831205	6.007 ug/ml
20) T n-Hexatriacontane (C36)	20.438	2172	0.017 ug/ml
22) T n-Tetracontane (C40)	22.059	577230	4.714 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070224AL\
Data File : FE048959.D
Signal(s) : FID1B.ch
Acq On : 02 Jul 2024 06:02
Operator : YP\AJ
Sample : MECL2
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_E
ClientSampleId :

Integration File: autoint1.e
Quant Time: Jul 03 01:23:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062124.M
Quant Title : GC Extractables
QLast Update : Thu Jun 20 17:53:58 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

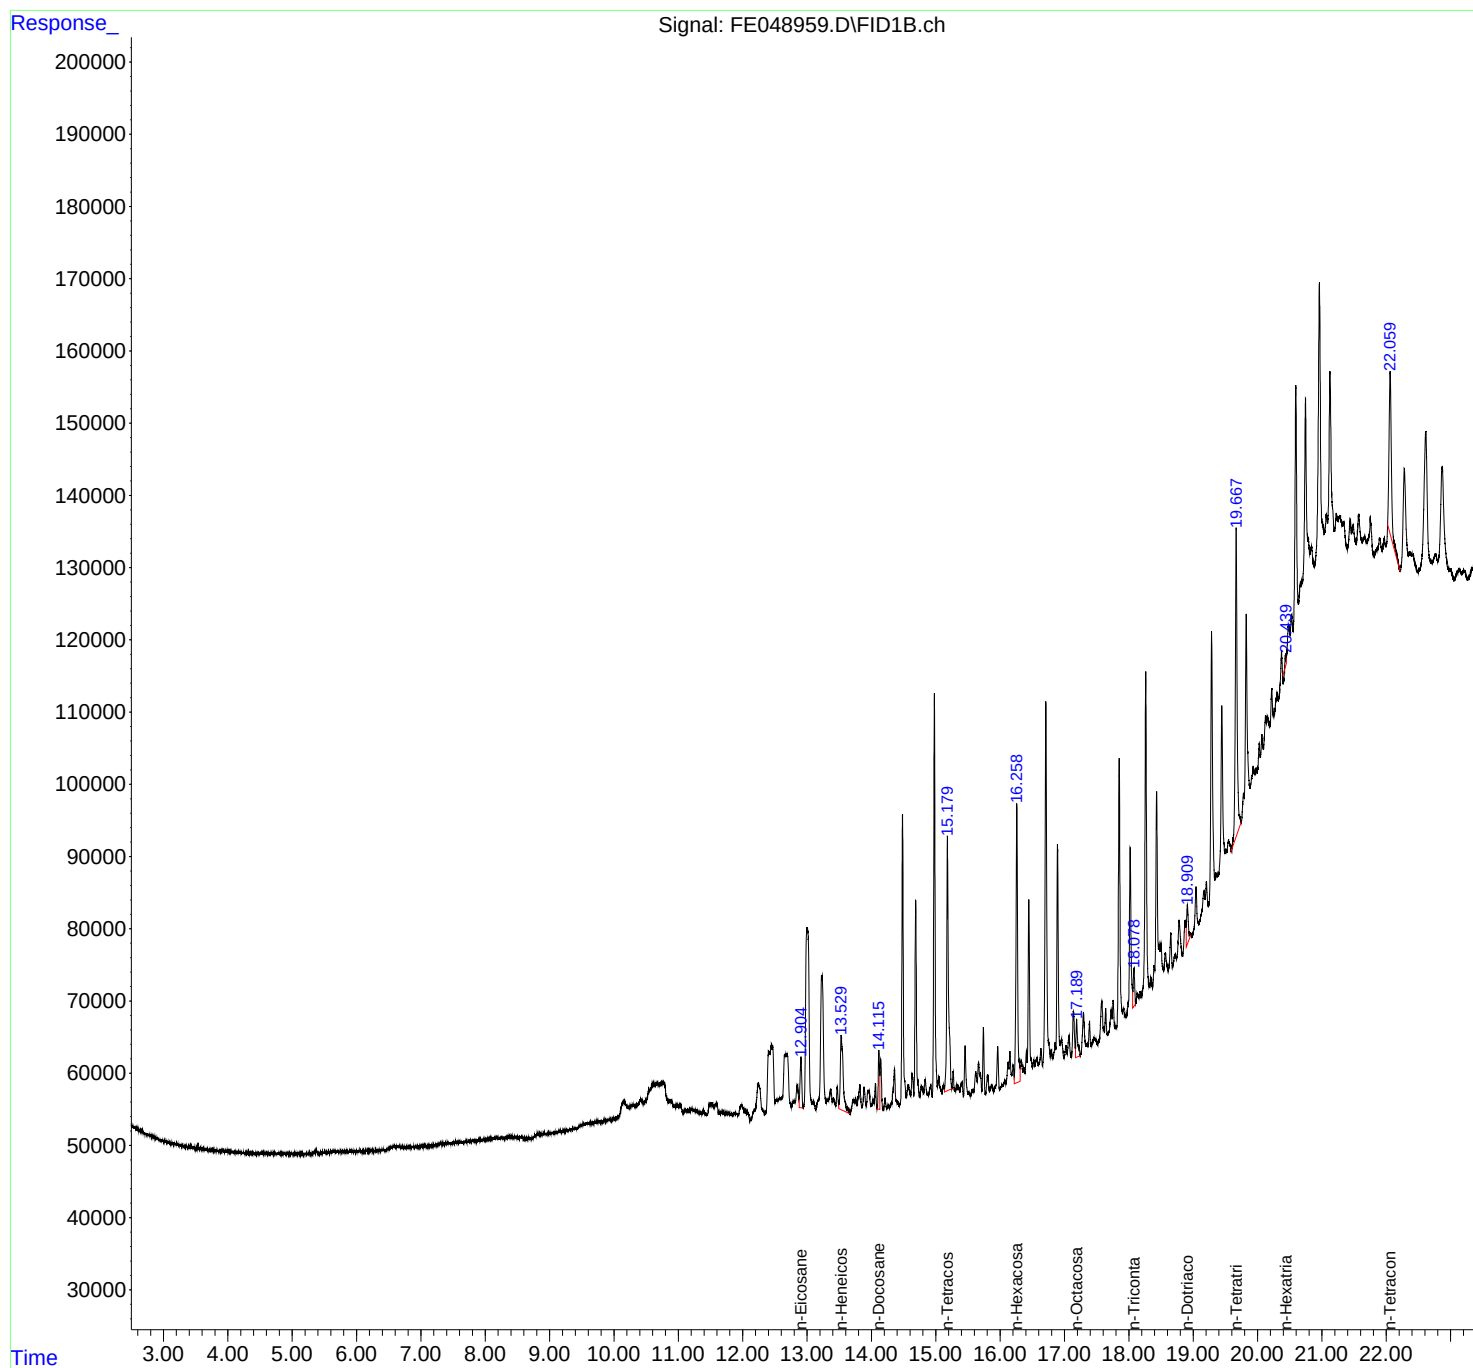


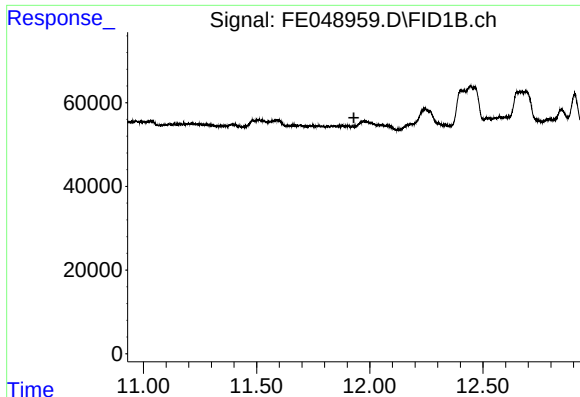

#9 ortho-Terphenyl (SURR)


R.T.: 0.000 min
Exp R.T.: 11.930 min
Response: 0
Conc: N.D.

Instrument :
FID_E
ClientSampleId :

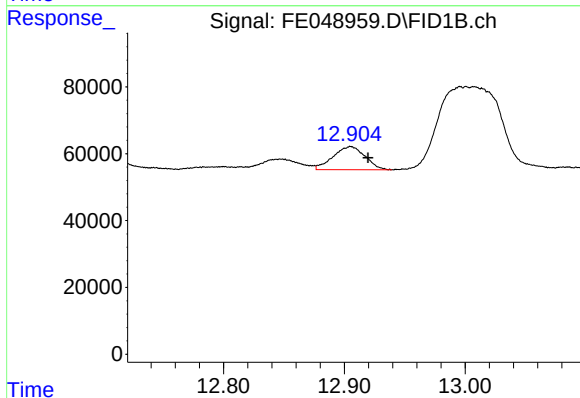


#10 n-Eicosane (C20)

R.T.: 12.905 min
Delta R.T.: -0.014 min
Response: 127666
Conc: 0.82 ug/ml

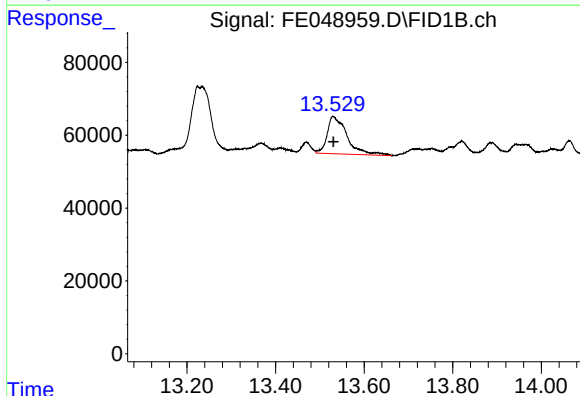


#11 n-Heneicosane (C21)

R.T.: 13.530 min
Delta R.T.: 0.000 min
Response: 321028
Conc: 2.11 ug/ml

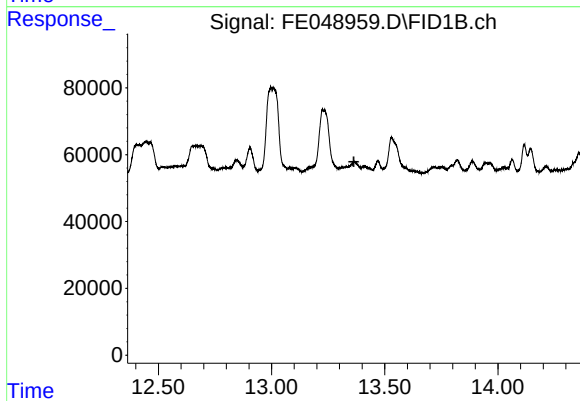

#12 1-chlorooctadecane (SURR)


R.T.: 0.000 min
Exp R.T.: 13.364 min
Response: 0
Conc: N.D.

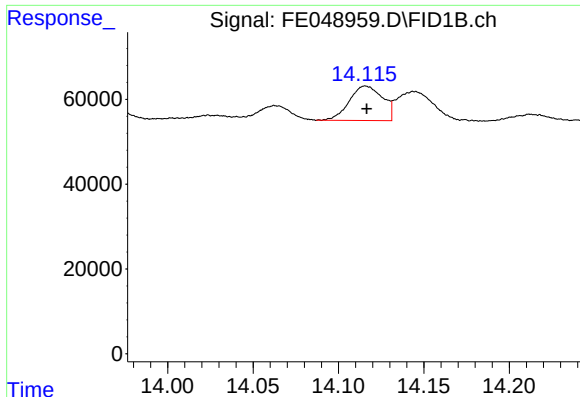

#13 n-Docosane (C22)


R.T.: 14.116 min
Delta R.T.: 0.000 min
Response: 110464
Conc: 0.73 ug/ml

Instrument :
FID_E
ClientSampleId :

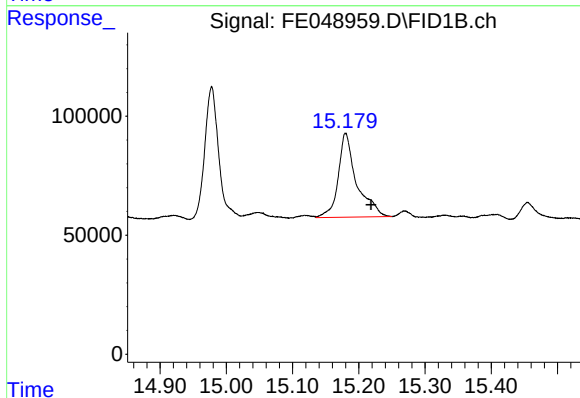


#14 n-Tetracosane (C24)

R.T.: 15.180 min
Delta R.T.: -0.038 min
Response: 682724
Conc: 4.54 ug/ml

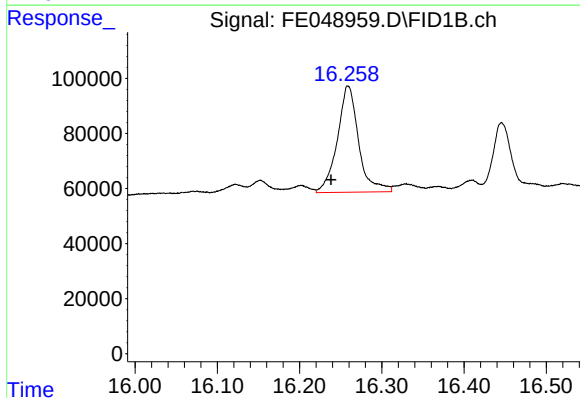


#15 n-Hexacosane (C26)

R.T.: 16.259 min
Delta R.T.: 0.021 min
Response: 695135
Conc: 4.71 ug/ml

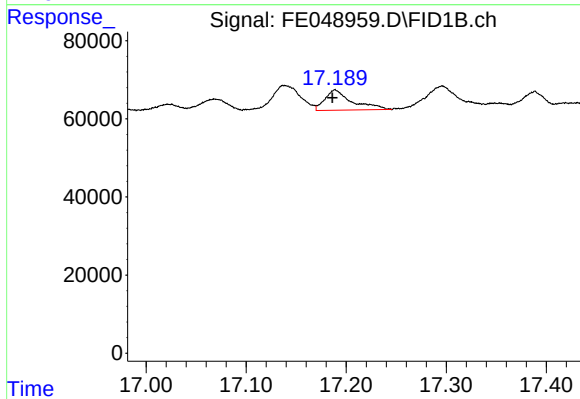

#16 n-Octacosane (C28)


R.T.: 17.189 min
Delta R.T.: 0.003 min
Response: 97134
Conc: 0.67 ug/ml

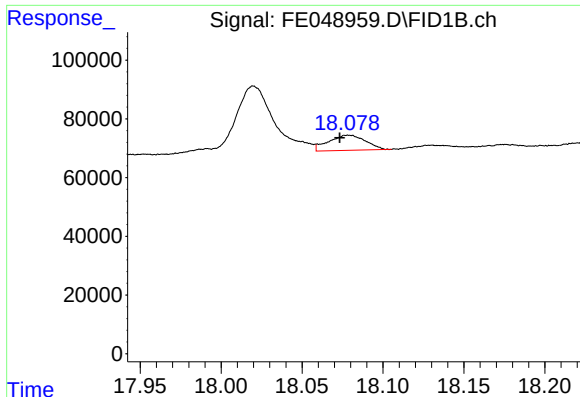

#17 n-Tricontane (C30)


R.T.: 18.079 min
Delta R.T.: 0.005 min
Response: 82441
Conc: 0.56 ug/ml

Instrument :
FID_E
ClientSampleId :

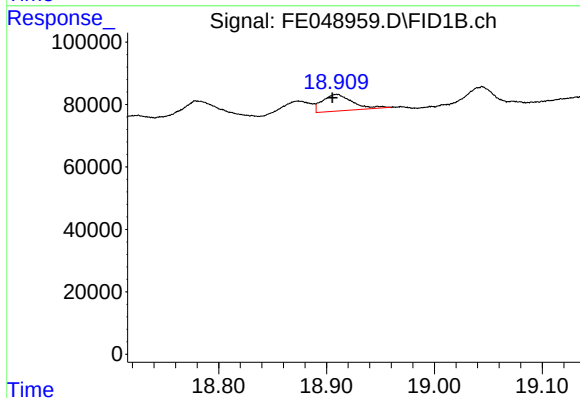


#18 n-Dotriacontane (C32)

R.T.: 18.910 min
Delta R.T.: 0.004 min
Response: 102367
Conc: 0.72 ug/ml

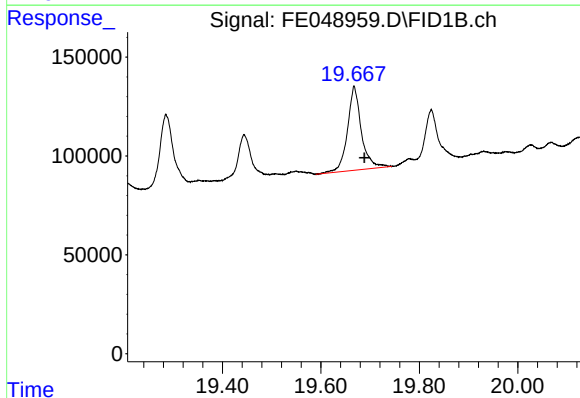


#19 n-Tetratriacontane (C34)

R.T.: 19.668 min
Delta R.T.: -0.020 min
Response: 831205
Conc: 6.01 ug/ml

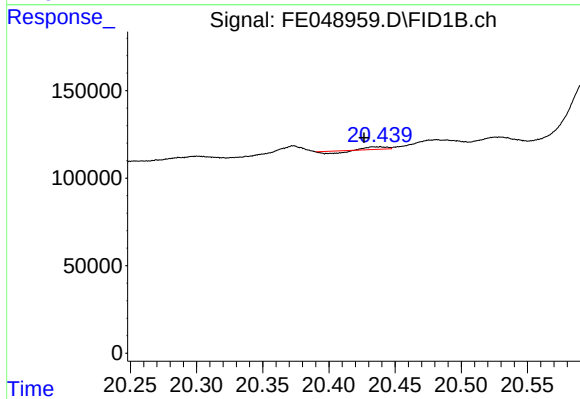

#20 n-Hexatriacontane (C36)

R.T.: 20.438 min
Delta R.T.: 0.011 min
Response: 2172
Conc: 0.02 ug/ml

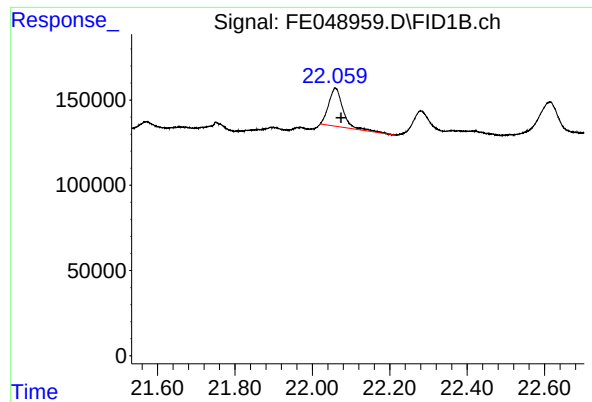

#22 n-Tetracontane (C40)

R.T.: 22.059 min
Delta R.T.: -0.015 min
Response: 577230
Conc: 4.71 ug/ml

Instrument :

FID_E

ClientSampleId :