

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070224AL\  
Data File : FE048962.D  
Signal(s) : FID1B.ch  
Acq On : 02 Jul 2024 09:03  
Operator : YP\AJ  
Sample : P3135-03DL 2X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
OK-628-01DL

Integration File: autoint1.e  
Quant Time: Jul 03 01:24:50 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062124.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 20 17:53:58 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response   | Conc Units   |
|--------------------------------|--------|------------|--------------|
| -----                          |        |            |              |
| System Monitoring Compounds    |        |            |              |
| 9) S ortho-Terphenyl (SURR)    | 11.932 | 2308258    | 13.805 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 27.61%       |
| 12) S 1-chlorooctadecane (S... | 13.367 | 1864386    | 14.499 ug/ml |
| Spiked Amount 50.000           |        | Recovery = | 29.00%       |

Target Compounds

-----

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070224AL\  
Data File : FE048962.D  
Signal(s) : FID1B.ch  
Acq On : 02 Jul 2024 09:03  
Operator : YP\AJ  
Sample : P3135-03DL 2X  
Misc :  
ALS Vial : 7 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
OK-628-01DL

Integration File: autoint1.e  
Quant Time: Jul 03 01:24:50 2024  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062124.M  
Quant Title : GC Extractables  
QLast Update : Thu Jun 20 17:53:58 2024  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

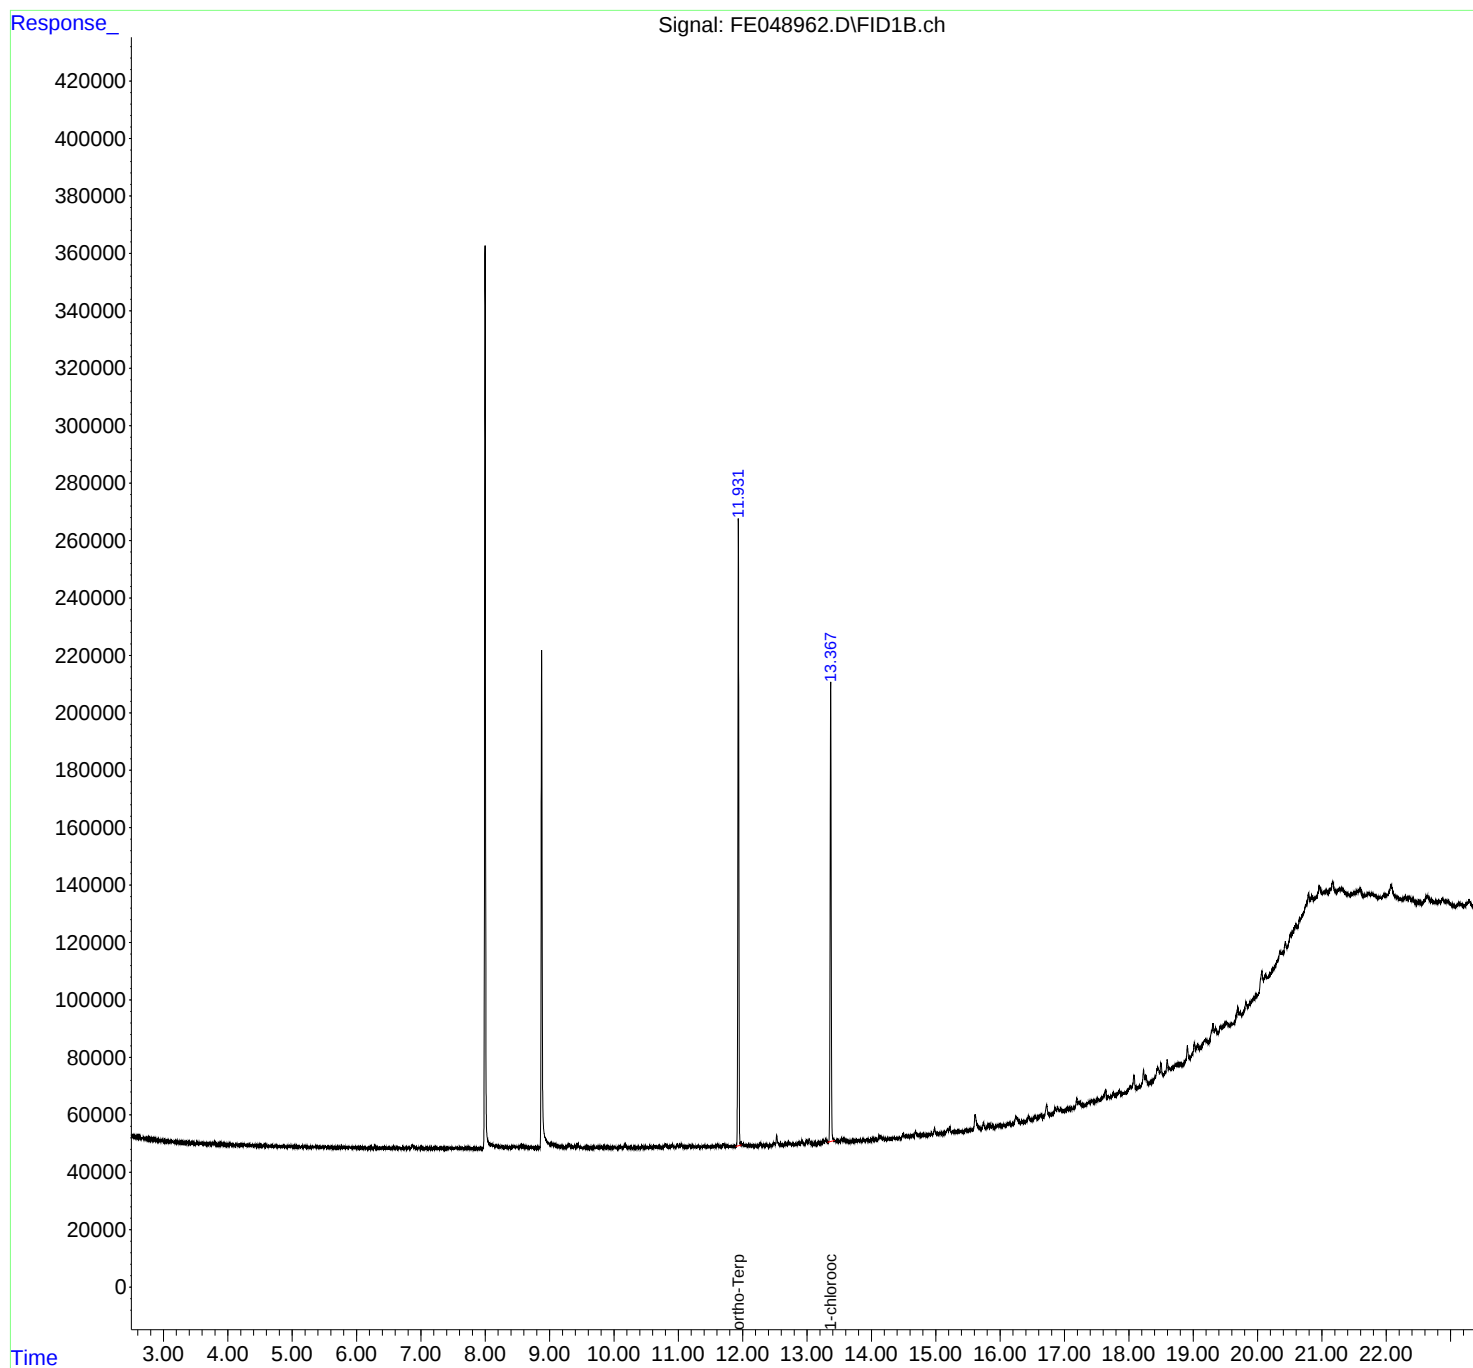


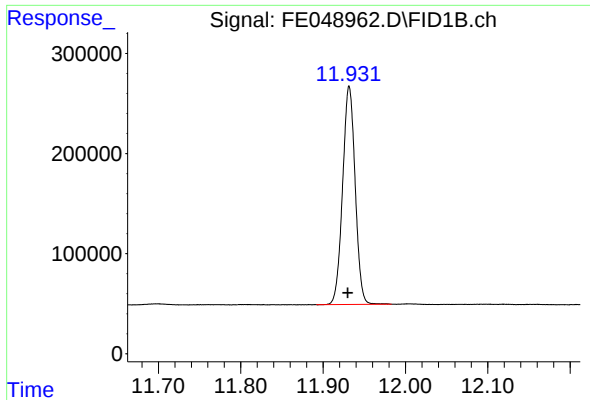

#9 ortho-Terphenyl (SURR)

R.T.: 11.932 min  
Delta R.T.: 0.002 min  
Response: 2308258  
Conc: 13.80 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
OK-628-01DL

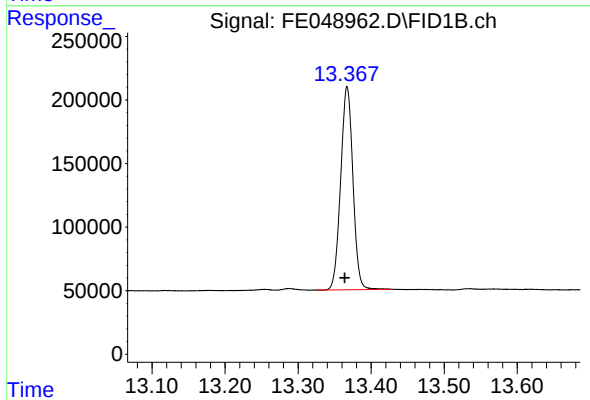

#12 1-chlorooctadecane (SURR)

R.T.: 13.367 min  
Delta R.T.: 0.003 min  
Response: 1864386  
Conc: 14.50 ug/ml