

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070323AL\  
 Data File : FE043043.D  
 Signal(s) : FID1B.ch  
 Acq On : 03 Jul 2023 10:11  
 Operator : YP\AJ  
 Sample : 03475-01  
 Misc :  
 ALS Vial : 13 Sample Multiplier: 1

Instrument :  
 FID\_E  
 ClientSampleId :  
 ALDENE-COMP-1

Integration File: autoint1.e  
 Quant Time: Jul 04 07:13:26 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062123.M  
 Quant Title : GC Extractables  
 QLast Update : Wed Jun 21 11:03:59 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 ul  
 Signal Phase : Rxi-1ms  
 Signal Info : 20M x 0.18mm x 0.18um

| Compound                       | R.T.   | Response | Conc Units   |
|--------------------------------|--------|----------|--------------|
| -----                          |        |          |              |
| System Monitoring Compounds    |        |          |              |
| 9) S ortho-Terphenyl (SURR)    | 11.907 | 4284022  | 23.320 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 46.64%     |
| 12) S 1-chlorooctadecane (S... | 13.345 | 3352016  | 24.631 ug/ml |
| Spiked Amount                  | 50.000 | Recovery | = 49.26%     |

Target Compounds

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_E\Data\FE070323AL\  
Data File : FE043043.D  
Signal(s) : FID1B.ch  
Acq On : 03 Jul 2023 10:11  
Operator : YP\AJ  
Sample : 03475-01  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Instrument :  
FID\_E  
ClientSampleId :  
ALDENE-COMP-1

Integration File: autoint1.e  
Quant Time: Jul 04 07:13:26 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_E\methods\Aliphatic EPH 062123.M  
Quant Title : GC Extractables  
QLast Update : Wed Jun 21 11:03:59 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 ul  
Signal Phase : Rxi-1ms  
Signal Info : 20M x 0.18mm x 0.18um

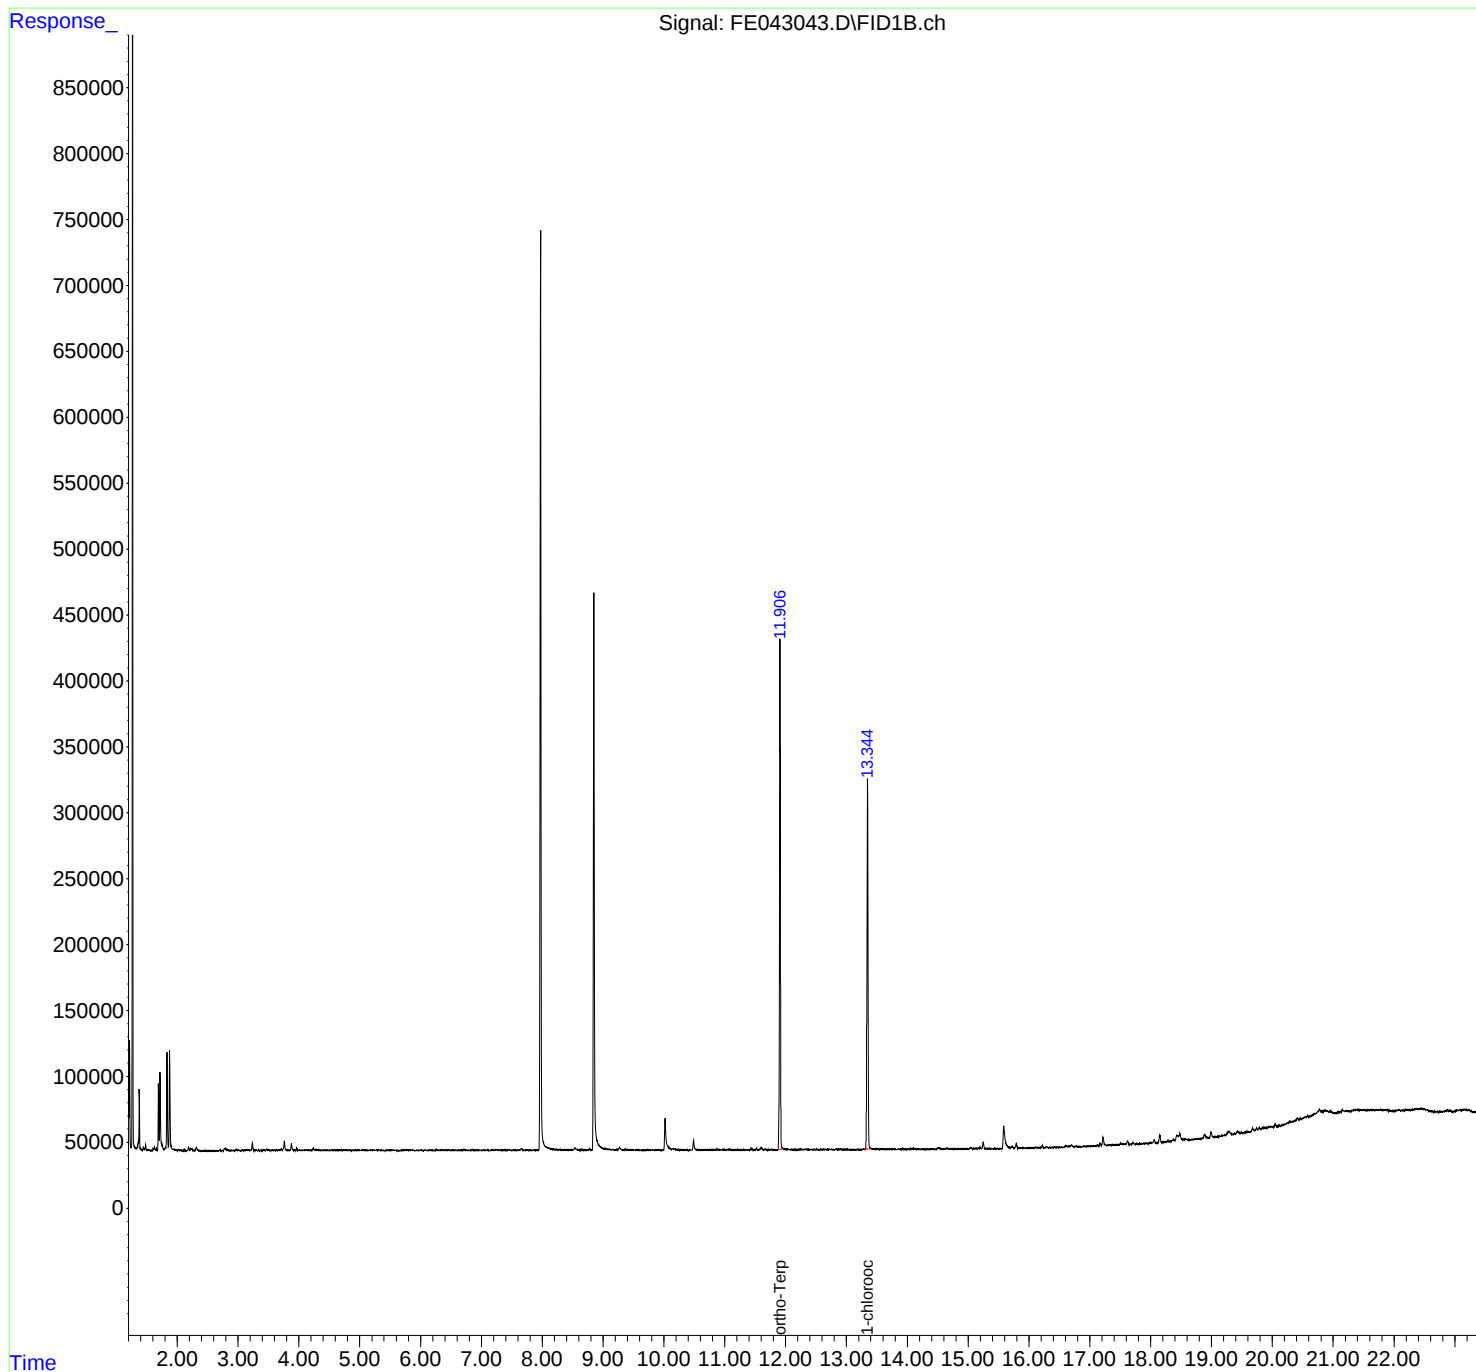


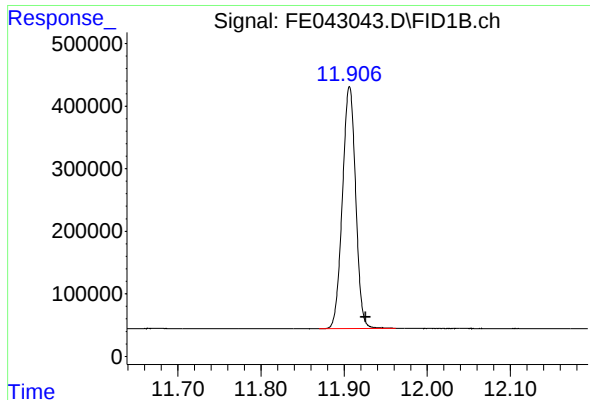

#9 ortho-Terphenyl (SURR)

R.T.: 11.907 min  
Delta R.T.: -0.019 min  
Response: 4284022  
Conc: 23.32 ug/ml

Instrument :  
FID\_E  
ClientSampleId :  
ALDENE-COMP-1

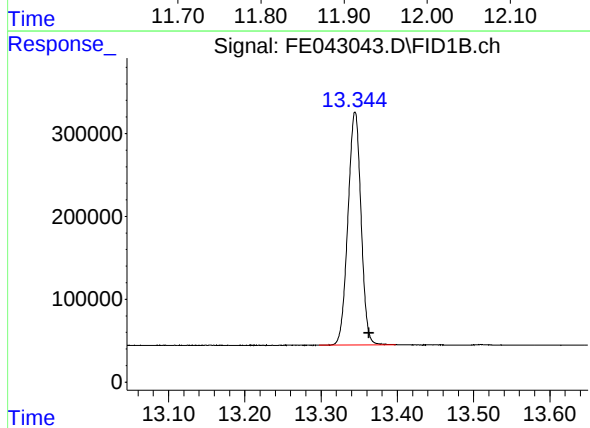

#12 1-chlorooctadecane (SURR)

R.T.: 13.345 min  
Delta R.T.: -0.018 min  
Response: 3352016  
Conc: 24.63 ug/ml