

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070523AL\
 Data File : FE043078.D
 Signal(s) : FID1B.ch
 Acq On : 05 Jul 2023 12:04
 Operator : YP\AJ
 Sample : 03497-01DL 5X
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_E
 ClientSampleId :
 OK-2-063023DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 07/06/2023
 Supervised By :Ankita Jodhani 07/06/2023

Integration File: autoint1.e
 Quant Time: Jul 06 02:08:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
 Quant Title : GC Extractables
 QLast Update : Wed Jun 21 11:03:59 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 ul
 Signal Phase : Rxi-1ms
 Signal Info : 20M x 0.18mm x 0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S ortho-Terphenyl (SURR)	11.902	1060534	5.773 ug/mlm
Spiked Amount 50.000		Recovery =	11.55%
12) S 1-chlorooctadecane (S...	13.342	1032973	7.590 ug/ml
Spiked Amount 50.000		Recovery =	15.18%

Target Compounds

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070523AL\
Data File : FE043078.D
Signal(s) : FID1B.ch
Acq On : 05 Jul 2023 12:04
Operator : YP\AJ
Sample : 03497-01DL 5X
Misc :
ALS Vial : 16 Sample Multiplier: 1


Instrument :
FID_E
ClientSampleId :
OK-2-063023DL


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/06/2023
Supervised By :Ankita Jodhani 07/06/2023

Integration File: autoint1.e
Quant Time: Jul 06 02:08:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\Aliphatic EPH 062123.M
Quant Title : GC Extractables
QLast Update : Wed Jun 21 11:03:59 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 ul
Signal Phase : Rxi-1ms
Signal Info : 20M x 0.18mm x 0.18um

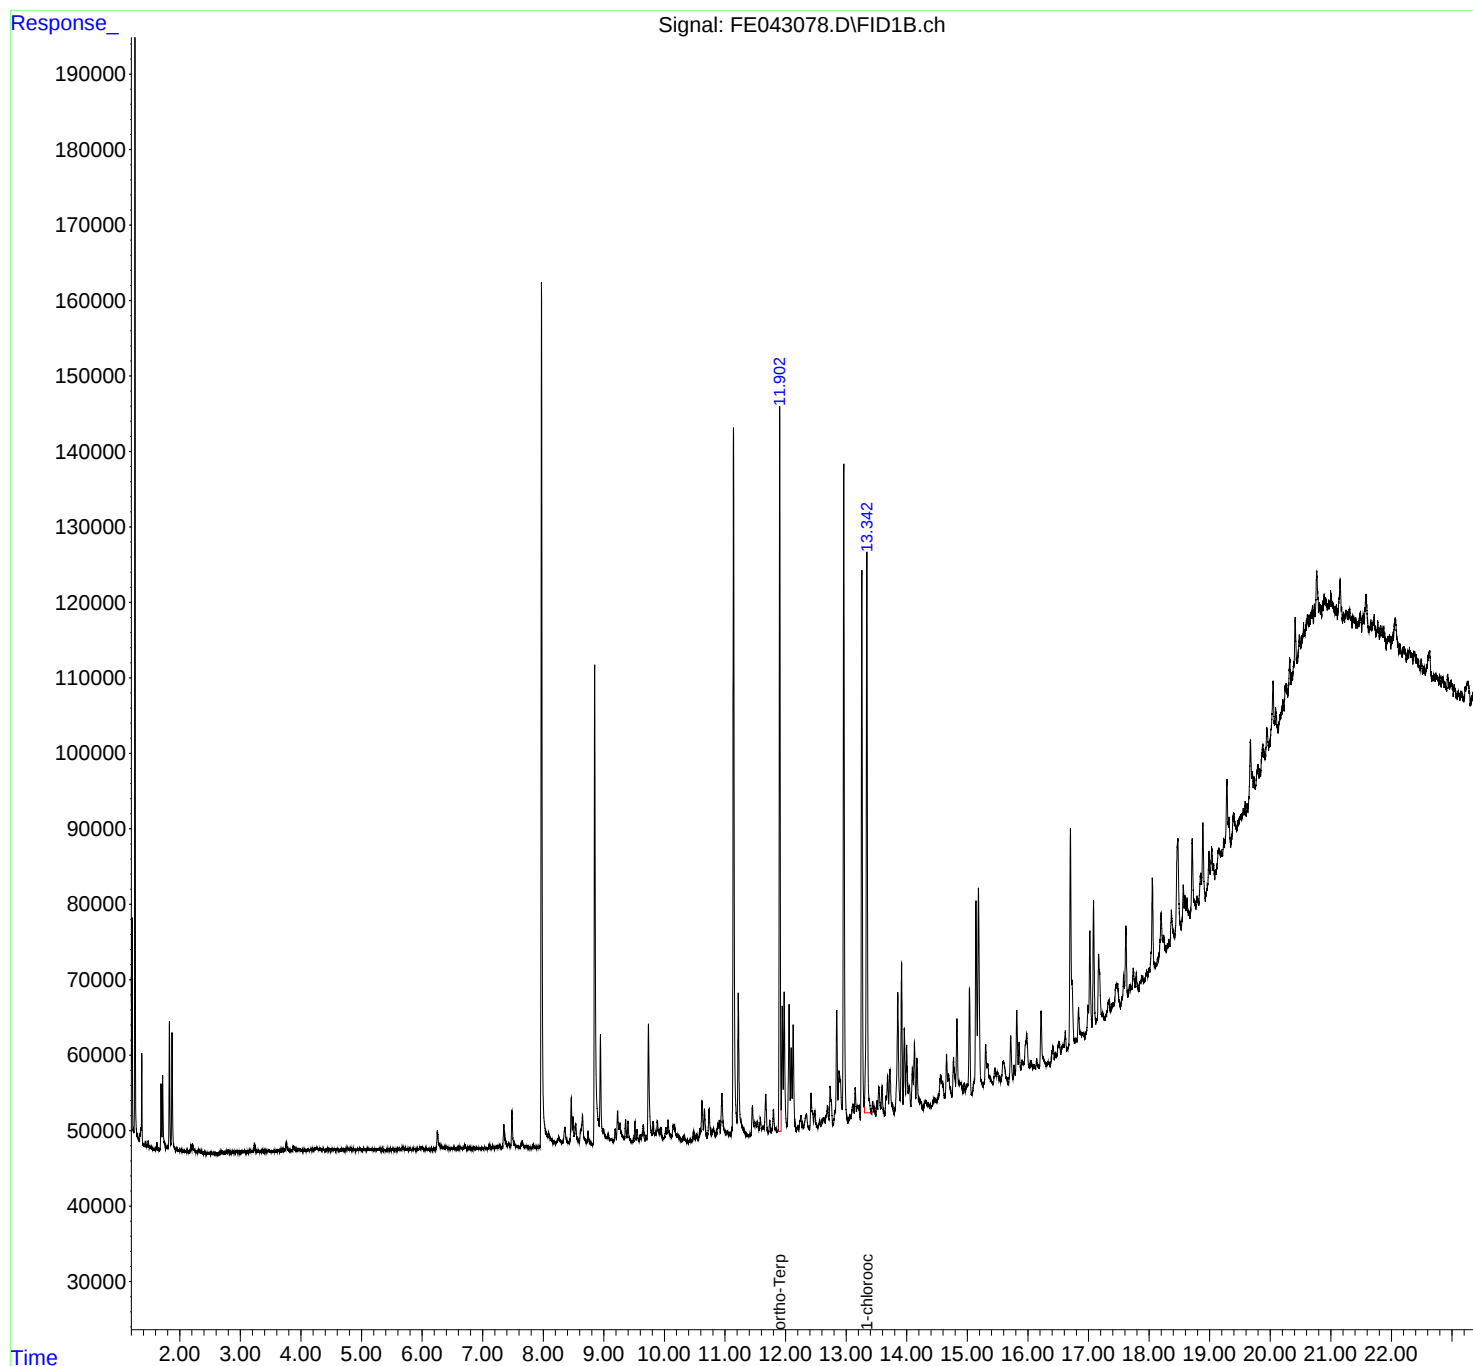

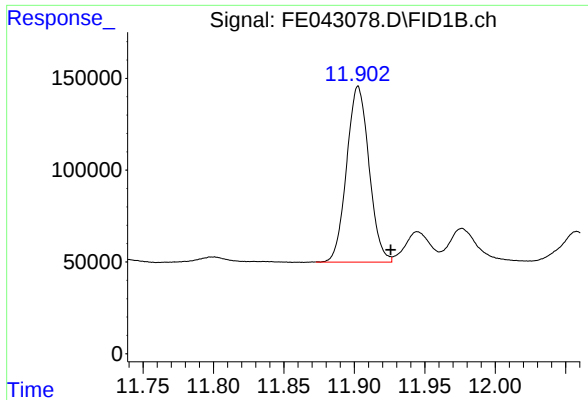


#9 ortho-Terphenyl (SURR)

R.T.: 11.902 min
Delta R.T.: -0.023 min
Response: 1060534
Conc: 5.77 ug/ml

Instrument :
FID_E
ClientSampleId :
OK-2-063023DL

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/06/2023
Supervised By :Ankita Jodhani 07/06/2023

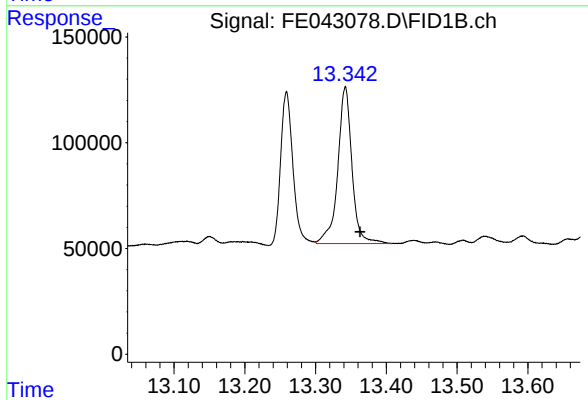

#12 1-chlorooctadecane (SURR)

R.T.: 13.342 min
Delta R.T.: -0.021 min
Response: 1032973
Conc: 7.59 ug/ml