

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070820\
 Data File : FE032313.D
 Signal(s) : FID1B.CH
 Acq On : 08 Jul 2020 12:58
 Operator : DD\AJ
 Sample : L3216-07
 Misc : LOD-WATER-1 PPM
 ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Jul 09 01:02:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
 Quant Title :
 QLast Update : Wed Jul 08 12:04:06 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.742	5845726	19.216 ug/ml
Target Compounds			
2) N-DECANE	4.487	432259	1.243 ug/ml
3) N-DODECANE	6.499	437789	1.254 ug/ml
4) N-TETRADECANE	8.292	435209	1.252 ug/ml
5) N-HEXADECANE	9.893	434727	1.247 ug/ml
6) N-OCTADECANE	11.333	443942	1.255 ug/ml
7) N-EICOSANE	12.642	440379	1.252 ug/ml
8) N-DOCOSANE	13.841	441641	1.257 ug/ml
10) N-TETRACOSANE	14.943	447064	1.263 ug/ml
11) N-HEXACOSANE	15.961	451719	1.287 ug/ml
12) N-OCTACOSANE	16.910	480697	1.367 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_E\Data\FE070820\
Data File : FE032313.D
Signal(s) : FID1B.CH
Acq On : 08 Jul 2020 12:58
Operator : DD\AJ
Sample : L3216-07
Misc : LOD-WATER-1 PPM
ALS Vial : 8 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Jul 09 01:02:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_E\methods\FE070720.M
Quant Title :
QLast Update : Wed Jul 08 12:04:06 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

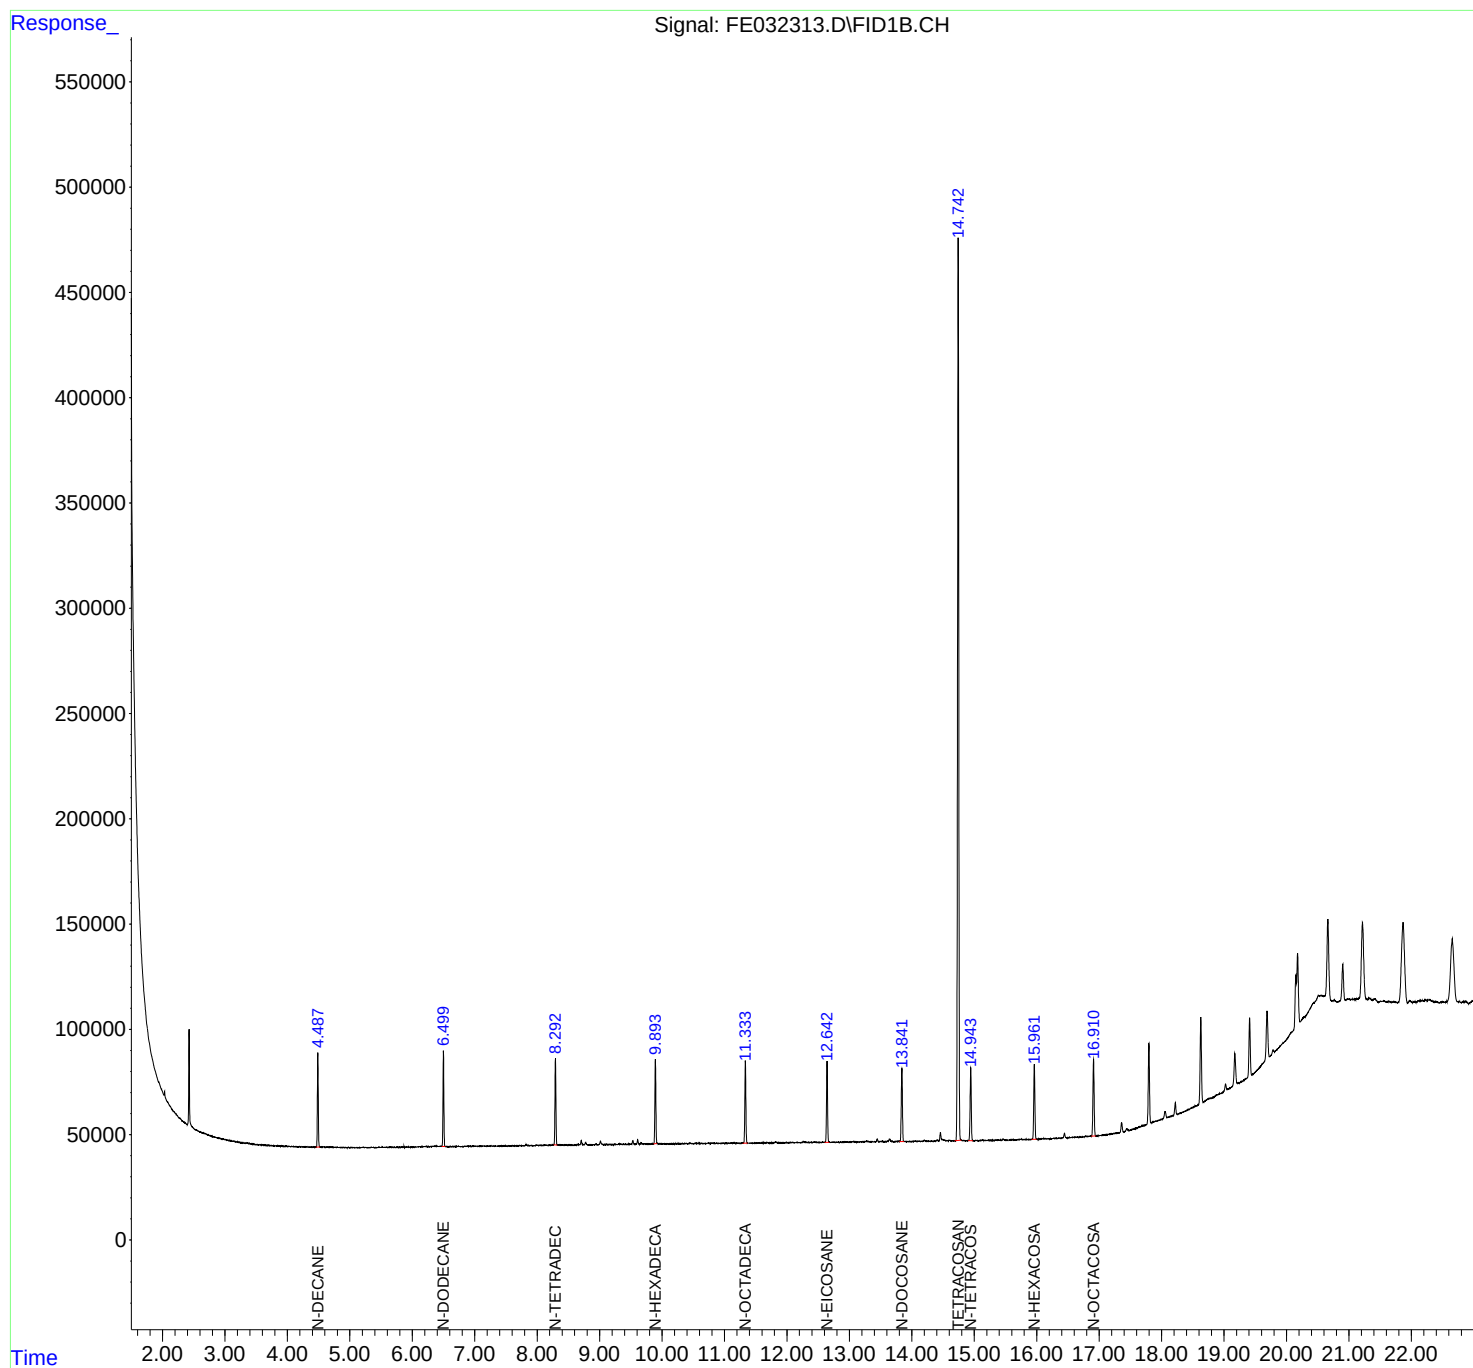

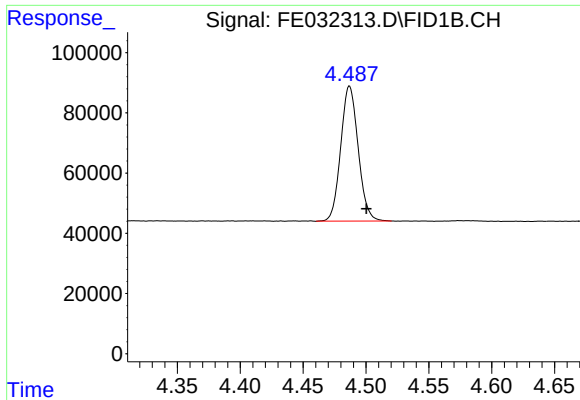


#2 N-DECANE

R.T.: 4.487 min
Delta R.T.: -0.013 min
Response: 432259
Conc: 1.24 ug/ml

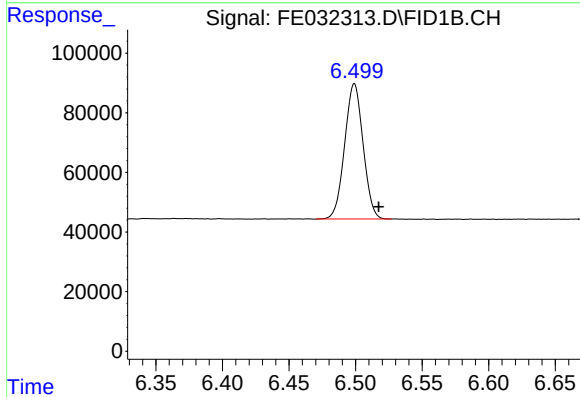


#3 N-DODECANE

R.T.: 6.499 min
Delta R.T.: -0.018 min
Response: 437789
Conc: 1.25 ug/ml

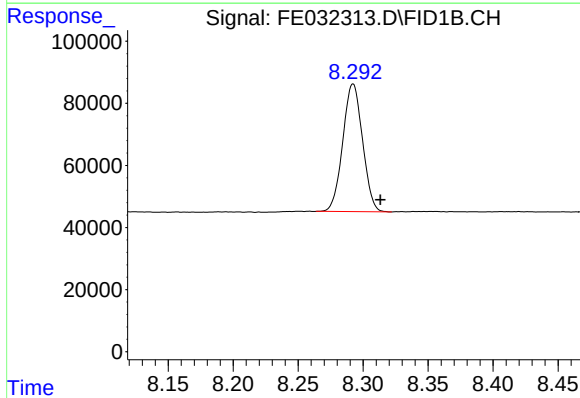


#4 N-TETRADECANE

R.T.: 8.292 min
Delta R.T.: -0.021 min
Response: 435209
Conc: 1.25 ug/ml

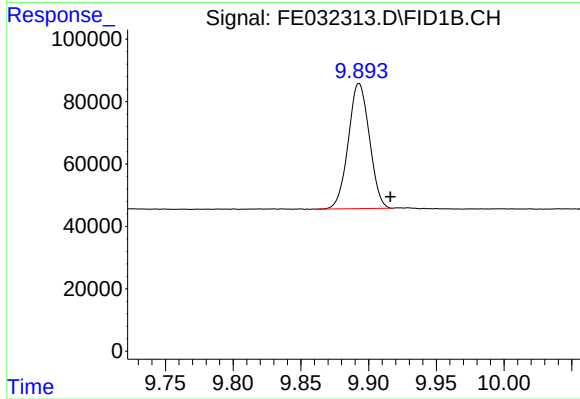


#5 N-HEXADECANE

R.T.: 9.893 min
Delta R.T.: -0.023 min
Response: 434727
Conc: 1.25 ug/ml

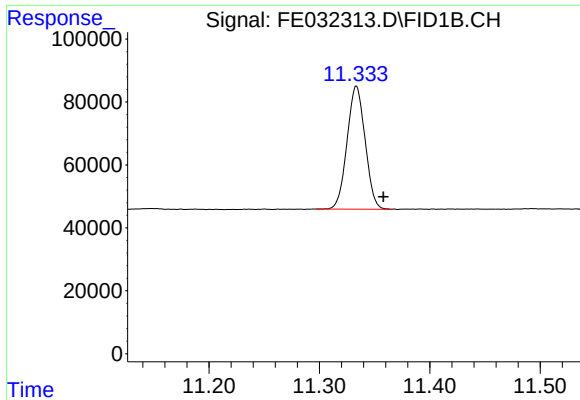


#6 N-OCTADECANE

R.T.: 11.333 min
Delta R.T.: -0.024 min
Response: 443942
Conc: 1.26 ug/ml

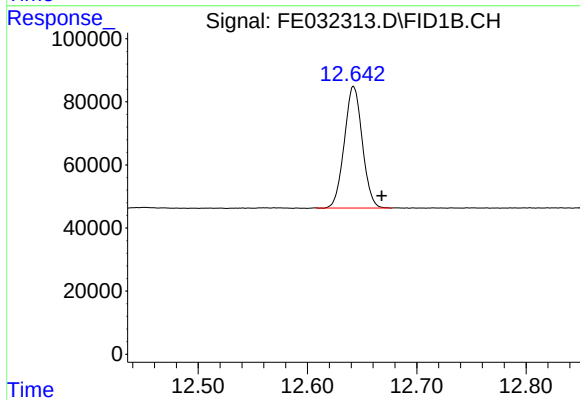


#7 N-EICOSANE

R.T.: 12.642 min
Delta R.T.: -0.026 min
Response: 440379
Conc: 1.25 ug/ml

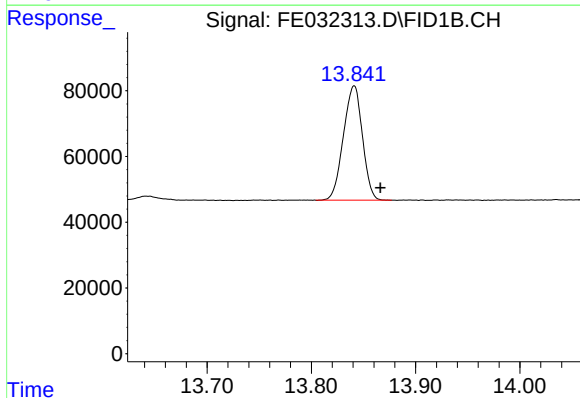


#8 N-DOCOSANE

R.T.: 13.841 min
Delta R.T.: -0.025 min
Response: 441641
Conc: 1.26 ug/ml

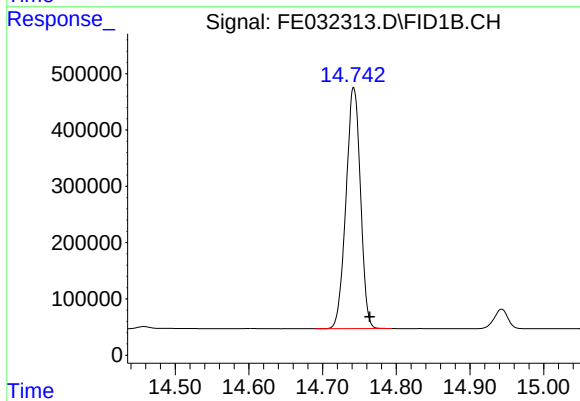


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.742 min
Delta R.T.: -0.022 min
Response: 5845726
Conc: 19.22 ug/ml

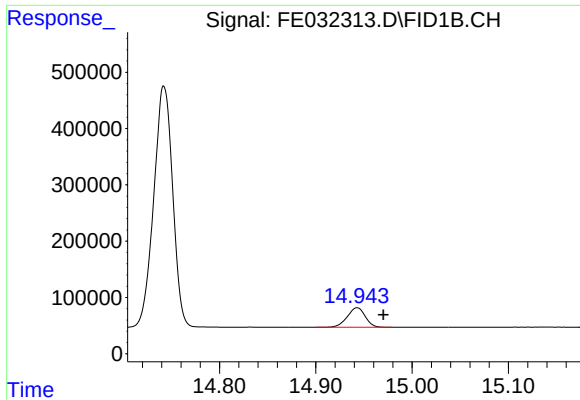


#10 N-TETRACOSANE

R.T.: 14.943 min
Delta R.T.: -0.027 min
Response: 447064
Conc: 1.26 ug/ml

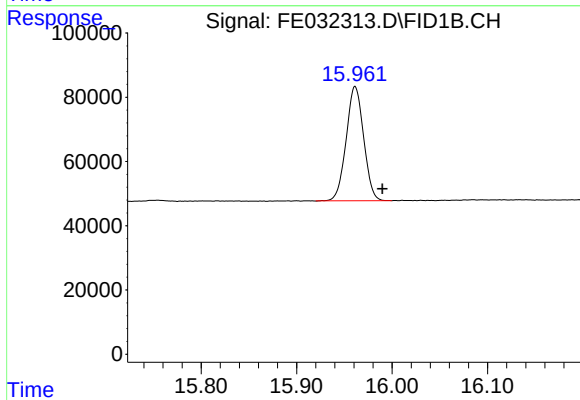

#11 N-HEXACOSANE

R.T.: 15.961 min
Delta R.T.: -0.028 min
Response: 451719
Conc: 1.29 ug/ml

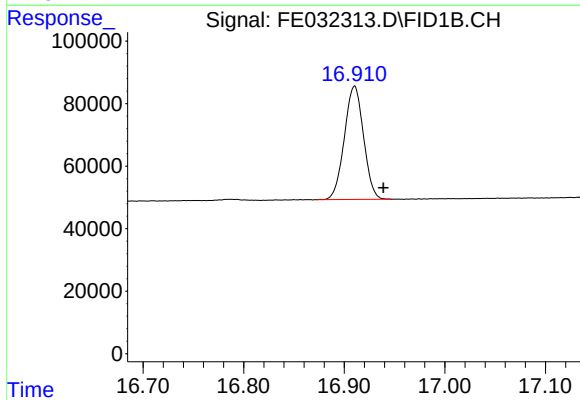

#12 N-OCTACOSANE

R.T.: 16.910 min
Delta R.T.: -0.029 min
Response: 480697
Conc: 1.37 ug/ml